

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016936.D
 Acq On : 15 Jun 2020 15:05
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	177681	179063	12.55%	1.640%
2	1.566	143	148	161	rVB	113450	130584	9.15%	1.196%
3	2.119	310	320	334	rBV	275685	420528	29.48%	3.851%
4	2.254	360	362	365	rBV3	2125	990	0.07%	0.009%
5	2.421	412	414	416	rBV3	1403	534	0.04%	0.005%
6	2.489	431	435	437	rBV4	1719	1161	0.08%	0.011%
7	2.515	437	443	445	rBV5	4503	4617	0.32%	0.042%
8	2.608	469	472	473	rBV3	1372	695	0.05%	0.006%
9	2.897	561	562	563	rBV	1280	481	0.03%	0.004%
10	3.026	598	602	603	rBV4	1385	983	0.07%	0.009%
11	3.036	603	605	608	rVB3	1599	768	0.05%	0.007%
12	3.055	608	611	613	rBV2	1549	849	0.06%	0.008%
13	3.177	647	649	655	rBV7	947	768	0.05%	0.007%
14	3.254	671	673	676	rBV3	1862	1354	0.09%	0.012%
15	3.325	693	695	698	rVB3	1282	699	0.05%	0.006%
16	3.341	698	700	701	rBV2	1063	542	0.04%	0.005%
17	3.373	708	710	713	rBV4	922	610	0.04%	0.006%
18	3.476	739	742	746	rVV4	1073	928	0.07%	0.008%
19	3.528	755	758	765	rBV8	1107	1409	0.10%	0.013%
20	3.556	765	767	769	rVB3	1600	569	0.04%	0.005%
21	3.708	809	814	816	rBV7	1654	1454	0.10%	0.013%
22	3.827	849	851	856	rVB5	1580	909	0.06%	0.008%
23	3.855	856	860	862	rBV4	1770	1374	0.10%	0.013%
24	3.897	862	873	904	rBV	103025	287982	20.19%	2.638%
25	4.373	1007	1021	1048	rVB	236283	572656	40.14%	5.245%
26	4.691	1117	1120	1122	rBV4	1574	1144	0.08%	0.010%
27	4.743	1133	1136	1139	rBV4	1539	942	0.07%	0.009%
28	4.781	1146	1148	1150	rBV3	1419	916	0.06%	0.008%
29	4.833	1162	1164	1166	rBV3	1422	859	0.06%	0.008%
30	4.958	1200	1203	1205	rBV3	1156	648	0.05%	0.006%
31	5.071	1221	1238	1259	rBV2	554756	1426593	100.00%	13.066%
32	5.254	1290	1295	1300	rBV7	2447	2589	0.18%	0.024%
33	5.386	1333	1336	1340	rVB6	1723	1214	0.09%	0.011%
34	5.405	1340	1342	1345	rBV3	1770	1218	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016936.D
 Acq On : 15 Jun 2020 15:05
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1400	1415	1436	rBV	456827	912030	63.93%	8.353%
36	5.926	1495	1504	1519	rVB2	31436	60329	4.23%	0.553%
37	6.093	1541	1556	1574	rBV	322746	649218	45.51%	5.946%
38	6.347	1633	1635	1639	rVB4	1646	881	0.06%	0.008%
39	6.367	1639	1641	1643	rBV3	1820	868	0.06%	0.008%
40	6.392	1646	1649	1652	rBV4	1918	1179	0.08%	0.011%
41	6.534	1691	1693	1697	rBV6	1640	955	0.07%	0.009%
42	6.707	1743	1747	1749	rBV4	1562	959	0.07%	0.009%
43	6.756	1759	1762	1765	rBV4	1584	1104	0.08%	0.010%
44	6.794	1772	1774	1777	rBV3	1212	937	0.07%	0.009%
45	6.855	1791	1793	1796	rVB3	1590	783	0.05%	0.007%
46	6.871	1796	1798	1803	rVB4	1086	680	0.05%	0.006%
47	6.894	1803	1805	1808	rVB2	1774	1069	0.07%	0.010%
48	6.920	1808	1813	1818	rBV7	2701	3338	0.23%	0.031%
49	7.006	1829	1840	1855	rBV	193720	342671	24.02%	3.138%
50	7.164	1887	1889	1895	rVB6	2378	1514	0.11%	0.014%
51	7.338	1931	1943	1960	rBV	675083	1166366	81.76%	10.682%
52	7.569	2011	2015	2018	rBV5	1472	1206	0.08%	0.011%
53	7.640	2028	2037	2051	rBV	135302	230947	16.19%	2.115%
54	7.990	2144	2146	2147	rBV2	1399	480	0.03%	0.004%
55	8.032	2155	2159	2160	rBV3	1225	923	0.06%	0.008%
56	8.109	2173	2183	2217	rBV2	300174	609923	42.75%	5.586%
57	8.299	2240	2242	2244	rBV3	1582	1046	0.07%	0.010%
58	8.778	2389	2391	2395	rBV4	1288	895	0.06%	0.008%
59	8.871	2409	2420	2438	rBV	681194	1097731	76.95%	10.054%
60	9.161	2504	2510	2517	rBV6	6672	10860	0.76%	0.099%
61	9.289	2548	2550	2553	rVB3	1515	785	0.06%	0.007%
62	9.421	2589	2591	2592	rBV2	1497	611	0.04%	0.006%
63	9.688	2671	2674	2678	rBV5	1758	1602	0.11%	0.015%
64	9.830	2715	2718	2721	rBV4	961	771	0.05%	0.007%
65	9.881	2732	2734	2737	rBV4	1771	1075	0.08%	0.010%
66	10.003	2768	2772	2777	rVB6	2151	2301	0.16%	0.021%
67	10.039	2777	2783	2787	rBV8	1489	2130	0.15%	0.020%
68	10.132	2809	2812	2816	rBV5	1615	1672	0.12%	0.015%
69	10.238	2830	2845	2861	rBV	381343	606031	42.48%	5.550%
70	10.386	2889	2891	2894	rBV3	1533	1080	0.08%	0.010%
71	10.611	2959	2961	2963	rBV3	1754	877	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016936.D
 Acq On : 15 Jun 2020 15:05
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.862	3037	3039	3042	rBV4	2226	962	0.07%	0.009%
73	10.878	3042	3044	3047	rVB4	1866	1095	0.08%	0.010%
74	10.894	3047	3049	3054	rBV4	1073	632	0.04%	0.006%
75	10.981	3074	3076	3080	rVB4	2203	1362	0.10%	0.012%
76	11.006	3080	3084	3086	rBV4	1349	1148	0.08%	0.011%
77	11.022	3086	3089	3092	rBV4	1075	838	0.06%	0.008%
78	11.090	3107	3110	3117	rVB7	1560	1991	0.14%	0.018%
79	11.270	3155	3166	3185	rBV	680196	1042417	73.07%	9.547%
80	11.646	3272	3283	3298	rBV	693803	1081093	75.78%	9.901%
81	12.000	3390	3393	3395	rBV3	1853	1079	0.08%	0.010%
82	12.077	3415	3417	3421	rVB4	1563	935	0.07%	0.009%
83	12.106	3421	3426	3427	rBV4	1701	1557	0.11%	0.014%
84	12.373	3506	3509	3513	rBV5	1994	1543	0.11%	0.014%
85	12.444	3530	3531	3534	rBV3	1019	535	0.04%	0.005%
86	12.501	3546	3549	3550	rBV2	1386	742	0.05%	0.007%
87	12.556	3561	3566	3571	rBV8	1918	1618	0.11%	0.015%
88	12.862	3657	3661	3664	rBV4	1320	708	0.05%	0.006%
89	12.878	3664	3666	3668	rBV2	1199	609	0.04%	0.006%
90	12.900	3670	3673	3676	rBV4	1328	919	0.06%	0.008%
91	12.952	3687	3689	3691	rVB3	1656	605	0.04%	0.006%
92	13.038	3714	3716	3719	rVB3	2025	776	0.05%	0.007%
93	13.225	3772	3774	3775	rBV2	1456	477	0.03%	0.004%
94	13.537	3869	3871	3873	rBV3	2071	762	0.05%	0.007%
95	13.701	3921	3922	3924	rBV2	1226	558	0.04%	0.005%
96	13.823	3956	3960	3964	rBV6	1991	2079	0.15%	0.019%
97	14.193	4072	4075	4080	rVB5	2463	1864	0.13%	0.017%
98	14.225	4080	4085	4086	rBV3	1937	1435	0.10%	0.013%
99	14.296	4106	4107	4111	rBV4	1421	904	0.06%	0.008%
100	14.691	4227	4230	4232	rBV4	1664	920	0.06%	0.008%


Sum of corrected areas: 10918620

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
Data File : VV016936.D
Acq On : 15 Jun 2020 15:05
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

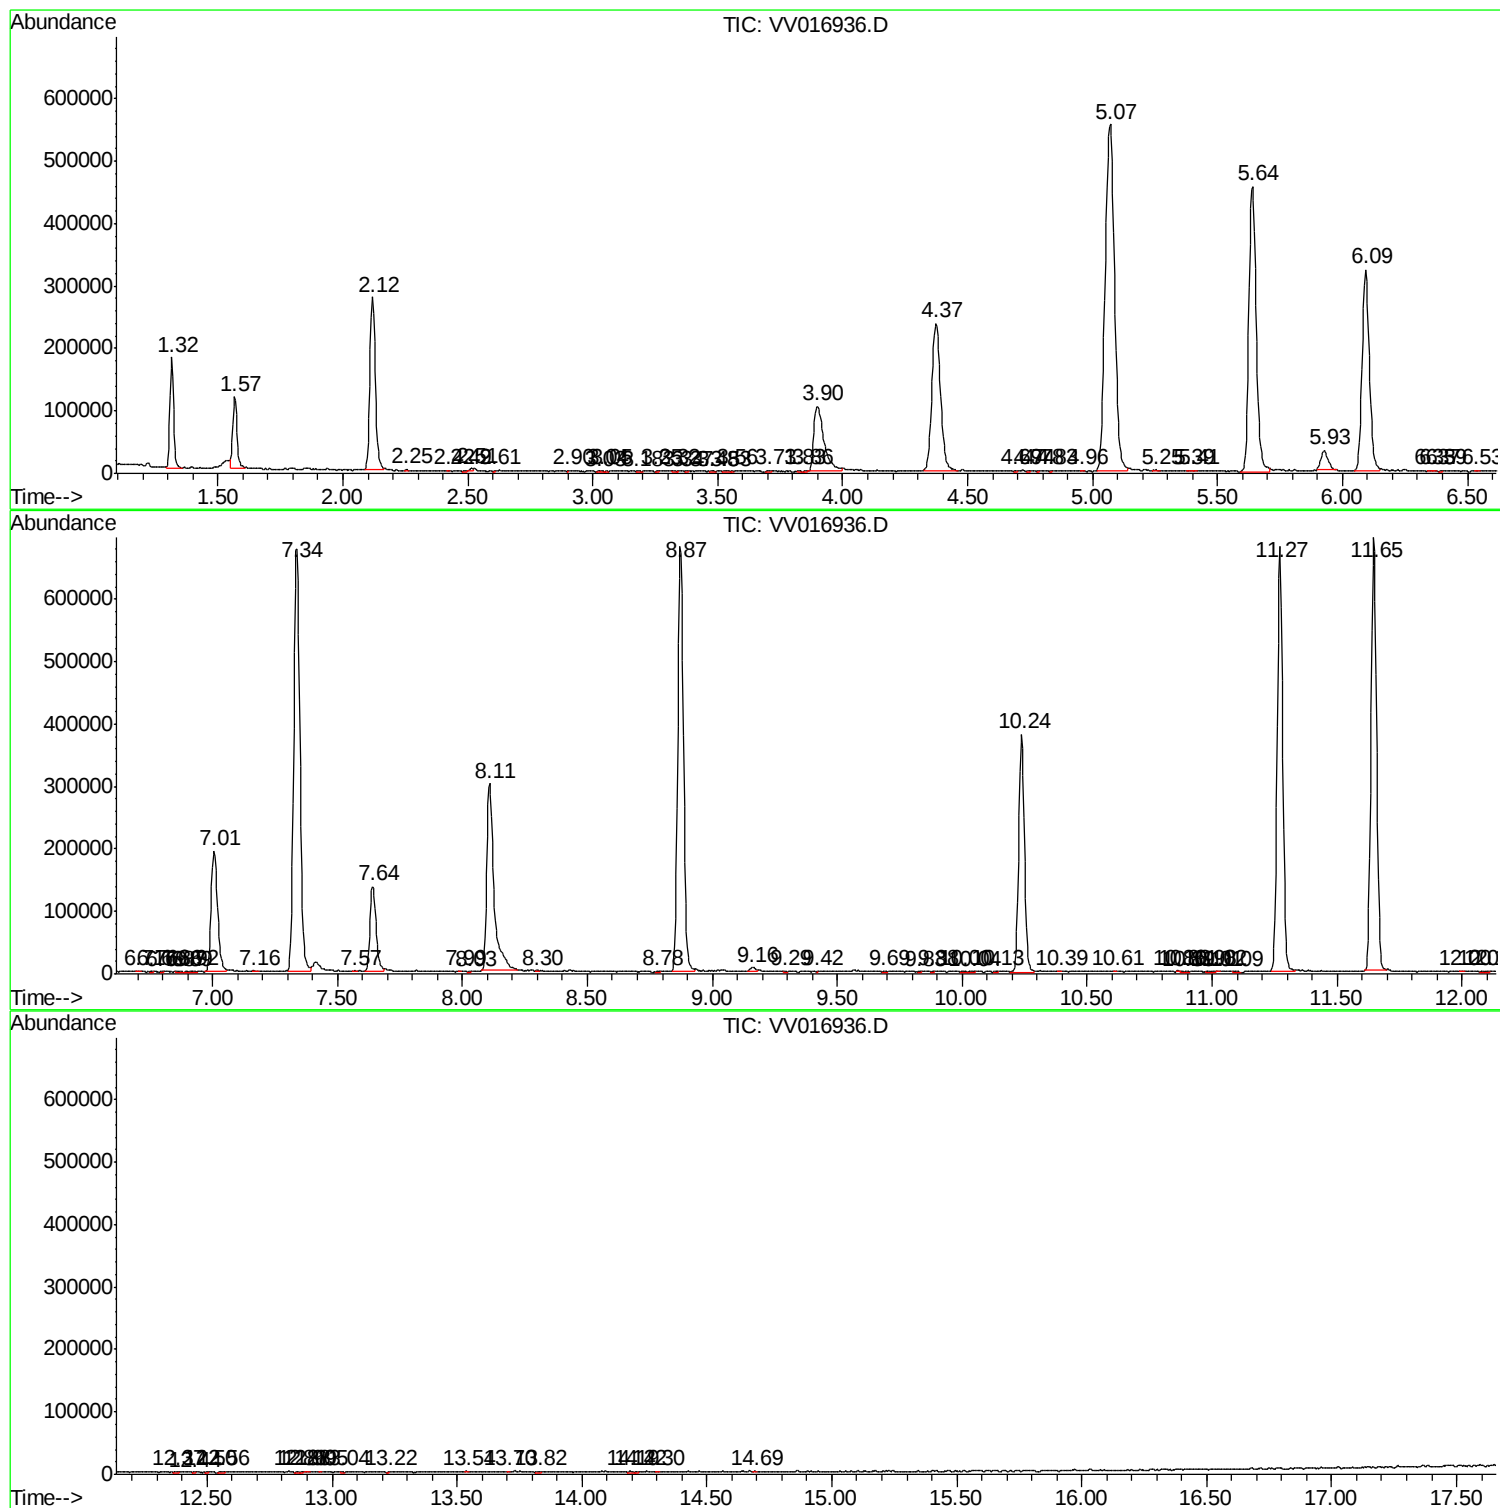

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016936.D
Acq On : 15 Jun 2020 15:05
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061520\
Data File : VV016936.D
Acq On : 15 Jun 2020 15:05
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK62

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc