

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016938.D
 Acq On : 15 Jun 2020 15:53
 Operator : SY/MD
 Sample : L2990-10DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	169216	172336	12.42%	1.527%
2	2.116	311	319	334	rVB	265113	393159	28.33%	3.485%
3	2.438	416	419	422	rVB4	1637	804	0.06%	0.007%
4	2.502	437	439	440	rBV2	1219	683	0.05%	0.006%
5	2.785	520	527	532	rBV8	2546	2473	0.18%	0.022%
6	2.846	542	546	547	rBV4	832	485	0.03%	0.004%
7	2.859	548	550	552	rBV3	762	419	0.03%	0.004%
8	2.939	573	575	577	rVB4	1017	416	0.03%	0.004%
9	2.958	577	581	583	rBV4	1140	866	0.06%	0.008%
10	3.036	600	605	609	rBV5	1824	1974	0.14%	0.017%
11	3.113	626	629	633	rBV6	1246	1066	0.08%	0.009%
12	3.158	641	643	644	rBV2	1089	369	0.03%	0.003%
13	3.261	670	675	678	rBV7	2011	1486	0.11%	0.013%
14	3.296	685	686	690	rBV3	703	520	0.04%	0.005%
15	3.344	699	701	703	rBV3	637	413	0.03%	0.004%
16	3.364	703	707	709	rBV4	1695	1344	0.10%	0.012%
17	3.463	736	738	740	rBV3	785	468	0.03%	0.004%
18	3.489	744	746	750	rVB4	2044	1289	0.09%	0.011%
19	3.524	750	757	761	rBV8	2081	2741	0.20%	0.024%
20	3.624	785	788	790	rBV3	1235	740	0.05%	0.007%
21	3.730	819	821	823	rVB3	1527	615	0.04%	0.005%
22	3.746	823	826	827	rBV2	1273	659	0.05%	0.006%
23	3.820	847	849	850	rBV2	889	441	0.03%	0.004%
24	3.897	860	873	894	rBV	102382	285559	20.58%	2.531%
25	4.145	948	950	952	rBV3	1186	719	0.05%	0.006%
26	4.254	981	984	991	rBV7	1151	1026	0.07%	0.009%
27	4.286	991	994	996	rBV3	1439	695	0.05%	0.006%
28	4.373	1007	1021	1052	rVB	224702	548981	39.56%	4.866%
29	4.585	1084	1087	1089	rBV4	1164	792	0.06%	0.007%
30	4.621	1094	1098	1100	rBV5	1355	889	0.06%	0.008%
31	4.634	1100	1102	1104	rBV3	1208	589	0.04%	0.005%
32	4.749	1136	1138	1142	rBV4	919	779	0.06%	0.007%
33	4.881	1176	1179	1184	rBV7	2126	1588	0.11%	0.014%
34	4.904	1184	1186	1187	rBV2	1043	499	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016938.D
 Acq On : 15 Jun 2020 15:53
 Operator : SY/MD
 Sample : L2990-10DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.952	1197	1201	1202	rBV2	1381	850	0.06%	0.008%
36	5.071	1221	1238	1263	rBV2	543747	1387616	100.00%	12.299%
37	5.640	1401	1415	1439	rBV	435308	884932	63.77%	7.843%
38	6.093	1540	1556	1579	rBV	311977	638430	46.01%	5.659%
39	6.566	1699	1703	1705	rBV4	1002	849	0.06%	0.008%
40	6.605	1712	1715	1717	rBV4	1835	1093	0.08%	0.010%
41	6.717	1746	1750	1751	rBV3	1819	1225	0.09%	0.011%
42	6.913	1808	1811	1813	rBV4	1607	1109	0.08%	0.010%
43	6.952	1819	1823	1825	rBV3	1140	950	0.07%	0.008%
44	7.006	1830	1840	1857	rVV	182814	322977	23.28%	2.863%
45	7.145	1881	1883	1888	rBV6	1268	921	0.07%	0.008%
46	7.232	1908	1910	1912	rBV3	1320	556	0.04%	0.005%
47	7.338	1931	1943	1961	rBV	654350	1115530	80.39%	9.887%
48	7.640	2028	2037	2053	rBV	132595	217494	15.67%	1.928%
49	7.904	2118	2119	2121	rBV	717	398	0.03%	0.004%
50	8.045	2161	2163	2166	rBV4	1801	651	0.05%	0.006%
51	8.109	2173	2183	2213	rBV2	294559	601699	43.36%	5.333%
52	8.534	2313	2315	2319	rBV5	1755	1630	0.12%	0.014%
53	8.682	2358	2361	2363	rBV4	1316	1113	0.08%	0.010%
54	8.823	2401	2405	2407	rBV5	1335	1134	0.08%	0.010%
55	8.875	2409	2421	2437	rVV	657592	1056963	76.17%	9.368%
56	9.035	2461	2471	2484	rBV	140660	226314	16.31%	2.006%
57	9.158	2499	2509	2526	rVB	434825	682546	49.19%	6.050%
58	10.035	2775	2782	2784	rBV8	1891	2135	0.15%	0.019%
59	10.122	2807	2809	2812	rVB4	1739	893	0.06%	0.008%
60	10.238	2834	2845	2861	rBV	368857	580630	41.84%	5.146%
61	10.344	2875	2878	2879	rBV3	1998	1105	0.08%	0.010%
62	10.723	2993	2996	2998	rBV4	1310	952	0.07%	0.008%
63	10.862	3034	3039	3040	rBV4	1463	1119	0.08%	0.010%
64	10.939	3057	3063	3073	rBV10	5204	7744	0.56%	0.069%
65	11.055	3096	3099	3101	rBV3	1678	980	0.07%	0.009%
66	11.270	3155	3166	3188	rBV	654544	1020757	73.56%	9.047%
67	11.473	3227	3229	3230	rBV2	1685	512	0.04%	0.005%
68	11.524	3243	3245	3248	rBV3	1318	493	0.04%	0.004%
69	11.592	3264	3266	3267	rBV2	996	360	0.03%	0.003%
70	11.646	3272	3283	3301	rVV	691076	1065474	76.78%	9.444%
71	11.929	3369	3371	3375	rVB4	1284	678	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016938.D
 Acq On : 15 Jun 2020 15:53
 Operator : SY/MD
 Sample : L2990-10DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.952	3375	3378	3379	rBV3	1187	726	0.05%	0.006%
73	11.990	3388	3390	3394	rVB4	1912	1214	0.09%	0.011%
74	12.064	3411	3413	3414	rBV2	1294	607	0.04%	0.005%
75	12.199	3452	3455	3457	rBV3	1167	676	0.05%	0.006%
76	12.212	3457	3459	3462	rVB3	1361	572	0.04%	0.005%
77	12.251	3468	3471	3476	rBV6	1862	1753	0.13%	0.016%
78	12.305	3486	3488	3489	rBV2	1328	494	0.04%	0.004%
79	12.392	3513	3515	3517	rBV4	907	386	0.03%	0.003%
80	12.408	3518	3520	3522	rBV4	1291	613	0.04%	0.005%
81	12.527	3554	3557	3558	rBV3	1018	479	0.03%	0.004%
82	12.582	3571	3574	3576	rBV4	1382	927	0.07%	0.008%
83	12.762	3628	3630	3633	rBV4	1073	750	0.05%	0.007%
84	12.897	3669	3672	3674	rBV4	1288	755	0.05%	0.007%
85	12.993	3700	3702	3705	rBV4	1489	649	0.05%	0.006%
86	13.013	3706	3708	3709	rBV2	955	388	0.03%	0.003%
87	13.048	3716	3719	3720	rBV3	2088	911	0.07%	0.008%
88	13.222	3771	3773	3775	rBV2	2061	795	0.06%	0.007%
89	13.505	3859	3861	3866	rVB5	1894	1089	0.08%	0.010%
90	13.530	3866	3869	3871	rBV4	1482	1151	0.08%	0.010%
91	13.678	3911	3915	3918	rVB5	1725	1230	0.09%	0.011%
92	13.694	3918	3920	3922	rBV3	1247	571	0.04%	0.005%
93	13.771	3940	3944	3947	rBV4	1440	1285	0.09%	0.011%
94	14.045	4026	4029	4033	rBV4	1731	1632	0.12%	0.014%
95	14.128	4052	4055	4056	rBV2	1816	1104	0.08%	0.010%
96	14.370	4128	4130	4131	rBV2	1040	402	0.03%	0.004%
97	14.424	4145	4147	4151	rBV5	1543	935	0.07%	0.008%
98	14.460	4156	4158	4159	rBV2	1409	563	0.04%	0.005%
99	14.546	4183	4185	4188	rBV4	1234	503	0.04%	0.004%
100	14.807	4264	4266	4268	rBV3	1444	704	0.05%	0.006%


Sum of corrected areas: 11282558

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
Data File : VV016938.D
Acq On : 15 Jun 2020 15:53
Operator : SY/MD
Sample : L2990-10DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YG6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

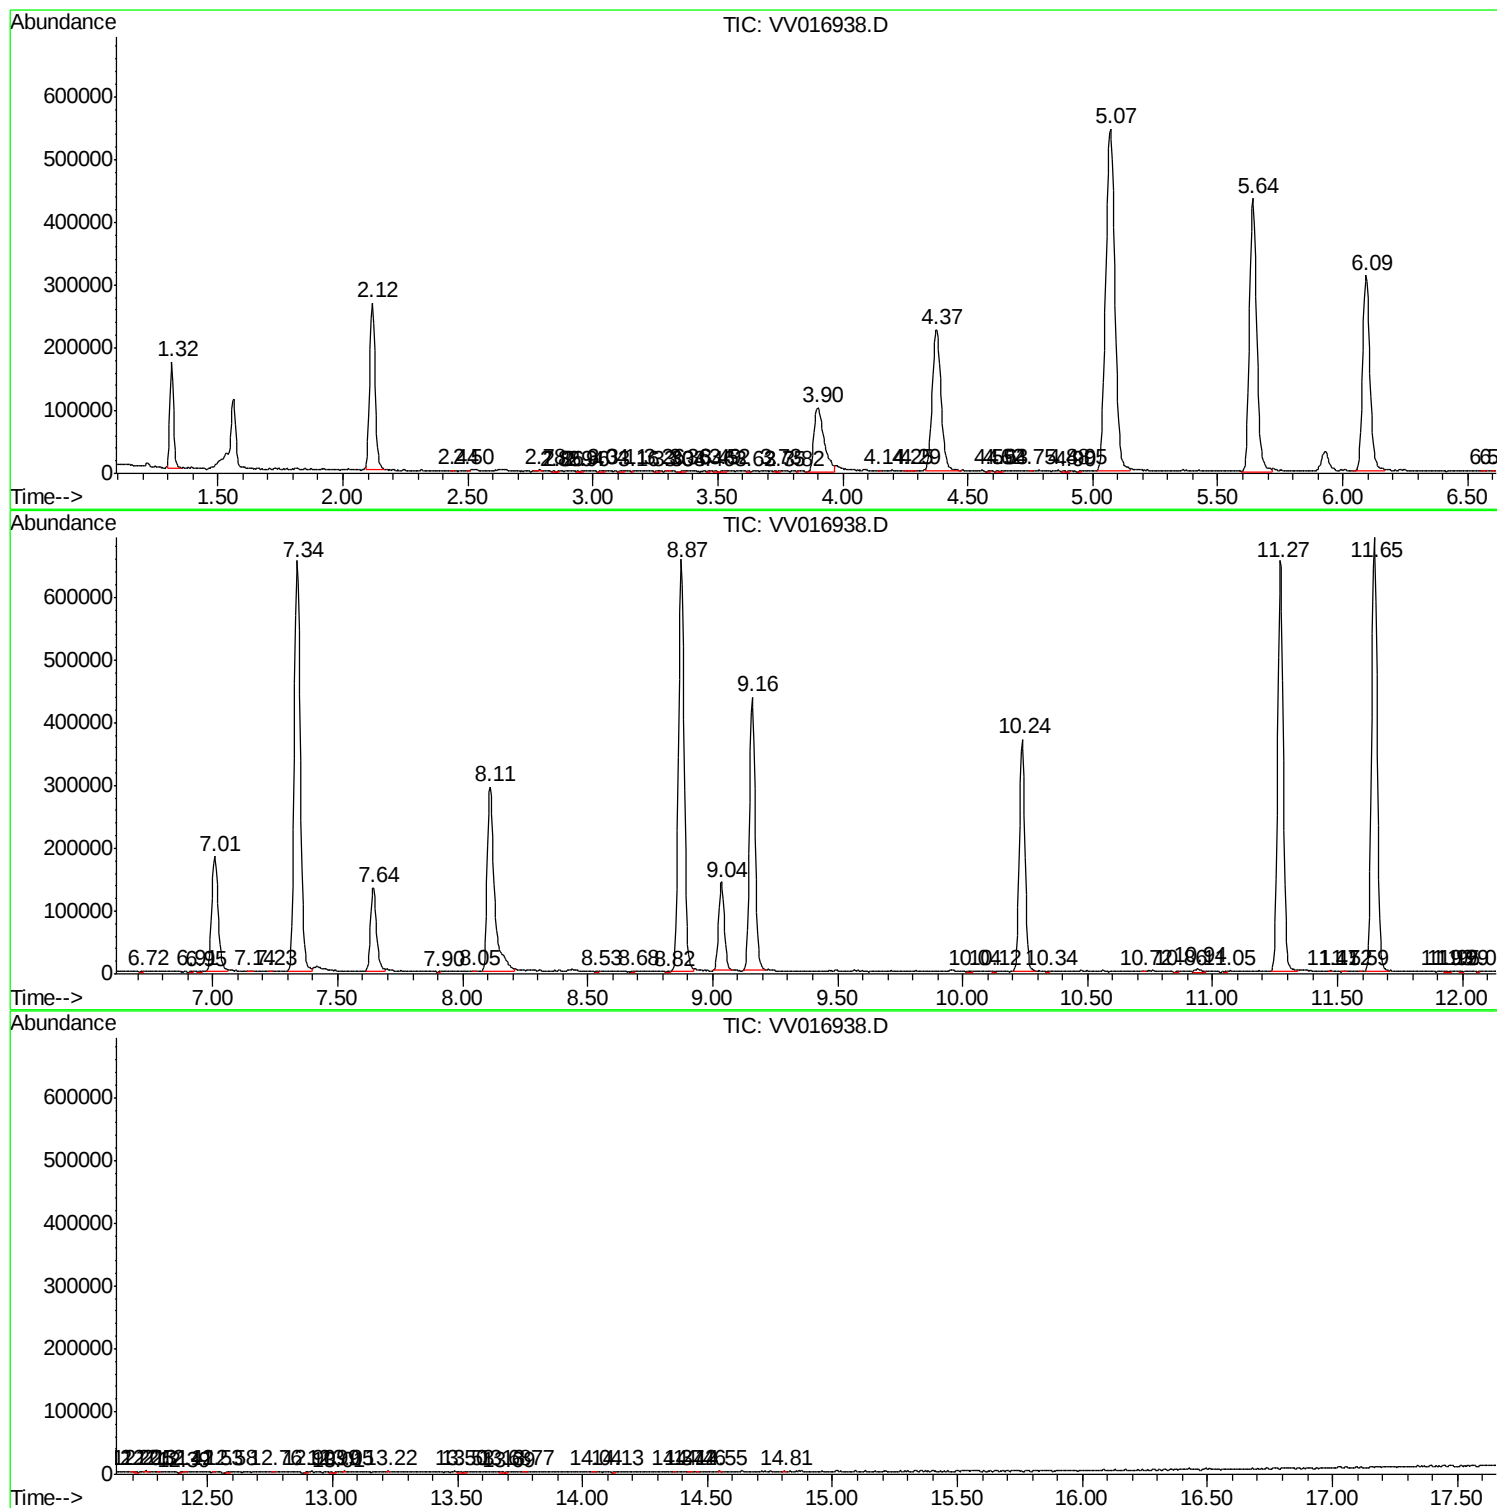

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016938.D
Acq On : 15 Jun 2020 15:53
Operator : SY/MD
Sample : L2990-10DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YG6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016938.D
Acq On : 15 Jun 2020 15:53
Operator : SY/MD
Sample : L2990-10DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YG6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc