

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016944.D
 Acq On : 15 Jun 2020 19:02
 Operator : SY/MD
 Sample : L2947-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	81	rVB	165439	164989	12.06%	1.575%
2	1.573	143	150	165	rVB	122210	139663	10.21%	1.333%
3	2.119	311	320	335	rVB	264167	387503	28.33%	3.699%
4	2.463	423	427	430	rBV4	1220	1060	0.08%	0.010%
5	2.727	507	509	512	rVB4	1812	937	0.07%	0.009%
6	2.798	529	531	535	rVB5	1274	886	0.06%	0.008%
7	2.897	557	562	564	rBV4	1806	1273	0.09%	0.012%
8	2.965	579	583	584	rBV4	978	703	0.05%	0.007%
9	3.267	673	677	679	rBV4	999	730	0.05%	0.007%
10	3.280	679	681	683	rBV3	1365	716	0.05%	0.007%
11	3.386	712	714	717	rBV3	1285	780	0.06%	0.007%
12	3.524	754	757	759	rBV4	1155	638	0.05%	0.006%
13	3.640	791	793	795	rVB3	1807	600	0.04%	0.006%
14	3.688	806	808	812	rVB3	1219	659	0.05%	0.006%
15	3.708	812	814	818	rVB4	1799	1150	0.08%	0.011%
16	3.733	818	822	823	rBV3	1447	1230	0.09%	0.012%
17	3.766	829	832	835	rBV4	1518	1124	0.08%	0.011%
18	3.791	838	840	842	rBV2	1229	641	0.05%	0.006%
19	3.897	863	873	906	rBV	101672	281492	20.58%	2.687%
20	4.377	1007	1022	1043	rVV	222191	542556	39.67%	5.179%
21	4.811	1155	1157	1159	rBV2	1386	713	0.05%	0.007%
22	4.830	1159	1163	1164	rVV3	1448	979	0.07%	0.009%
23	4.862	1168	1173	1175	rBV3	1858	1575	0.12%	0.015%
24	4.910	1185	1188	1189	rBV3	1517	778	0.06%	0.007%
25	4.942	1195	1198	1201	rVB4	1462	901	0.07%	0.009%
26	4.997	1213	1215	1218	rVB3	2092	940	0.07%	0.009%
27	5.071	1220	1238	1259	rBV2	532614	1367610	100.00%	13.055%
28	5.261	1295	1297	1303	rVB6	2056	1255	0.09%	0.012%
29	5.489	1365	1368	1370	rBV3	1918	1095	0.08%	0.010%
30	5.640	1402	1415	1436	rBV	431570	852985	62.37%	8.142%
31	5.872	1485	1487	1492	rBV6	1448	1053	0.08%	0.010%
32	5.930	1492	1505	1522	rBV3	29993	66845	4.89%	0.638%
33	6.093	1542	1556	1578	rBV	308659	626509	45.81%	5.981%
34	6.550	1695	1698	1700	rBV4	1482	870	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016944.D
 Acq On : 15 Jun 2020 19:02
 Operator : SY/MD
 Sample : L2947-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.608	1713	1716	1718	rVB4	1365	753	0.06%	0.007%
36	6.643	1724	1727	1729	rBV4	1317	926	0.07%	0.009%
37	6.704	1743	1746	1747	rBV3	1297	796	0.06%	0.008%
38	6.811	1775	1779	1780	rBV4	1140	822	0.06%	0.008%
39	6.823	1781	1783	1790	rVV8	1875	1966	0.14%	0.019%
40	6.856	1791	1793	1796	rVB4	1362	610	0.04%	0.006%
41	6.958	1820	1825	1827	rBV5	1585	1369	0.10%	0.013%
42	7.007	1830	1840	1857	rVV	177780	313415	22.92%	2.992%
43	7.216	1901	1905	1909	rBV6	2276	1971	0.14%	0.019%
44	7.338	1927	1943	1960	rBV	649713	1111433	81.27%	10.610%
45	7.643	2028	2038	2054	rBV2	127903	218319	15.96%	2.084%
46	7.772	2077	2078	2083	rVB4	1958	1203	0.09%	0.011%
47	7.894	2113	2116	2117	rBV3	1327	630	0.05%	0.006%
48	8.106	2172	2182	2215	rBV2	301461	585051	42.78%	5.585%
49	8.479	2296	2298	2301	rBV4	1410	652	0.05%	0.006%
50	8.566	2323	2325	2326	rBV2	1394	699	0.05%	0.007%
51	8.875	2405	2421	2438	rBV	643151	1042619	76.24%	9.953%
52	9.138	2501	2503	2505	rBV3	1838	833	0.06%	0.008%
53	9.283	2546	2548	2550	rBV2	1557	624	0.05%	0.006%
54	9.325	2558	2561	2563	rBV3	2032	1137	0.08%	0.011%
55	9.376	2575	2577	2581	rBV5	1493	727	0.05%	0.007%
56	9.463	2601	2604	2607	rBV4	1599	1086	0.08%	0.010%
57	9.505	2614	2617	2620	rBV5	1305	973	0.07%	0.009%
58	9.707	2678	2680	2683	rVB3	1679	826	0.06%	0.008%
59	9.958	2753	2758	2759	rBV5	1582	1468	0.11%	0.014%
60	10.142	2812	2815	2818	rBV4	1437	1035	0.08%	0.010%
61	10.238	2833	2845	2859	rBV	373015	577647	42.24%	5.514%
62	10.334	2873	2875	2879	rBV3	1417	683	0.05%	0.007%
63	10.392	2890	2893	2897	rBV6	1174	901	0.07%	0.009%
64	10.553	2940	2943	2945	rBV4	977	660	0.05%	0.006%
65	10.669	2977	2979	2984	rVB6	1344	975	0.07%	0.009%
66	11.016	3085	3087	3091	rBV4	1854	1197	0.09%	0.011%
67	11.119	3116	3119	3121	rBV4	1268	671	0.05%	0.006%
68	11.154	3126	3130	3133	rBV6	1122	790	0.06%	0.008%
69	11.183	3135	3139	3141	rBV4	1354	983	0.07%	0.009%
70	11.270	3154	3166	3184	rBV	666075	1029636	75.29%	9.829%
71	11.486	3230	3233	3237	rBV3	2524	2102	0.15%	0.020%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061520\
 Data File : VV016944.D
 Acq On : 15 Jun 2020 19:02
 Operator : SY/MD
 Sample : L2947-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3269	3283	3300	rBV	690639	1082153	79.13%	10.330%
73	11.836	3340	3342	3343	rBV2	1272	619	0.05%	0.006%
74	11.907	3361	3364	3366	rBV4	1218	854	0.06%	0.008%
75	12.331	3492	3496	3497	rBV4	1174	812	0.06%	0.008%
76	12.405	3516	3519	3522	rBV5	1339	904	0.07%	0.009%
77	12.421	3522	3524	3529	rVB7	1329	984	0.07%	0.009%
78	12.553	3563	3565	3569	rBV5	1417	933	0.07%	0.009%
79	12.595	3576	3578	3583	rVB4	1999	1156	0.08%	0.011%
80	12.617	3583	3585	3587	rBV3	1602	840	0.06%	0.008%
81	12.762	3625	3630	3634	rBV6	1486	1706	0.12%	0.016%
82	13.026	3710	3712	3716	rVB5	1694	1136	0.08%	0.011%
83	13.135	3741	3746	3749	rBV6	2215	2374	0.17%	0.023%
84	13.276	3786	3790	3792	rBV3	1946	1426	0.10%	0.014%
85	13.350	3810	3813	3815	rBV4	1411	891	0.07%	0.009%
86	13.367	3816	3818	3822	rVB4	1693	1074	0.08%	0.010%
87	13.466	3847	3849	3853	rVB4	1778	1057	0.08%	0.010%
88	13.534	3867	3870	3871	rBV2	1882	1016	0.07%	0.010%
89	13.604	3889	3892	3893	rBV3	1308	656	0.05%	0.006%
90	13.627	3896	3899	3902	rBV3	1923	1290	0.09%	0.012%
91	13.646	3902	3905	3907	rBV4	1165	695	0.05%	0.007%
92	13.788	3947	3949	3955	rVB6	1413	1004	0.07%	0.010%
93	13.810	3955	3956	3959	rBV3	1039	626	0.05%	0.006%
94	13.830	3959	3962	3965	rBV3	1428	1186	0.09%	0.011%
95	13.900	3977	3984	3989	rBV10	1947	2760	0.20%	0.026%
96	13.948	3998	3999	4003	rBV2	978	601	0.04%	0.006%
97	13.971	4003	4006	4008	rBV3	952	567	0.04%	0.005%
98	14.106	4045	4048	4049	rBV2	1288	618	0.05%	0.006%
99	14.267	4096	4098	4104	rVB7	1134	926	0.07%	0.009%
100	14.714	4233	4237	4244	rBV8	2099	3236	0.24%	0.031%


Sum of corrected areas: 10475726

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061520\
Data File : VV016944.D
Acq On : 15 Jun 2020 19:02
Operator : SY/MD
Sample : L2947-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

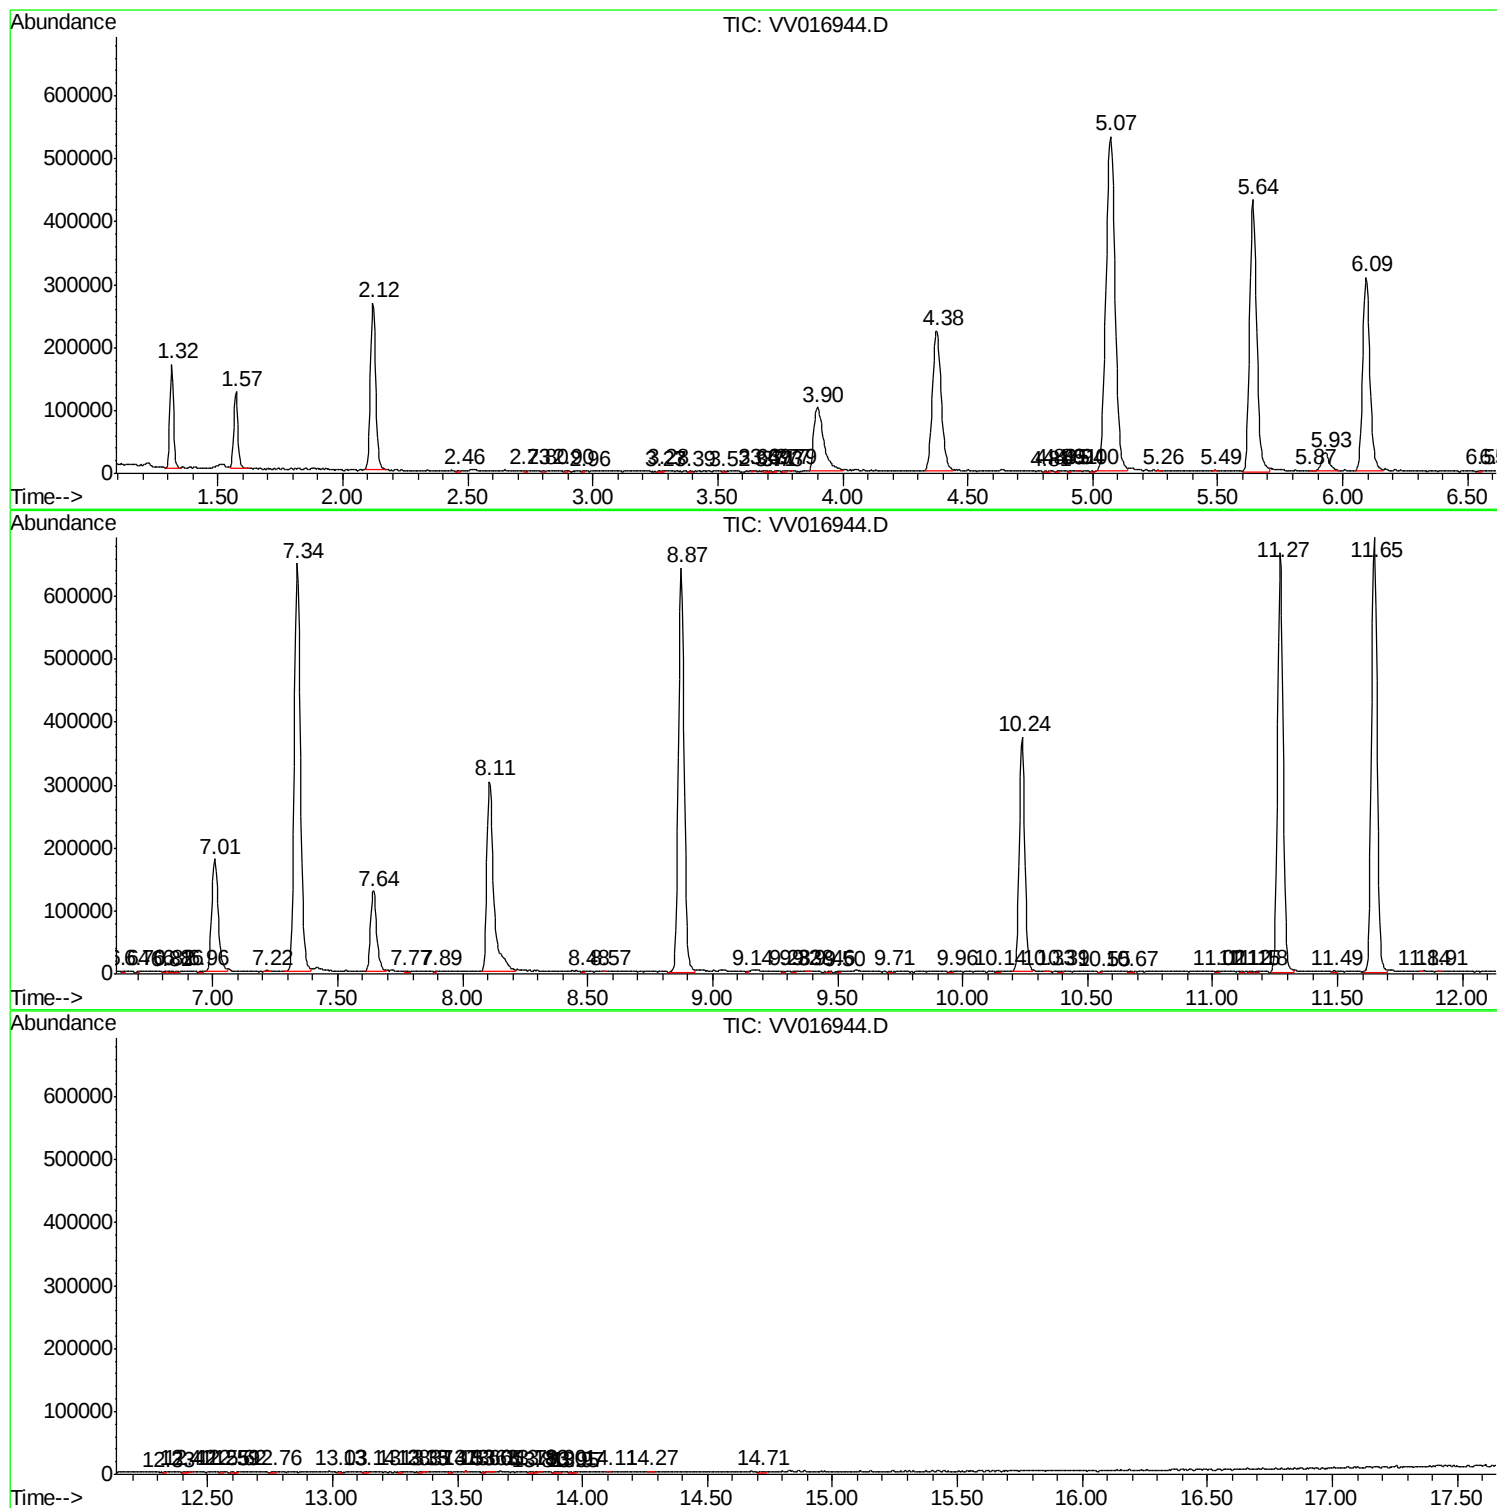

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016944.D
Acq On : 15 Jun 2020 19:02
Operator : SY/MD
Sample : L2947-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061520\
Data File : VV016944.D
Acq On : 15 Jun 2020 19:02
Operator : SY/MD
Sample : L2947-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc