


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061520\
 Data File : VV016924.D
 Acq On : 15 Jun 2020 09:26
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 16 05:46:50 2020

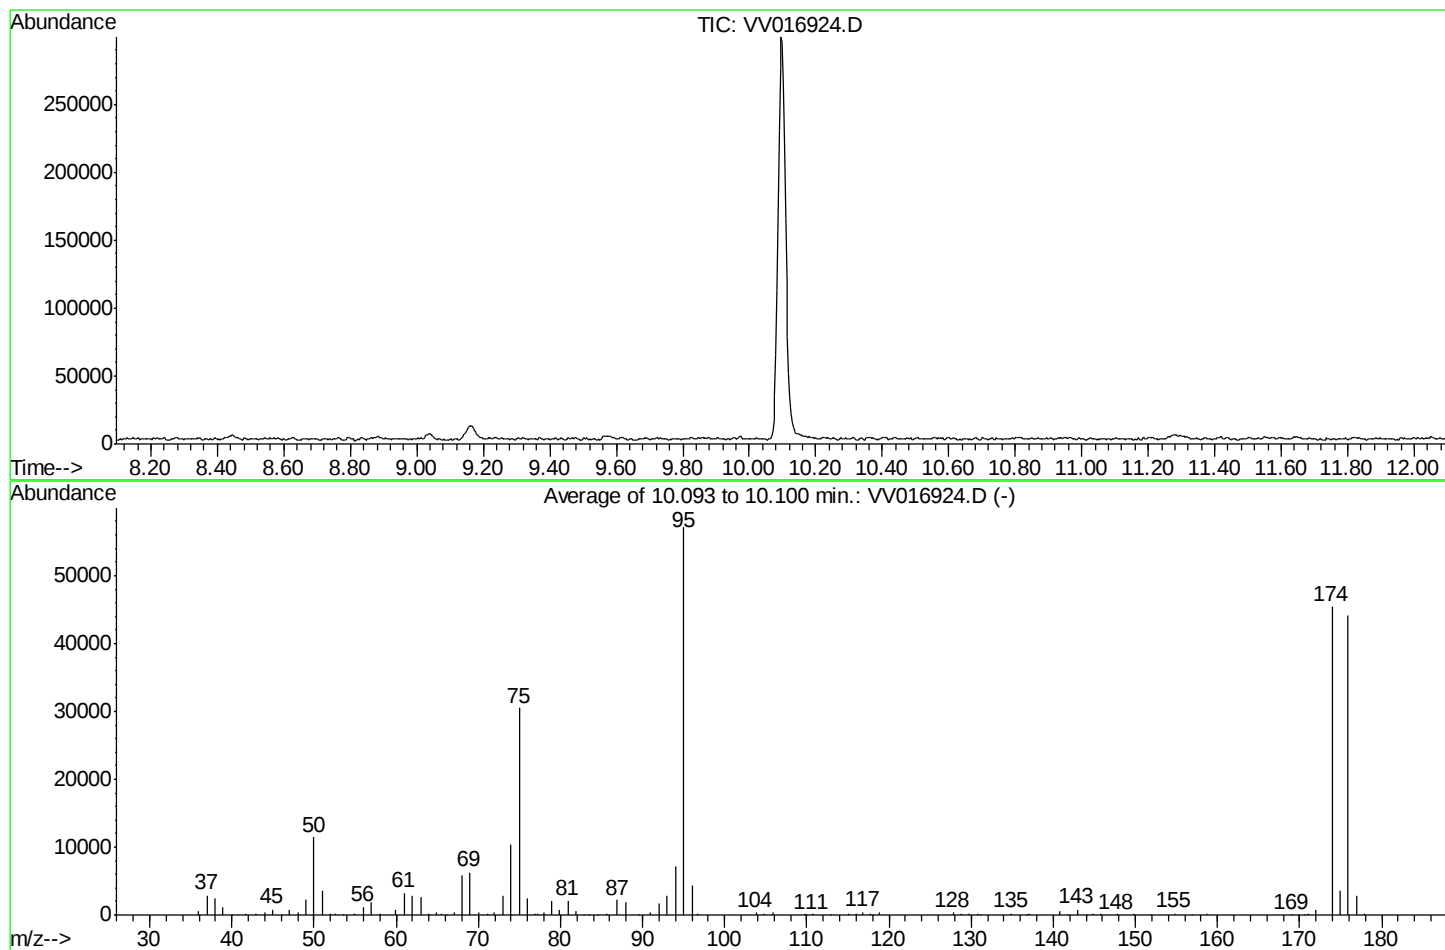

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11450	PASS
75	95	30	80	53.4	30528	PASS
95	95	100	100	100.0	57117	PASS
96	95	5	9	7.6	4319	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.4	45376	PASS
175	174	5	9	7.9	3571	PASS
176	174	95	101	97.3	44165	PASS
177	176	5	9	6.5	2854	PASS

m/z	Abundance
36.00	532.0
37.00	3048.0
38.00	2523.0
39.00	1238.0
40.00	479.0
41.10	128.0
41.70	193.0
42.80	233.0
44.00	680.0
44.90	715.0
46.10	166.0
47.00	749.0
48.10	485.0
49.00	2329.0
50.00	11315.0
51.00	3657.0
52.00	267.0
52.70	145.0
53.70	105.0
55.00	223.0
56.00	1179.0
57.00	1725.0
58.00	181.0
59.90	779.0
61.00	3007.0
62.00	2740.0
63.00	2470.0
64.00	194.0
64.90	421.0
67.00	278.0
68.00	5860.0
69.00	6301.0
70.00	453.0
71.10	132.0
71.80	327.0
73.00	2784.0
74.00	9928.0
75.00	29240.0
76.00	2551.0
76.90	323.0
78.00	296.0
78.90	2031.0
79.90	713.0
80.90	2105.0
82.00	531.0
83.40	104.0
84.50	120.0
85.60	135.0
86.90	2375.0
88.00	1894.0
91.00	384.0
92.00	1760.0
93.00	2601.0
94.00	6834.0
95.00	54272.0
96.00	4323.0
96.70	162.0
103.80	334.0
104.90	136.0
105.90	285.0
109.80	147.0
110.60	148.0
112.90	122.0
114.90	163.0
115.90	238.0
116.90	434.0
117.80	287.0
118.80	286.0
127.90	324.0
128.90	158.0
129.70	206.0
130.80	114.0
131.10	119.0
134.90	199.0
136.80	145.0
140.90	630.0
141.70	165.0
142.90	703.0
144.90	159.0
145.80	118.0
147.70	142.0
149.90	120.0
151.80	103.0
154.80	261.0
156.90	144.0
158.70	114.0
171.00	142.0
172.00	701.0
173.90	42560.0
174.90	3345.0
175.90	40104.0
176.90	2695.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

177.90

155.0

Instrument :

MSVOA_V

ClientSampleId :

BFB89

m/z	Abundance
36.00	607.0
37.00	3130.0
38.00	2762.0
39.00	1315.0
39.90	429.0
41.10	133.0
41.80	174.0
43.00	192.0
44.00	747.0
45.00	795.0
46.10	167.0
47.00	778.0
48.10	523.0
49.00	2388.0
50.00	11698.0
51.00	3800.0
52.00	198.0
52.60	145.0
54.90	244.0
56.00	1237.0
57.00	1852.0
58.00	197.0
59.90	797.0
61.00	3382.0
62.00	3001.0
63.00	2647.0
63.90	210.0
64.90	398.0
65.60	149.0
67.10	305.0
68.00	6060.0
69.00	6537.0
70.00	423.0
71.20	156.0
71.90	380.0
73.00	3054.0
74.00	10710.0
75.00	31472.0
76.00	2524.0
77.10	323.0
78.10	327.0
78.90	2188.0
79.90	834.0
80.90	2213.0
82.00	514.0
82.80	107.0
85.70	136.0
86.90	2221.0
88.00	1999.0
90.90	393.0
92.00	1810.0
93.00	2856.0
94.00	7483.0
95.00	58992.0
96.00	4482.0
96.80	171.0
103.80	376.0
104.80	133.0
105.90	305.0
109.80	120.0
110.60	171.0
115.00	135.0
116.00	255.0
116.90	424.0
117.80	245.0
118.90	398.0
127.90	382.0
128.80	177.0
129.70	255.0
130.80	130.0
134.90	208.0
137.00	178.0
140.80	664.0
141.60	137.0
142.90	835.0
144.80	146.0
145.70	148.0
147.80	151.0
149.90	124.0
154.80	252.0
156.90	101.0
158.80	145.0
169.10	127.0
171.00	178.0
172.00	747.0
173.90	46744.0
175.00	3706.0
175.90	45640.0
177.00	3011.0
177.80	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.10	129.0
35.90	669.0
37.00	2837.0
38.00	2674.0
39.00	1213.0
39.90	364.0
41.10	117.0
42.00	175.0
43.00	208.0
44.00	774.0
45.00	786.0
46.20	188.0
46.90	708.0
48.00	493.0
49.00	2334.0
50.00	11338.0
51.00	3543.0
51.90	152.0
52.50	102.0
53.50	105.0
54.80	290.0
56.00	1104.0
57.00	1852.0
58.00	223.0
60.00	634.0
61.00	3326.0
62.00	3031.0
63.00	2630.0
63.90	231.0
64.90	318.0
65.60	163.0
66.10	113.0
67.10	311.0
68.00	5675.0
69.00	6244.0
70.00	407.0
71.30	179.0
71.90	420.0
73.00	2931.0
74.00	10320.0
75.00	30872.0
76.00	2429.0
77.20	344.0
78.10	306.0
78.90	2147.0
79.90	772.0
80.90	2136.0
81.90	472.0
82.80	123.0
85.80	140.0
86.90	2014.0
88.00	1972.0
89.50	109.0
90.90	341.0
92.00	1694.0
93.00	2808.0
94.00	7258.0
95.00	58088.0
96.00	4153.0
96.80	181.0
103.80	371.0
104.70	135.0
105.90	341.0
109.90	101.0
110.00	101.0
110.70	155.0
115.10	118.0
115.90	239.0
116.80	418.0
117.70	213.0
118.00	187.0
118.90	413.0
127.80	359.0
128.80	174.0
129.70	297.0
130.90	136.0
134.90	192.0
137.00	176.0
140.80	671.0
142.90	919.0
144.00	111.0
144.80	156.0
145.70	191.0
147.70	157.0
149.90	118.0
154.80	217.0
158.80	154.0
169.00	135.0
169.80	103.0
170.50	106.0
171.00	164.0
171.90	635.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

173.90	46824.0
175.00	3664.0
175.90	46752.0
177.00	2856.0
177.80	225.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.30	142.0
36.00	102.0
37.10	128.0
38.00	127.0
38.90	119.0
39.90	343.0
41.20	164.0
42.10	104.0
42.90	234.0
44.00	412.0
46.00	113.0
48.20	128.0
48.70	103.0
49.30	117.0
53.90	151.0
58.80	107.0
59.60	104.0
68.80	108.0
77.80	136.0
78.90	109.0
94.60	103.0
111.50	106.0
138.50	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89