

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031545.D
 Acq On : 15 Jun 2023 21:56
 Operator : SY/MD
 Sample : VW0616WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK357

Quant Time: Jun 16 05:51:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 16 05:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	252085	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	246326	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	123307	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.285	65	63153	37.643	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.280%		
7) Chloroethane-d5	1.539	69	61892	42.280	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.560%		
11) 1,1-Dichloroethene-d2	2.066	65	33673	38.944	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.880%		
21) 2-Butanone-d5	3.802	46	113757	83.738	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.740%		
24) Chloroform-d	4.259	84	171506	40.818	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.640%		
26) 1,2-Dichloroethane-d4	4.950	65	115473	43.925	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.860%		
32) Benzene-d6	4.969	84	306609	44.221	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.440%		
36) 1,2-Dichloropropane-d6	5.995	67	109245	44.454	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.900%		
41) Toluene-d8	7.252	98	266337	41.860	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.720%		
43) trans-1,3-Dichloroprop...	7.558	79	50288	41.977	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.960%		
47) 2-Hexanone-d5	8.034	63	85100	87.706	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.710%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	155258	41.856	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.720%		
66) 1,2-Dichlorobenzene-d4	11.567	152	112762	47.975	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.940%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.918	75	3297	0.922	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031545.D
Acq On : 15 Jun 2023 21:56
Operator : SY/MD
Sample : VV0616WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Time: Jun 16 05:51:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 16 05:51:14 2023
Response via : Initial Calibration

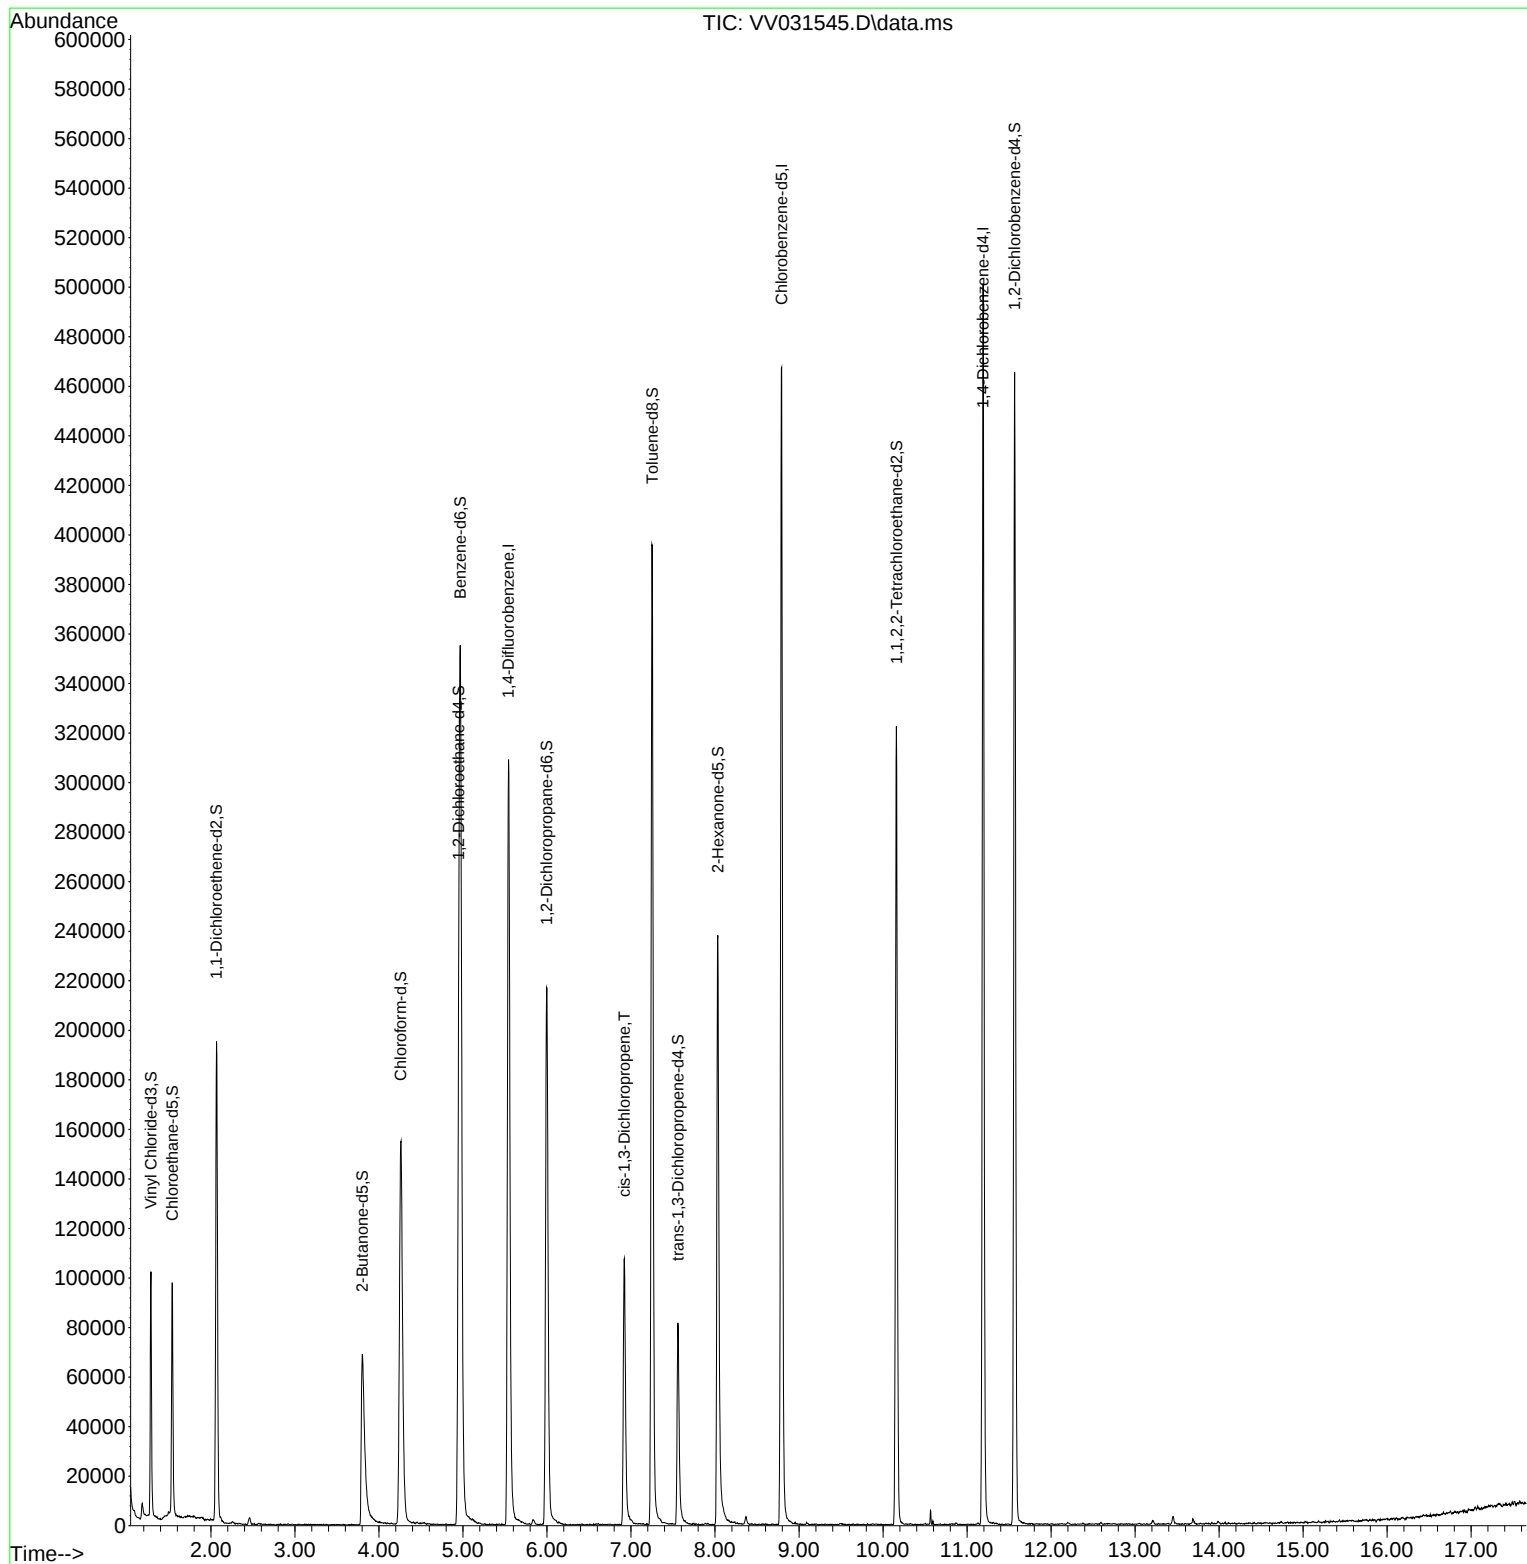

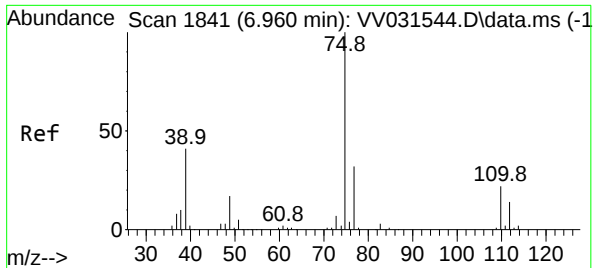

#39
 cis-1,3-Dichloropropene
 Concen: 0.922 ug/L
 RT: 6.918 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV031545.D
 Acq: 15 Jun 2023 21:56

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK357

Tgt Ion: 75 Resp: 3297
 Ion Ratio Lower Upper
 75 100
 77 39.8 21.8 40.6

