

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031520.D
 Acq On : 15 Jun 2023 10:59
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK356

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	104200	111188	12.27%	1.604%
2	1.539	148	155	168	rVB	93711	112803	12.45%	1.628%
3	2.063	309	318	337	rVB	196339	288917	31.89%	4.169%
4	2.404	416	424	425	rBV2	279	334	0.04%	0.005%
5	2.458	433	441	448	rVB4	2073	3273	0.36%	0.047%
6	2.507	453	456	459	rBV2	336	227	0.03%	0.003%
7	2.526	459	462	463	rBV2	160	97	0.01%	0.001%
8	2.600	483	485	487	rBV	194	120	0.01%	0.002%
9	2.645	495	499	504	rVV3	369	358	0.04%	0.005%
10	2.667	504	506	512	rVB2	307	242	0.03%	0.003%
11	2.809	549	550	551	rBV2	142	42	0.00%	0.001%
12	2.828	551	556	562	rVV	482	545	0.06%	0.008%
13	2.960	592	597	600	rBV	164	171	0.02%	0.002%
14	2.979	600	603	606	rBV2	219	164	0.02%	0.002%
15	2.998	606	609	613	rVV2	212	204	0.02%	0.003%
16	3.111	640	644	645	rBV	276	169	0.02%	0.002%
17	3.137	650	652	653	rBV	148	76	0.01%	0.001%
18	3.195	666	670	672	rBV2	377	311	0.03%	0.004%
19	3.227	677	680	684	rVV	198	146	0.02%	0.002%
20	3.355	717	720	723	rBV	144	126	0.01%	0.002%
21	3.375	723	726	728	rVV	257	170	0.02%	0.002%
22	3.404	732	735	738	rBV	122	81	0.01%	0.001%
23	3.423	739	741	747	rVB	326	266	0.03%	0.004%
24	3.445	747	748	751	rBV	247	132	0.01%	0.002%
25	3.548	773	780	787	rBV3	273	430	0.05%	0.006%
26	3.580	787	790	793	rBB	221	172	0.02%	0.002%
27	3.609	795	799	803	rBV2	242	261	0.03%	0.004%
28	3.651	810	812	815	rBV2	151	70	0.01%	0.001%
29	3.722	831	834	835	rBV	343	200	0.02%	0.003%
30	3.802	850	859	891	rBV	57667	166107	18.34%	2.397%
31	4.256	984	1000	1030	rBV2	155192	395075	43.61%	5.701%
32	4.696	1135	1137	1139	rBV	182	83	0.01%	0.001%
33	4.735	1147	1149	1150	rBV	176	82	0.01%	0.001%
34	4.760	1155	1157	1160	rVB	181	63	0.01%	0.001%
35	4.847	1180	1184	1186	rBV2	242	159	0.02%	0.002%
36	4.867	1186	1190	1193	rBV	183	130	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031520.D
 Acq On : 15 Jun 2023 10:59
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK356

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	4.886	1193	1196	1197	rBV	175	103	0.01%	0.001%
38	4.963	1202	1220	1247	rBV2	340482	905930	100.00%	13.072%
39	5.236	1304	1305	1309	rVB2	267	144	0.02%	0.002%
40	5.333	1332	1335	1337	rBV2	238	158	0.02%	0.002%
41	5.539	1387	1399	1424	rBV	270837	564352	62.30%	8.143%
42	5.841	1483	1493	1497	rBV6	1708	3008	0.33%	0.043%
43	5.931	1518	1521	1523	rBV	221	107	0.01%	0.002%
44	5.995	1527	1541	1564	rBV	209262	436679	48.20%	6.301%
45	6.133	1582	1584	1589	rBV3	778	515	0.06%	0.007%
46	6.227	1610	1613	1614	rBV	163	78	0.01%	0.001%
47	6.323	1640	1643	1644	rBV	247	125	0.01%	0.002%
48	6.362	1650	1655	1657	rBV2	220	192	0.02%	0.003%
49	6.609	1730	1732	1735	rVB3	515	260	0.03%	0.004%
50	6.632	1736	1739	1742	rVB	253	139	0.02%	0.002%
51	6.677	1751	1753	1755	rBV	71	35	0.00%	0.001%
52	6.693	1755	1758	1763	rBV2	294	278	0.03%	0.004%
53	6.866	1810	1812	1817	rBV2	142	133	0.01%	0.002%
54	6.918	1817	1828	1853	rBV	103235	193101	21.32%	2.786%
55	7.143	1896	1898	1904	rVB4	588	511	0.06%	0.007%
56	7.172	1904	1907	1908	rBV2	313	174	0.02%	0.003%
57	7.249	1918	1931	1956	rBV	369684	655376	72.34%	9.456%
58	7.500	2006	2009	2012	rBV3	314	206	0.02%	0.003%
59	7.558	2016	2027	2054	rBV	77828	141451	15.61%	2.041%
60	7.844	2113	2116	2118	rBV2	356	230	0.03%	0.003%
61	7.921	2139	2140	2145	rVB2	320	114	0.01%	0.002%
62	8.030	2164	2174	2208	rBV	211533	392253	43.30%	5.660%
63	8.342	2269	2271	2275	rBV2	397	173	0.02%	0.002%
64	8.378	2275	2282	2286	rBV5	576	766	0.08%	0.011%
65	8.429	2295	2298	2306	rBV2	362	426	0.05%	0.006%
66	8.632	2357	2361	2366	rVB3	442	342	0.04%	0.005%
67	8.728	2390	2391	2392	rBV3	174	60	0.01%	0.001%
68	8.789	2398	2410	2442	rBV	433956	705599	77.89%	10.181%
69	8.989	2471	2472	2476	rVB	213	64	0.01%	0.001%
70	9.056	2491	2493	2495	rBV2	361	189	0.02%	0.003%
71	9.124	2512	2514	2519	rBV2	292	183	0.02%	0.003%
72	9.223	2543	2545	2547	rVB	175	57	0.01%	0.001%
73	9.243	2547	2551	2554	rVB	269	179	0.02%	0.003%
74	9.272	2554	2560	2562	rBV2	305	365	0.04%	0.005%
75	9.931	2762	2765	2767	rBV2	276	182	0.02%	0.003%
76	10.159	2824	2836	2855	rBV	311061	483606	53.38%	6.978%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031520.D
 Acq On : 15 Jun 2023 10:59
 Operator : SY/MD
 Sample : VV0615WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK356

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	10.320	2884	2886	2887	rBV	538	242	0.03%	0.003%
78	10.371	2898	2902	2906	rBV2	422	376	0.04%	0.005%
79	10.574	2963	2965	2968	rBV	195	106	0.01%	0.002%
80	10.792	3031	3033	3035	rBV	208	104	0.01%	0.002%
81	10.860	3051	3054	3056	rBV	427	304	0.03%	0.004%
82	10.902	3063	3067	3070	rBV	399	279	0.03%	0.004%
83	10.918	3070	3072	3074	rBV	189	64	0.01%	0.001%
84	11.191	3145	3157	3182	rBV	431393	666837	73.61%	9.622%
85	11.352	3204	3207	3210	rBV2	443	336	0.04%	0.005%
86	11.394	3217	3220	3221	rBV2	318	180	0.02%	0.003%
87	11.567	3262	3274	3292	rBV	431081	672380	74.22%	9.702%
88	11.802	3345	3347	3350	rVB2	407	177	0.02%	0.003%
89	11.821	3350	3353	3355	rBV	430	279	0.03%	0.004%
90	12.011	3406	3412	3416	rVB3	464	541	0.06%	0.008%
91	12.378	3523	3526	3535	rVB3	473	497	0.05%	0.007%
92	12.638	3604	3607	3610	rBV2	348	299	0.03%	0.004%
93	13.156	3763	3768	3770	rBV2	460	402	0.04%	0.006%
94	13.207	3778	3784	3794	rBV5	2451	3046	0.34%	0.044%
95	13.451	3854	3860	3874	rVB3	5309	8335	0.92%	0.120%
96	13.689	3927	3934	3945	rVB7	2715	4218	0.47%	0.061%
97	14.496	4182	4185	4190	rBV3	660	676	0.07%	0.010%




Sum of corrected areas: 6930515

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031520.D
Acq On : 15 Jun 2023 10:59
Operator : SY/MD
Sample : VV0615WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK356

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

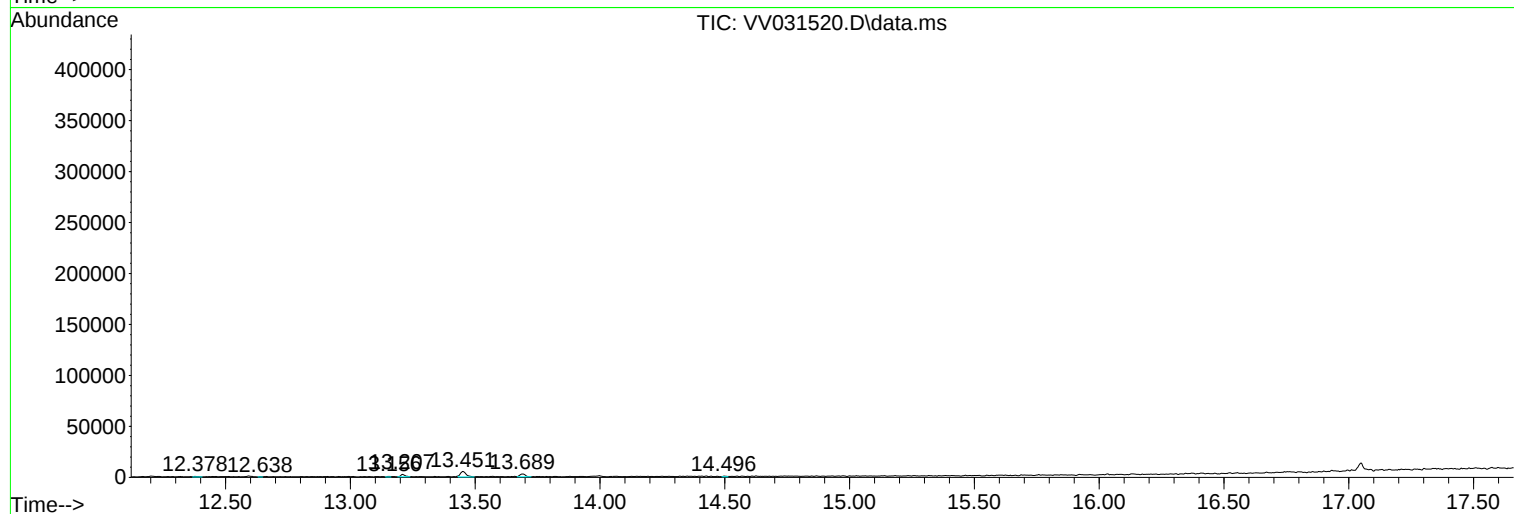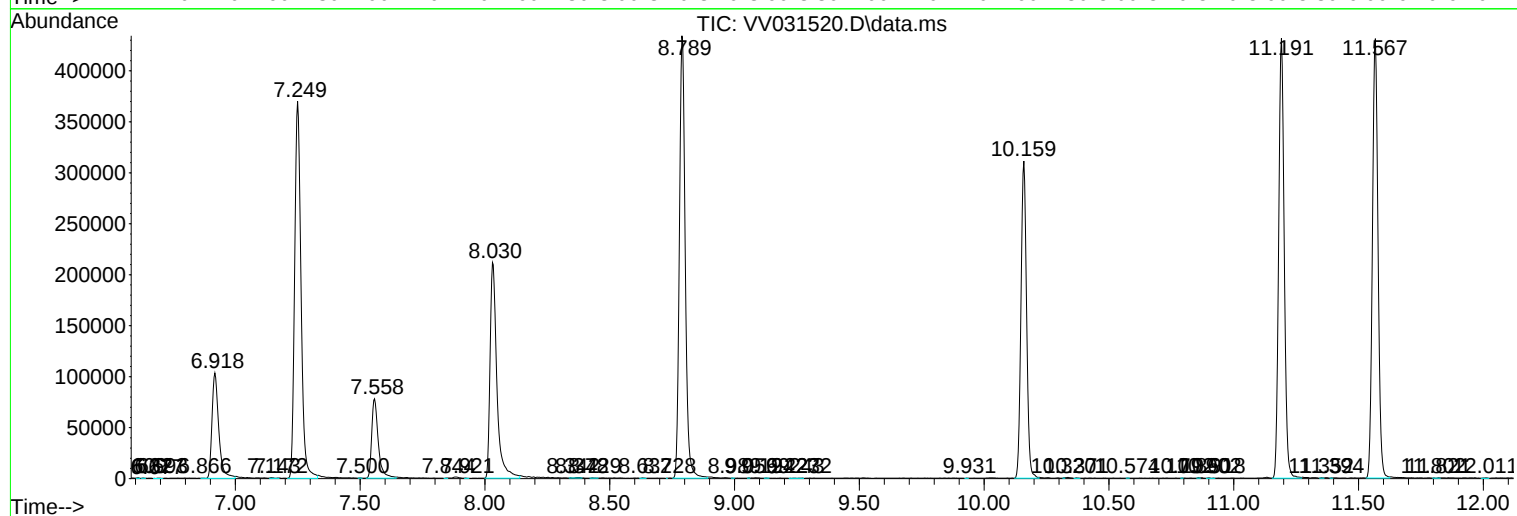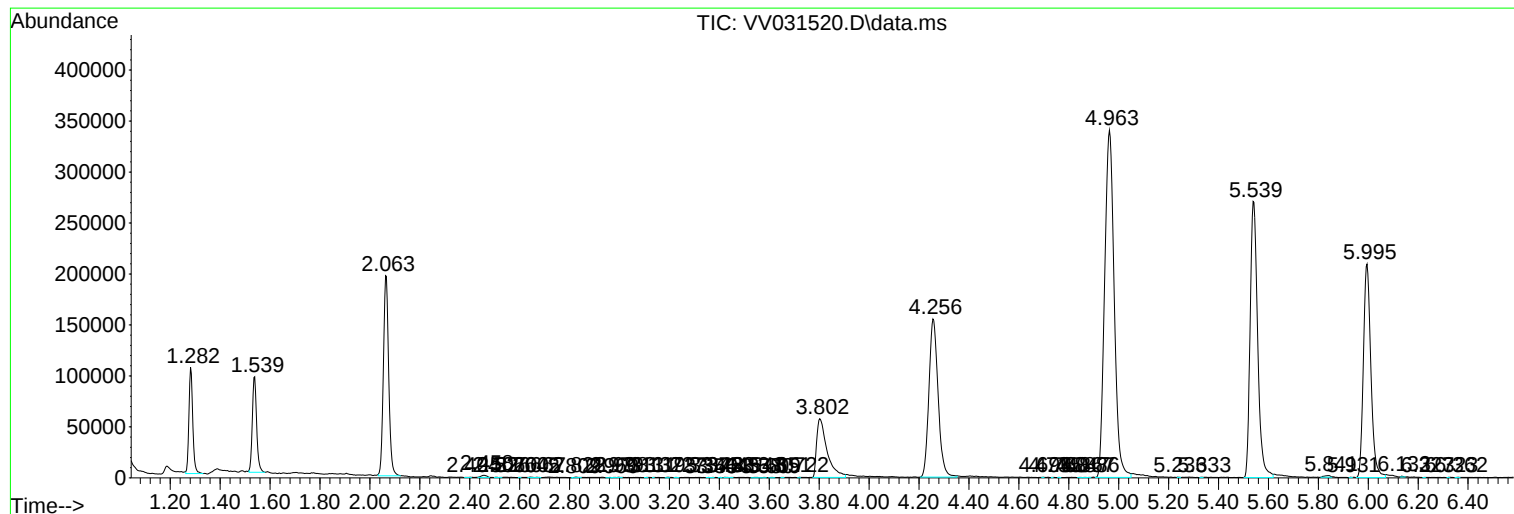

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031520.D
Acq On : 15 Jun 2023 10:59
Operator : SY/MD
Sample : VV0615WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK356

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031520.D
Acq On : 15 Jun 2023 10:59
Operator : SY/MD
Sample : VV0615WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK356

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------