

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031521.D
 Acq On : 15 Jun 2023 11:23
 Operator : SY/MD
 Sample : 03254-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	53	rBV	11343	15177	1.65%	0.204%
2	1.282	69	75	95	rVB	103760	113034	12.29%	1.523%
3	1.397	102	111	129	rBV	7404	23664	2.57%	0.319%
4	1.539	148	155	173	rVB	96145	119693	13.01%	1.613%
5	2.066	309	319	335	rVB	196591	285265	31.01%	3.843%
6	2.240	368	373	374	rBV2	452	407	0.04%	0.005%
7	2.310	390	395	402	rVB3	741	767	0.08%	0.010%
8	2.458	435	441	448	rVB4	1096	1353	0.15%	0.018%
9	2.564	470	474	481	rBV4	361	365	0.04%	0.005%
10	2.709	509	519	528	rBV3	7574	13253	1.44%	0.179%
11	2.783	538	542	549	rVB2	366	472	0.05%	0.006%
12	3.124	633	648	671	rVB2	12407	27028	2.94%	0.364%
13	3.217	671	677	681	rBV2	417	540	0.06%	0.007%
14	3.699	824	827	832	rVB3	464	416	0.05%	0.006%
15	3.741	832	840	845	rBV	309	480	0.05%	0.006%
16	3.806	849	860	898	rBV2	66954	220433	23.96%	2.970%
17	4.121	954	958	966	rVB5	644	762	0.08%	0.010%
18	4.185	975	978	983	rBV3	260	265	0.03%	0.004%
19	4.259	983	1001	1027	rBV2	155242	405103	44.03%	5.458%
20	4.523	1068	1083	1105	rVB3	27168	70980	7.72%	0.956%
21	4.966	1203	1221	1263	rVV2	341055	919988	100.00%	12.395%
22	5.349	1336	1340	1341	rBV2	302	229	0.02%	0.003%
23	5.542	1385	1400	1421	rBV	274397	559444	60.81%	7.537%
24	5.703	1448	1450	1457	rVB4	580	540	0.06%	0.007%
25	5.844	1482	1494	1513	rVV3	40846	84544	9.19%	1.139%
26	5.995	1527	1541	1578	rVV	210934	443496	48.21%	5.975%
27	6.162	1592	1593	1598	rVB3	713	412	0.04%	0.006%
28	6.185	1598	1600	1606	rVB3	557	515	0.06%	0.007%
29	6.310	1636	1639	1644	rBV2	326	237	0.03%	0.003%
30	6.375	1656	1659	1665	rVB2	427	285	0.03%	0.004%
31	6.439	1674	1679	1681	rBV	360	289	0.03%	0.004%
32	6.593	1724	1727	1730	rBV3	303	223	0.02%	0.003%
33	6.764	1777	1780	1783	rVV2	320	237	0.03%	0.003%
34	6.918	1817	1828	1847	rBV	104626	194070	21.09%	2.615%
35	7.072	1873	1876	1880	rVB3	308	260	0.03%	0.004%
36	7.111	1884	1888	1891	rVB2	282	244	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031521.D
 Acq On : 15 Jun 2023 11:23
 Operator : SY/MD
 Sample : 03254-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.133	1891	1895	1897	rBV2	550	402	0.04%	0.005%
38	7.182	1904	1910	1912	rBV	455	357	0.04%	0.005%
39	7.249	1920	1931	1965	rBV	372496	657333	71.45%	8.856%
40	7.513	2011	2013	2016	rVB2	426	234	0.03%	0.003%
41	7.558	2016	2027	2055	rBV	82055	148935	16.19%	2.007%
42	7.683	2064	2066	2070	rVB3	484	277	0.03%	0.004%
43	7.911	2117	2137	2157	rVB3	76481	143129	15.56%	1.928%
44	8.030	2164	2174	2209	rBV	219385	404541	43.97%	5.450%
45	8.227	2234	2235	2238	rBV2	469	258	0.03%	0.003%
46	8.320	2261	2264	2267	rBV2	377	264	0.03%	0.004%
47	8.538	2329	2332	2335	rBV	230	217	0.02%	0.003%
48	8.789	2398	2410	2431	rBV	434682	697359	75.80%	9.395%
49	8.953	2457	2461	2463	rBV3	520	452	0.05%	0.006%
50	8.966	2463	2465	2467	rVV	524	300	0.03%	0.004%
51	8.982	2467	2470	2472	rVV3	524	403	0.04%	0.005%
52	9.091	2499	2504	2511	rVV4	615	757	0.08%	0.010%
53	9.506	2629	2633	2636	rBV2	273	221	0.02%	0.003%
54	9.735	2700	2704	2706	rBV2	285	211	0.02%	0.003%
55	9.783	2716	2719	2722	rBV	248	214	0.02%	0.003%
56	9.969	2770	2777	2784	rBV2	254	385	0.04%	0.005%
57	10.159	2824	2836	2854	rBV	311321	493137	53.60%	6.644%
58	10.329	2879	2889	2902	rVB2	6241	9940	1.08%	0.134%
59	10.805	3033	3037	3042	rVB4	271	224	0.02%	0.003%
60	10.876	3049	3059	3062	rBV3	369	525	0.06%	0.007%
61	11.133	3134	3139	3145	rVB3	798	959	0.10%	0.013%
62	11.191	3145	3157	3181	rBV	424134	662659	72.03%	8.928%
63	11.297	3188	3190	3194	rVB4	399	226	0.02%	0.003%
64	11.567	3262	3274	3296	rVV	433753	673186	73.17%	9.070%
65	11.696	3312	3314	3319	rBV2	411	327	0.04%	0.004%
66	11.763	3331	3335	3338	rBV3	356	316	0.03%	0.004%
67	11.783	3338	3341	3344	rBV	337	271	0.03%	0.004%
68	11.824	3351	3354	3357	rVB2	354	233	0.03%	0.003%
69	11.911	3378	3381	3385	rBV3	288	217	0.02%	0.003%
70	11.956	3391	3395	3399	rBV2	306	262	0.03%	0.004%
71	12.201	3464	3471	3480	rVB5	2077	3228	0.35%	0.043%
72	12.294	3497	3500	3505	rVB	293	213	0.02%	0.003%
73	12.358	3518	3520	3525	rBV2	340	294	0.03%	0.004%
74	12.426	3534	3541	3546	rBV3	408	483	0.05%	0.007%
75	12.455	3547	3550	3556	rVB3	294	237	0.03%	0.003%
76	12.587	3589	3591	3592	rBV	593	250	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031521.D
 Acq On : 15 Jun 2023 11:23
 Operator : SY/MD
 Sample : 03254-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.796	3652	3656	3658	rBV	352	310	0.03%	0.004%
78	12.850	3671	3673	3678	rVB2	288	223	0.02%	0.003%
79	12.908	3687	3691	3693	rBV2	314	241	0.03%	0.003%
80	13.111	3751	3754	3758	rVB3	517	365	0.04%	0.005%
81	13.149	3764	3766	3770	rVB2	313	213	0.02%	0.003%
82	13.210	3779	3785	3792	rVV6	1577	1817	0.20%	0.024%
83	13.307	3812	3815	3818	rVB	333	222	0.02%	0.003%
84	13.451	3854	3860	3871	rVB2	2446	3254	0.35%	0.044%
85	13.689	3926	3934	3942	rVB6	1337	1687	0.18%	0.023%
86	13.738	3944	3949	3952	rBV2	310	299	0.03%	0.004%
87	13.850	3981	3984	3986	rBV2	347	234	0.03%	0.003%
88	13.959	4013	4018	4020	rBV2	523	401	0.04%	0.005%
89	13.976	4020	4023	4025	rVV	347	269	0.03%	0.004%
90	13.995	4025	4029	4035	rVB	819	936	0.10%	0.013%
91	14.149	4075	4077	4082	rVB2	389	223	0.02%	0.003%
92	14.230	4098	4102	4105	rBV3	442	449	0.05%	0.006%
93	14.281	4115	4118	4120	rBV3	367	298	0.03%	0.004%
94	14.307	4124	4126	4130	rBV3	289	214	0.02%	0.003%
95	14.352	4138	4140	4143	rBV5	452	289	0.03%	0.004%
96	14.580	4207	4211	4214	rBV4	652	588	0.06%	0.008%
97	14.596	4214	4216	4222	rVB3	577	482	0.05%	0.006%
98	14.721	4252	4255	4257	rBV3	455	315	0.03%	0.004%
99	15.204	4403	4405	4409	rBV2	696	611	0.07%	0.008%
100	15.297	4431	4434	4437	rBV2	525	432	0.05%	0.006%




Sum of corrected areas: 7422278

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031521.D
Acq On : 15 Jun 2023 11:23
Operator : SY/MD
Sample : 03254-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

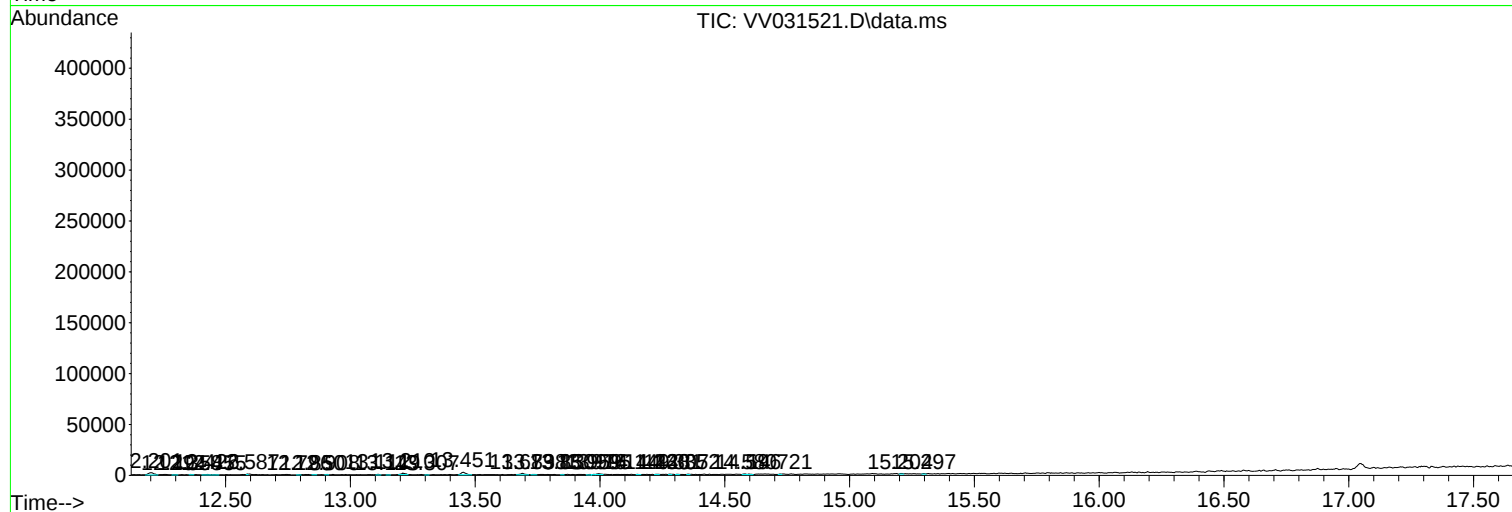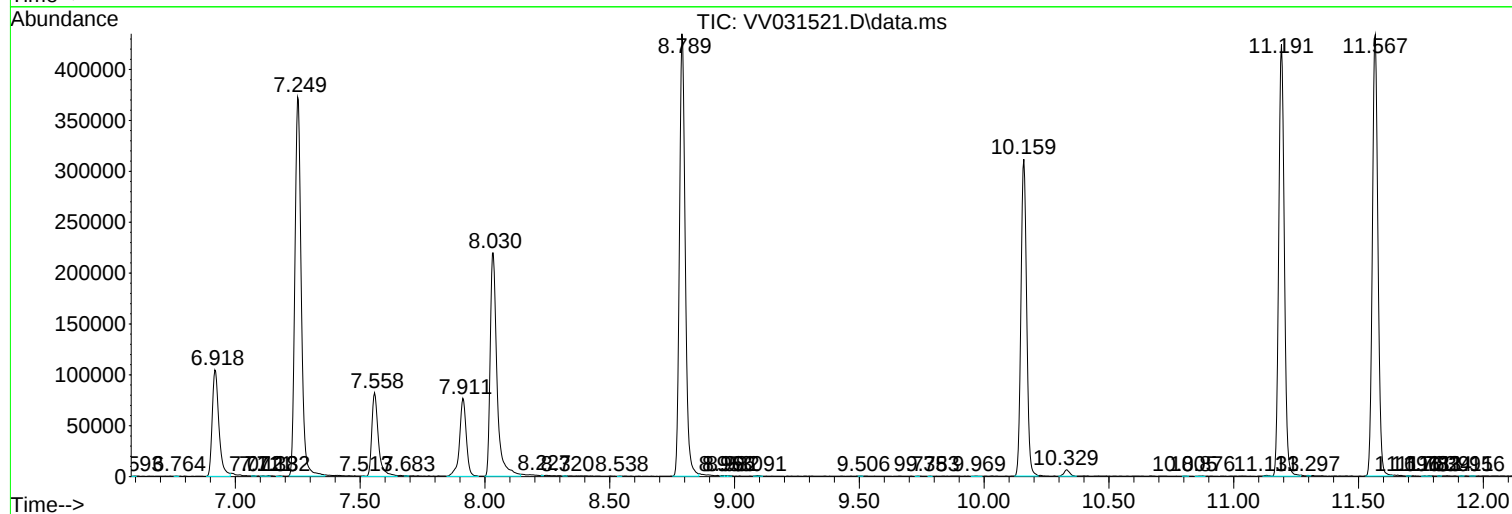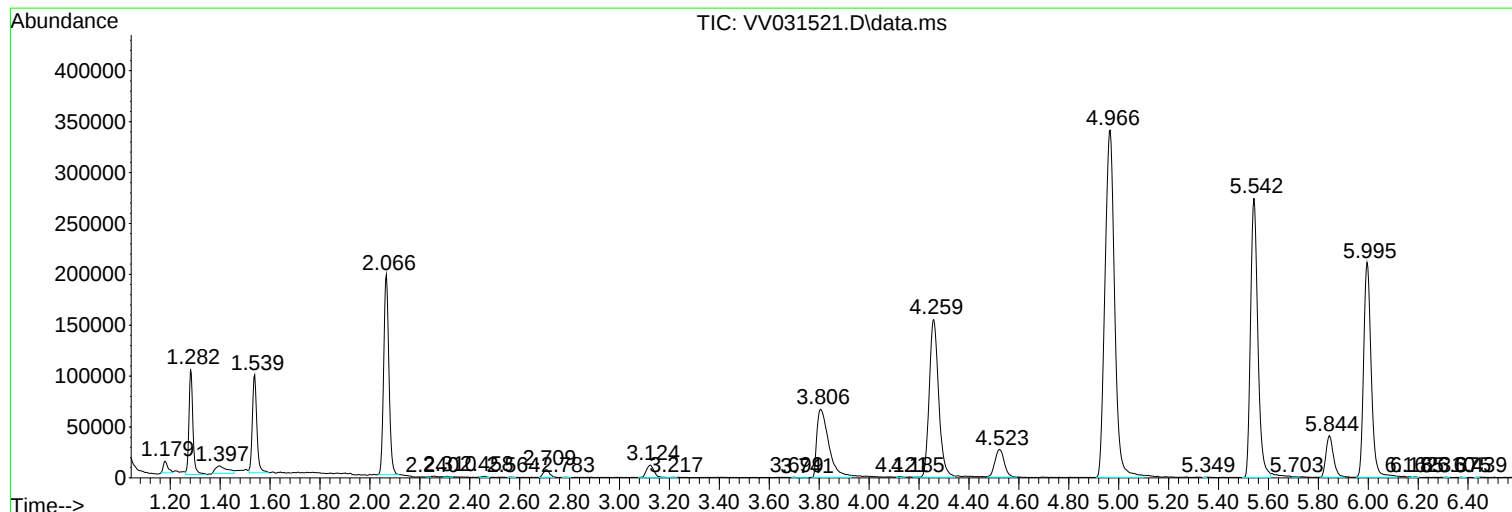

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031521.D
Acq On : 15 Jun 2023 11:23
Operator : SY/MD
Sample : 03254-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031521.D
Acq On : 15 Jun 2023 11:23
Operator : SY/MD
Sample : 03254-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------