

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031529.D
 Acq On : 15 Jun 2023 14:27
 Operator : SY/MD
 Sample : 03249-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	53	rBV	17311	21321	0.48%	0.147%
2	1.285	69	76	90	rVB2	213668	237065	5.28%	1.629%
3	1.539	148	155	176	rVB2	76728	132419	2.95%	0.910%
4	2.066	309	319	335	rBV3	168783	276612	6.16%	1.901%
5	2.252	370	377	381	rVB3	914	1170	0.03%	0.008%
6	2.458	435	441	449	rVB3	1356	1721	0.04%	0.012%
7	2.706	505	518	533	rBV2	22834	42543	0.95%	0.292%
8	2.793	541	545	551	rVB3	482	553	0.01%	0.004%
9	2.969	595	600	605	rVB2	289	329	0.01%	0.002%
10	3.121	630	647	676	rBV	793302	1664053	37.09%	11.437%
11	3.477	754	758	764	rVB3	301	343	0.01%	0.002%
12	3.513	764	769	772	rBV3	435	359	0.01%	0.002%
13	3.532	772	775	779	rVV3	345	303	0.01%	0.002%
14	3.555	779	782	789	rVB3	462	443	0.01%	0.003%
15	3.584	789	791	795	rBV2	586	439	0.01%	0.003%
16	3.686	818	823	825	rBV3	415	364	0.01%	0.003%
17	3.821	848	865	907	rBV	1834525	4486913	100.00%	30.838%
18	4.259	986	1001	1034	rBV	128674	335519	7.48%	2.306%
19	4.522	1062	1083	1114	rBV	772329	1981661	44.17%	13.620%
20	4.966	1203	1221	1243	rBV2	292909	787375	17.55%	5.412%
21	5.207	1294	1296	1300	rVB2	520	361	0.01%	0.002%
22	5.233	1300	1304	1309	rVB4	453	446	0.01%	0.003%
23	5.262	1309	1313	1316	rVB3	393	348	0.01%	0.002%
24	5.294	1316	1323	1327	rVB4	467	487	0.01%	0.003%
25	5.326	1327	1333	1335	rBV4	466	432	0.01%	0.003%
26	5.455	1368	1373	1377	rBV3	355	350	0.01%	0.002%
27	5.542	1386	1400	1424	rBV	218049	446647	9.95%	3.070%
28	5.844	1483	1494	1514	rBV4	22272	47122	1.05%	0.324%
29	5.995	1528	1541	1571	rBV	178549	375516	8.37%	2.581%
30	6.098	1571	1573	1576	rVB4	650	463	0.01%	0.003%
31	6.358	1651	1654	1660	rVB2	350	338	0.01%	0.002%
32	6.921	1818	1829	1849	rBV	91255	172342	3.84%	1.184%
33	7.143	1895	1898	1903	rVV4	397	302	0.01%	0.002%
34	7.249	1917	1931	1954	rBV	306666	547406	12.20%	3.762%
35	7.558	2018	2027	2053	rBV	70303	128315	2.86%	0.882%
36	7.789	2091	2099	2107	rVB5	1197	2005	0.04%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031529.D
 Acq On : 15 Jun 2023 14:27
 Operator : SY/MD
 Sample : 03249-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.911	2116	2137	2153	rBV2	90918	160402	3.57%	1.102%
38	8.030	2165	2174	2204	rBV	218466	387253	8.63%	2.662%
39	8.243	2237	2240	2245	rVB5	640	580	0.01%	0.004%
40	8.429	2297	2298	2301	rVB2	753	299	0.01%	0.002%
41	8.673	2371	2374	2379	rVB3	478	340	0.01%	0.002%
42	8.792	2399	2411	2437	rBV	332101	551917	12.30%	3.793%
43	8.956	2456	2462	2469	rBV5	1980	2709	0.06%	0.019%
44	9.011	2476	2479	2483	rVB4	576	348	0.01%	0.002%
45	9.085	2494	2502	2514	rBV4	5109	8663	0.19%	0.060%
46	9.403	2595	2601	2603	rBV3	284	330	0.01%	0.002%
47	9.490	2619	2628	2643	rBV3	9133	14548	0.32%	0.100%
48	9.644	2669	2676	2682	rBV4	983	1381	0.03%	0.009%
49	9.712	2694	2697	2700	rBV2	431	355	0.01%	0.002%
50	9.844	2735	2738	2741	rVV	347	333	0.01%	0.002%
51	9.869	2741	2746	2758	rVB4	1273	1987	0.04%	0.014%
52	10.159	2822	2836	2853	rBV	282351	442489	9.86%	3.041%
53	10.297	2871	2879	2884	rBV3	2454	3491	0.08%	0.024%
54	10.329	2886	2889	2899	rVB4	2430	2842	0.06%	0.020%
55	10.394	2901	2909	2915	rBV3	4319	6511	0.15%	0.045%
56	10.487	2931	2938	2945	rBV5	3075	4249	0.09%	0.029%
57	10.683	2990	2999	3008	rBV3	4015	5423	0.12%	0.037%
58	10.805	3032	3037	3043	rVB4	867	1172	0.03%	0.008%
59	10.860	3043	3054	3069	rBV2	17800	26932	0.60%	0.185%
60	10.998	3090	3097	3099	rBV3	1038	1125	0.03%	0.008%
61	11.037	3101	3109	3115	rVB2	3517	5001	0.11%	0.034%
62	11.133	3131	3139	3140	rBV3	1203	1015	0.02%	0.007%
63	11.191	3146	3157	3172	rBV	355078	536696	11.96%	3.689%
64	11.281	3178	3185	3197	rVB	8866	13466	0.30%	0.093%
65	11.329	3197	3200	3202	rVB2	646	333	0.01%	0.002%
66	11.435	3228	3233	3238	rBV4	351	354	0.01%	0.002%
67	11.477	3238	3246	3254	rBV7	5507	8908	0.20%	0.061%
68	11.567	3263	3274	3296	rVV	381677	603011	13.44%	4.144%
69	11.644	3296	3298	3302	rVB2	706	491	0.01%	0.003%
70	11.686	3307	3311	3316	rVB5	725	749	0.02%	0.005%
71	11.770	3332	3337	3340	rBV4	740	617	0.01%	0.004%
72	11.812	3347	3350	3353	rBV3	403	326	0.01%	0.002%
73	11.866	3359	3367	3381	rVB6	5768	10611	0.24%	0.073%
74	11.940	3383	3390	3393	rBV7	2121	2822	0.06%	0.019%
75	12.062	3417	3428	3430	rBV5	2019	2752	0.06%	0.019%
76	12.078	3431	3433	3441	rVV4	2882	3851	0.09%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031529.D
 Acq On : 15 Jun 2023 14:27
 Operator : SY/MD
 Sample : 03249-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.111	3441	3443	3446	rVB3	625	369	0.01%	0.003%
78	12.201	3465	3471	3479	rVB4	1282	1996	0.04%	0.014%
79	12.413	3532	3537	3545	rVB7	1295	1675	0.04%	0.012%
80	12.590	3588	3592	3595	rBV	966	879	0.02%	0.006%
81	12.635	3600	3606	3612	rVB5	668	858	0.02%	0.006%
82	12.670	3612	3617	3620	rBV3	297	340	0.01%	0.002%
83	12.799	3653	3657	3659	rBV3	490	369	0.01%	0.003%
84	12.828	3659	3666	3675	rVB7	2259	3391	0.08%	0.023%
85	12.898	3678	3688	3693	rBV4	1455	2188	0.05%	0.015%
86	12.956	3701	3706	3709	rBV2	568	487	0.01%	0.003%
87	12.988	3712	3716	3723	rVB5	1183	1516	0.03%	0.010%
88	13.210	3780	3785	3792	rVB4	1055	1284	0.03%	0.009%
89	13.297	3808	3812	3815	rBV2	436	321	0.01%	0.002%
90	13.371	3832	3835	3841	rBV3	348	401	0.01%	0.003%
91	13.451	3848	3860	3874	rBV	9405	16697	0.37%	0.115%
92	13.512	3876	3879	3886	rVB5	382	365	0.01%	0.003%
93	13.692	3930	3935	3936	rBV	762	582	0.01%	0.004%
94	13.837	3977	3980	3984	rBV2	406	308	0.01%	0.002%
95	14.104	4058	4063	4064	rBV2	500	419	0.01%	0.003%
96	14.139	4070	4074	4077	rBV3	357	329	0.01%	0.002%
97	14.577	4205	4210	4213	rBV4	2296	2279	0.05%	0.016%
98	14.699	4245	4248	4251	rBV2	499	337	0.01%	0.002%
99	14.969	4329	4332	4334	rBV3	611	398	0.01%	0.003%
100	15.760	4575	4578	4583	rBV2	824	1003	0.02%	0.007%




Sum of corrected areas: 14549858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031529.D
Acq On : 15 Jun 2023 14:27
Operator : SY/MD
Sample : 03249-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

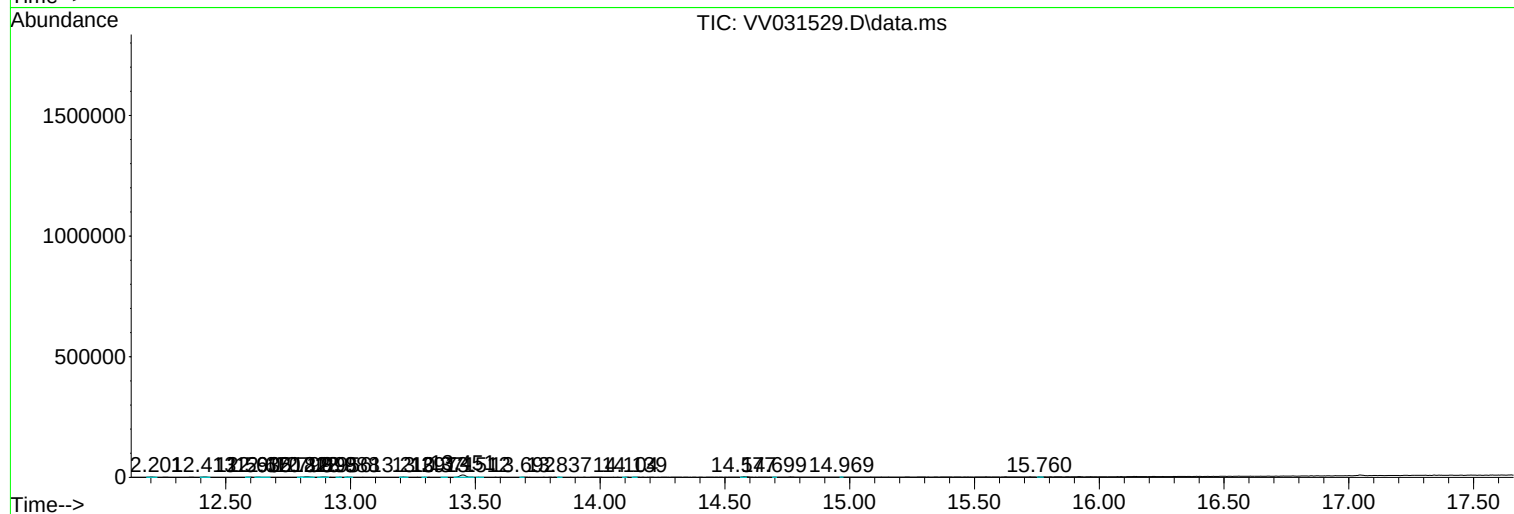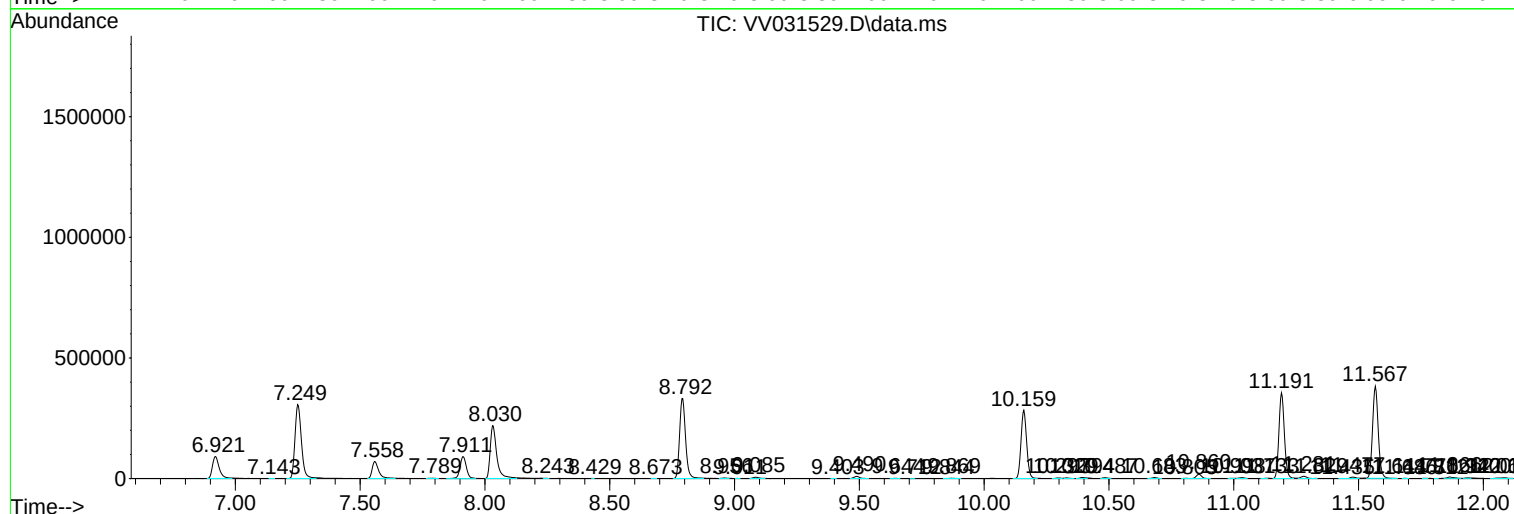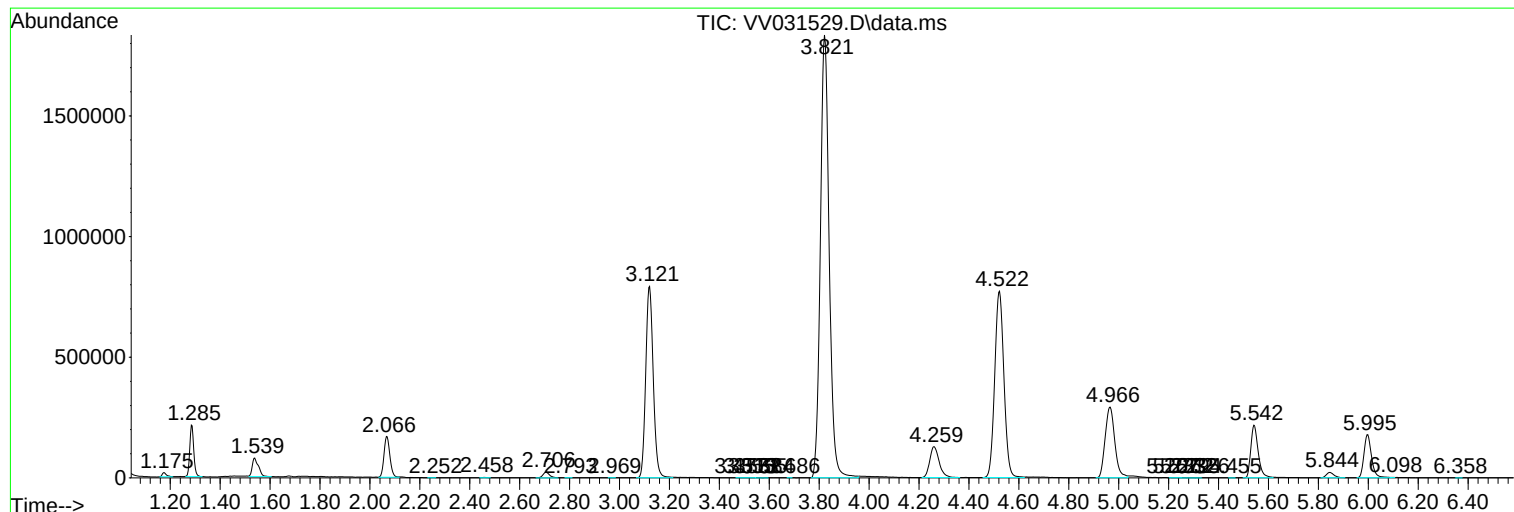

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031529.D
Acq On : 15 Jun 2023 14:27
Operator : SY/MD
Sample : 03249-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031529.D
Acq On : 15 Jun 2023 14:27
Operator : SY/MD
Sample : 03249-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc