

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031533.D
 Acq On : 15 Jun 2023 16:00
 Operator : SY/MD
 Sample : 03249-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	55	rBV	13240	18255	2.00%	0.242%
2	1.282	69	75	86	rBV	95254	99653	10.94%	1.322%
3	1.539	148	155	170	rVB	91930	112793	12.38%	1.497%
4	2.066	310	319	334	rVB	191428	282226	30.99%	3.745%
5	2.452	432	439	442	rBV4	812	816	0.09%	0.011%
6	2.671	503	507	511	rBV2	345	327	0.04%	0.004%
7	2.712	511	520	531	rVB8	1865	3641	0.40%	0.048%
8	2.754	531	533	534	rBV	120	46	0.01%	0.001%
9	2.767	534	537	541	rBV2	208	168	0.02%	0.002%
10	2.819	550	553	556	rBV2	232	169	0.02%	0.002%
11	2.973	599	601	603	rBV	249	98	0.01%	0.001%
12	3.040	620	622	624	rBV	181	123	0.01%	0.002%
13	3.124	633	648	663	rBV2	25997	55165	6.06%	0.732%
14	3.227	677	680	684	rVB2	220	163	0.02%	0.002%
15	3.291	698	700	703	rVB	224	97	0.01%	0.001%
16	3.401	732	734	738	rVB2	283	162	0.02%	0.002%
17	3.433	740	744	748	rBV2	205	193	0.02%	0.003%
18	3.455	748	751	755	rBV	194	231	0.03%	0.003%
19	3.474	755	757	758	rBV	192	88	0.01%	0.001%
20	3.510	766	768	771	rBV	150	84	0.01%	0.001%
21	3.536	775	776	777	rBV	97	25	0.00%	0.000%
22	3.555	780	782	784	rBV	161	56	0.01%	0.001%
23	3.610	797	799	801	rBV2	171	98	0.01%	0.001%
24	3.683	819	822	825	rVB2	144	96	0.01%	0.001%
25	3.706	825	829	834	rVB2	268	258	0.03%	0.003%
26	3.732	834	837	840	rBV	221	142	0.02%	0.002%
27	3.757	841	845	848	rBV2	228	230	0.03%	0.003%
28	3.806	849	860	900	rBV4	72508	248804	27.32%	3.302%
29	4.259	985	1001	1028	rBV	151002	393860	43.25%	5.226%
30	4.523	1068	1083	1105	rVB3	86187	221545	24.33%	2.940%
31	4.719	1142	1144	1146	rBV	215	114	0.01%	0.002%
32	4.732	1146	1148	1154	rVB	307	245	0.03%	0.003%
33	4.757	1154	1156	1157	rBV	370	141	0.02%	0.002%
34	4.793	1165	1167	1169	rBV	217	110	0.01%	0.001%
35	4.873	1188	1192	1196	rVB2	188	171	0.02%	0.002%
36	4.896	1196	1199	1201	rBV2	191	132	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031533.D
 Acq On : 15 Jun 2023 16:00
 Operator : SY/MD
 Sample : 03249-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	4.966	1204	1221	1249	rBV2	343260	910742	100.00%	12.085%
38	5.230	1301	1303	1305	rBV	254	120	0.01%	0.002%
39	5.320	1328	1331	1332	rBV	278	117	0.01%	0.002%
40	5.375	1345	1348	1352	rBV2	255	253	0.03%	0.003%
41	5.407	1355	1358	1361	rBV2	213	167	0.02%	0.002%
42	5.439	1366	1368	1369	rBV2	285	137	0.02%	0.002%
43	5.542	1388	1400	1424	rBV	298792	606291	66.57%	8.045%
44	5.847	1482	1495	1510	rBV7	8156	18429	2.02%	0.245%
45	5.934	1517	1522	1525	rVB	382	302	0.03%	0.004%
46	5.995	1526	1541	1565	rBV	209513	438447	48.14%	5.818%
47	6.307	1633	1638	1639	rBV	204	147	0.02%	0.002%
48	6.336	1644	1647	1649	rBV2	344	207	0.02%	0.003%
49	6.394	1663	1665	1666	rBV2	131	43	0.00%	0.001%
50	6.568	1716	1719	1720	rBV2	218	139	0.02%	0.002%
51	6.677	1748	1753	1756	rBV2	214	182	0.02%	0.002%
52	6.696	1756	1759	1763	rVB2	171	110	0.01%	0.001%
53	6.722	1763	1767	1769	rBV	170	130	0.01%	0.002%
54	6.738	1769	1772	1775	rBV2	225	177	0.02%	0.002%
55	6.812	1790	1795	1797	rBV3	181	158	0.02%	0.002%
56	6.841	1802	1804	1805	rBV2	134	33	0.00%	0.000%
57	6.851	1805	1807	1810	rBV	165	93	0.01%	0.001%
58	6.921	1818	1829	1851	rBV	105439	198296	21.77%	2.631%
59	7.249	1920	1931	1966	rBV	372044	661086	72.59%	8.772%
60	7.558	2017	2027	2044	rBV2	79245	140440	15.42%	1.864%
61	7.809	2102	2105	2109	rBV	250	185	0.02%	0.002%
62	7.912	2119	2137	2152	rBV3	27373	49997	5.49%	0.663%
63	7.986	2156	2160	2162	rBV2	128	90	0.01%	0.001%
64	8.031	2162	2174	2200	rBV	231313	419144	46.02%	5.562%
65	8.426	2296	2297	2299	rBV	233	101	0.01%	0.001%
66	8.555	2333	2337	2338	rBV	205	121	0.01%	0.002%
67	8.577	2342	2344	2347	rBV	307	199	0.02%	0.003%
68	8.596	2347	2350	2352	rBV2	282	179	0.02%	0.002%
69	8.648	2364	2366	2367	rBV	147	62	0.01%	0.001%
70	8.674	2371	2374	2378	rVV2	241	192	0.02%	0.003%
71	8.789	2399	2410	2429	rBV	447962	730887	80.25%	9.699%
72	9.005	2475	2477	2479	rBV	286	142	0.02%	0.002%
73	9.085	2497	2502	2503	rBV2	746	576	0.06%	0.008%
74	9.220	2541	2544	2550	rVB4	539	524	0.06%	0.007%
75	9.262	2550	2557	2561	rBV3	492	624	0.07%	0.008%
76	9.317	2571	2574	2577	rBV	266	208	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031533.D
 Acq On : 15 Jun 2023 16:00
 Operator : SY/MD
 Sample : 03249-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.445	2610	2614	2620	rBV	342	342	0.04%	0.005%
78	9.494	2626	2629	2634	rVB2	684	516	0.06%	0.007%
79	9.709	2693	2696	2699	rBV2	303	217	0.02%	0.003%
80	9.780	2713	2718	2720	rBV	283	232	0.03%	0.003%
81	9.879	2745	2749	2754	rBV3	313	320	0.04%	0.004%
82	9.966	2773	2776	2782	rBV	279	231	0.03%	0.003%
83	10.104	2815	2819	2823	rVB2	384	303	0.03%	0.004%
84	10.159	2823	2836	2859	rBV	317457	499906	54.89%	6.634%
85	10.551	2955	2958	2962	rBV	252	154	0.02%	0.002%
86	10.657	2989	2991	2993	rBV2	222	116	0.01%	0.002%
87	10.825	3041	3043	3044	rBV	209	114	0.01%	0.002%
88	10.940	3075	3079	3080	rBV	225	158	0.02%	0.002%
89	11.008	3097	3100	3101	rBV	250	127	0.01%	0.002%
90	11.095	3124	3127	3130	rBV2	294	174	0.02%	0.002%
91	11.191	3146	3157	3179	rBV	473507	723089	79.40%	9.595%
92	11.567	3262	3274	3290	rBV	443786	685729	75.29%	9.099%
93	11.870	3361	3368	3376	rBV5	1325	1886	0.21%	0.025%
94	12.191	3462	3468	3479	rBV4	1212	2119	0.23%	0.028%
95	13.095	3747	3749	3750	rBV4	217	73	0.01%	0.001%
96	13.686	3932	3933	3934	rBV4	336	107	0.01%	0.001%




Sum of corrected areas: 7535915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031533.D
Acq On : 15 Jun 2023 16:00
Operator : SY/MD
Sample : 03249-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

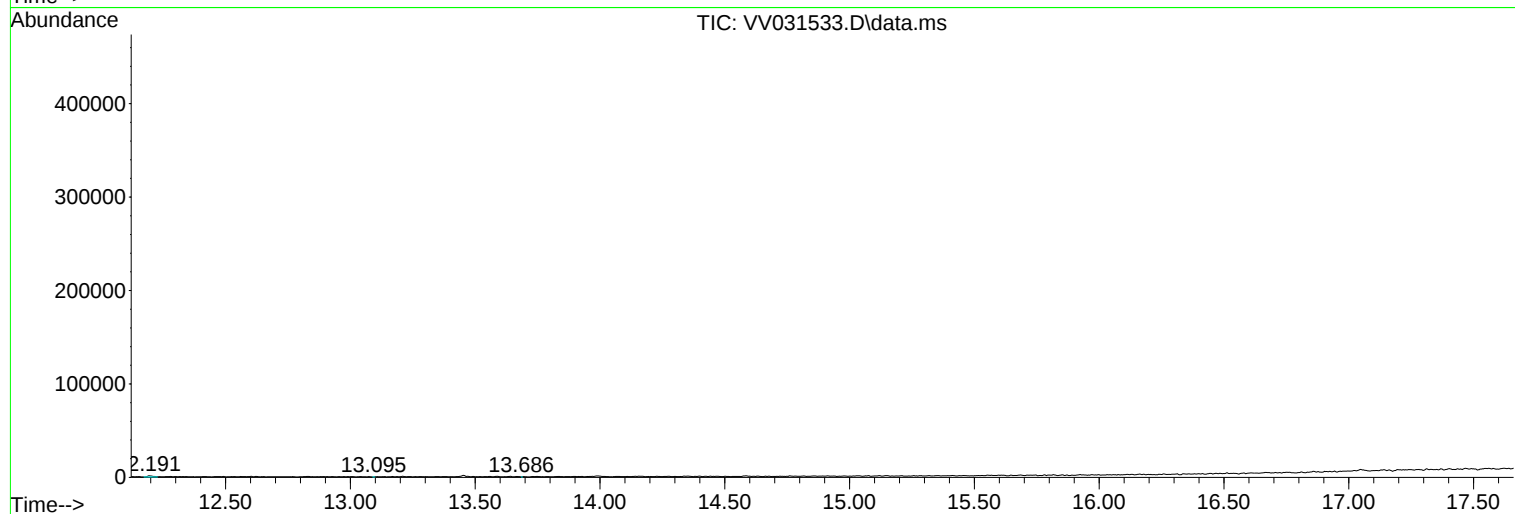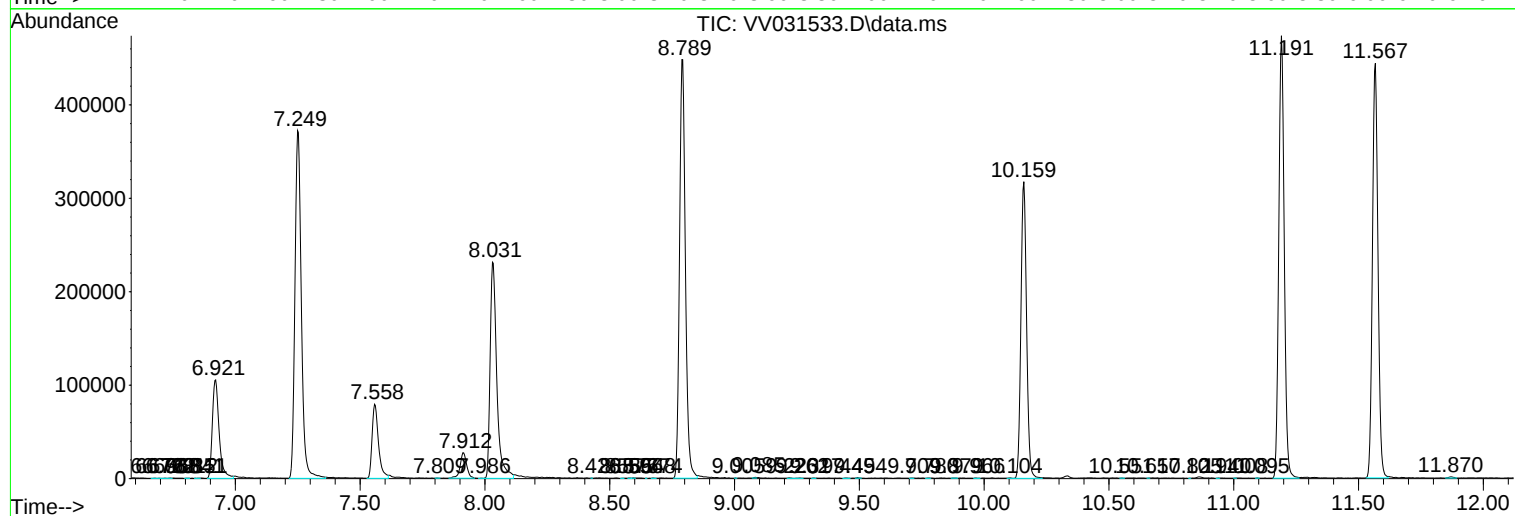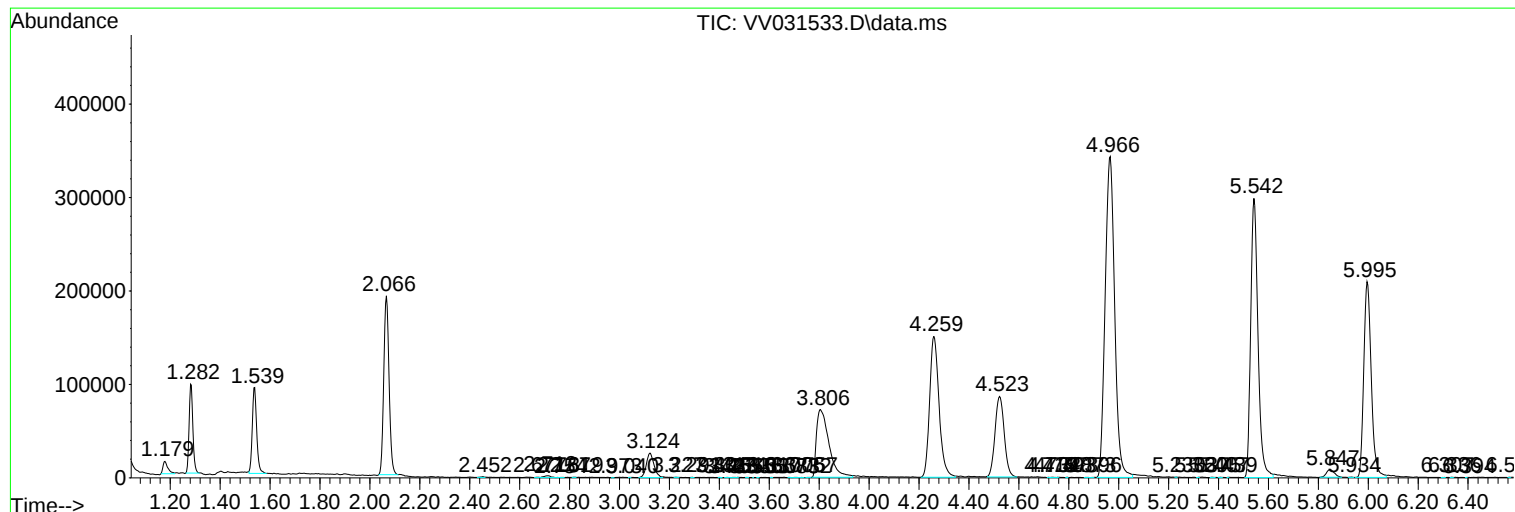

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031533.D
Acq On : 15 Jun 2023 16:00
Operator : SY/MD
Sample : 03249-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031533.D
Acq On : 15 Jun 2023 16:00
Operator : SY/MD
Sample : 03249-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------