

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031535.D
 Acq On : 15 Jun 2023 16:46
 Operator : SY/MD
 Sample : 03249-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	38	42	54	rBV	10901	14499	0.34%	0.099%
2	1.285	70	76	87	rVB2	107282	116973	2.76%	0.799%
3	1.532	148	153	167	rVB	76378	93441	2.20%	0.638%
4	2.066	309	319	335	rBV3	177129	288249	6.79%	1.969%
5	2.461	434	442	447	rBV5	1261	1614	0.04%	0.011%
6	2.706	508	518	532	rVB2	15541	27650	0.65%	0.189%
7	2.847	560	562	563	rBV2	258	108	0.00%	0.001%
8	2.963	595	598	599	rBV2	370	155	0.00%	0.001%
9	2.992	604	607	609	rBV	302	220	0.01%	0.002%
10	3.047	621	624	627	rBV	301	189	0.00%	0.001%
11	3.060	627	628	629	rBV	160	42	0.00%	0.000%
12	3.121	629	647	674	rBV	1003815	2116345	49.86%	14.460%
13	3.497	761	764	767	rVB2	388	222	0.01%	0.002%
14	3.561	781	784	787	rVB3	448	250	0.01%	0.002%
15	3.574	787	788	793	rVB2	180	127	0.00%	0.001%
16	3.600	793	796	801	rBV	431	318	0.01%	0.002%
17	3.638	801	808	810	rBV3	311	421	0.01%	0.003%
18	3.732	834	837	844	rVB3	326	344	0.01%	0.002%
19	3.822	847	865	902	rBV	1741559	4244207	100.00%	28.998%
20	4.259	987	1001	1036	rVB	122707	321060	7.56%	2.194%
21	4.522	1064	1083	1107	rBV	881855	2249884	53.01%	15.372%
22	4.860	1185	1188	1191	rBV2	481	328	0.01%	0.002%
23	4.899	1198	1200	1203	rBV	319	257	0.01%	0.002%
24	4.966	1204	1221	1265	rVV2	284906	772069	18.19%	5.275%
25	5.436	1365	1367	1370	rVB2	192	54	0.00%	0.000%
26	5.542	1388	1400	1424	rBV2	229603	474004	11.17%	3.239%
27	5.764	1467	1469	1470	rBV2	411	162	0.00%	0.001%
28	5.844	1485	1494	1512	rBV7	13394	28386	0.67%	0.194%
29	5.937	1520	1523	1528	rBV2	290	254	0.01%	0.002%
30	5.995	1528	1541	1566	rBV	170641	356244	8.39%	2.434%
31	6.188	1599	1601	1602	rBV	183	70	0.00%	0.000%
32	6.320	1637	1642	1644	rBV2	315	251	0.01%	0.002%
33	6.336	1644	1647	1651	rBV2	398	351	0.01%	0.002%
34	6.407	1664	1669	1671	rBV2	280	317	0.01%	0.002%
35	6.461	1682	1686	1690	rVB3	338	303	0.01%	0.002%
36	6.481	1690	1692	1694	rBV	106	57	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031535.D
 Acq On : 15 Jun 2023 16:46
 Operator : SY/MD
 Sample : 03249-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.641	1739	1742	1746	rBV	172	117	0.00%	0.001%
38	6.680	1752	1754	1756	rBV2	191	77	0.00%	0.001%
39	6.731	1767	1770	1773	rBV2	261	154	0.00%	0.001%
40	6.760	1773	1779	1780	rBV2	332	288	0.01%	0.002%
41	6.818	1792	1797	1799	rBV2	317	374	0.01%	0.003%
42	6.921	1818	1829	1857	rBV	87995	167696	3.95%	1.146%
43	7.120	1888	1891	1894	rBV4	533	425	0.01%	0.003%
44	7.188	1910	1912	1916	rVB3	523	269	0.01%	0.002%
45	7.249	1920	1931	1951	rBV	294774	522681	12.32%	3.571%
46	7.503	2008	2010	2014	rBV	347	187	0.00%	0.001%
47	7.558	2015	2027	2049	rBV2	76666	145931	3.44%	0.997%
48	7.915	2121	2138	2154	rVB3	41515	77586	1.83%	0.530%
49	8.034	2164	2175	2199	rBV	217839	389219	9.17%	2.659%
50	8.410	2289	2292	2295	rBV2	487	360	0.01%	0.002%
51	8.468	2308	2310	2311	rBV	240	136	0.00%	0.001%
52	8.641	2359	2364	2369	rBV4	499	529	0.01%	0.004%
53	8.706	2379	2384	2386	rBV	424	382	0.01%	0.003%
54	8.744	2394	2396	2400	rBV2	295	217	0.01%	0.001%
55	8.792	2400	2411	2435	rBV	354455	584270	13.77%	3.992%
56	9.082	2493	2501	2502	rBV3	4111	3418	0.08%	0.023%
57	9.278	2558	2562	2566	rBV3	241	311	0.01%	0.002%
58	9.490	2618	2628	2639	rBV4	7344	11155	0.26%	0.076%
59	9.554	2645	2648	2654	rVB2	571	502	0.01%	0.003%
60	9.587	2655	2658	2659	rBV2	179	106	0.00%	0.001%
61	9.625	2667	2670	2671	rBV	234	107	0.00%	0.001%
62	9.844	2734	2738	2741	rBV3	349	264	0.01%	0.002%
63	9.873	2741	2747	2749	rBV3	759	762	0.02%	0.005%
64	9.886	2749	2751	2753	rVB	409	150	0.00%	0.001%
65	10.062	2802	2806	2813	rBV3	335	405	0.01%	0.003%
66	10.095	2813	2816	2819	rBV	310	207	0.00%	0.001%
67	10.159	2824	2836	2865	rBV	278613	432174	10.18%	2.953%
68	10.300	2869	2880	2883	rBV3	1746	2338	0.06%	0.016%
69	10.394	2902	2909	2916	rBV5	3067	5245	0.12%	0.036%
70	10.487	2931	2938	2945	rVB4	2553	3112	0.07%	0.021%
71	10.551	2957	2958	2959	rBV4	236	60	0.00%	0.000%
72	10.651	2985	2989	2990	rBV	201	144	0.00%	0.001%
73	10.683	2993	2999	3007	rVV6	2726	3710	0.09%	0.025%
74	10.860	3045	3054	3069	rBV	14550	21528	0.51%	0.147%
75	11.072	3117	3120	3125	rBV2	407	414	0.01%	0.003%
76	11.191	3146	3157	3175	rBV	368531	559626	13.19%	3.824%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031535.D
 Acq On : 15 Jun 2023 16:46
 Operator : SY/MD
 Sample : 03249-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.477	3239	3246	3256	rVB8	4682	7271	0.17%	0.050%
78	11.567	3262	3274	3293	rBV	356600	548626	12.93%	3.748%
79	11.866	3359	3367	3380	rBV4	7439	12394	0.29%	0.085%
80	12.117	3443	3445	3449	rBV2	268	174	0.00%	0.001%
81	12.406	3531	3535	3537	rBV2	898	729	0.02%	0.005%
82	12.538	3573	3576	3579	rBV	426	379	0.01%	0.003%
83	12.937	3698	3700	3705	rVB	275	173	0.00%	0.001%
84	12.966	3705	3709	3713	rBV3	516	431	0.01%	0.003%
85	13.033	3725	3730	3734	rBV2	323	406	0.01%	0.003%
86	13.384	3838	3839	3840	rBV	344	77	0.00%	0.001%
87	13.448	3850	3859	3869	rBV2	8587	13165	0.31%	0.090%
88	13.590	3900	3903	3906	rBV2	462	326	0.01%	0.002%
89	13.754	3952	3954	3958	rBV2	513	310	0.01%	0.002%
90	13.815	3972	3973	3976	rBV	370	244	0.01%	0.002%
91	13.857	3983	3986	3990	rBV2	410	436	0.01%	0.003%
92	13.927	4005	4008	4009	rBV2	394	221	0.01%	0.002%
93	14.178	4084	4086	4087	rBV	430	198	0.00%	0.001%
94	14.583	4205	4212	4225	rBV4	2678	4294	0.10%	0.029%
95	14.815	4281	4284	4285	rBV	624	361	0.01%	0.002%




Sum of corrected areas: 14636276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031535.D
Acq On : 15 Jun 2023 16:46
Operator : SY/MD
Sample : 03249-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

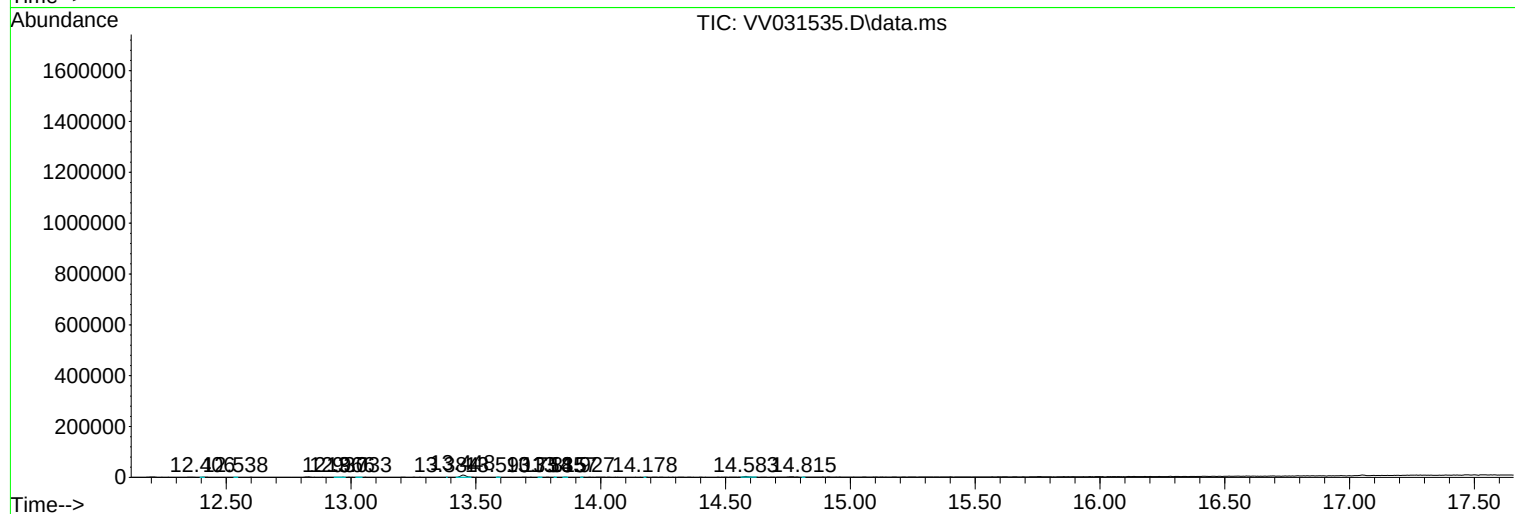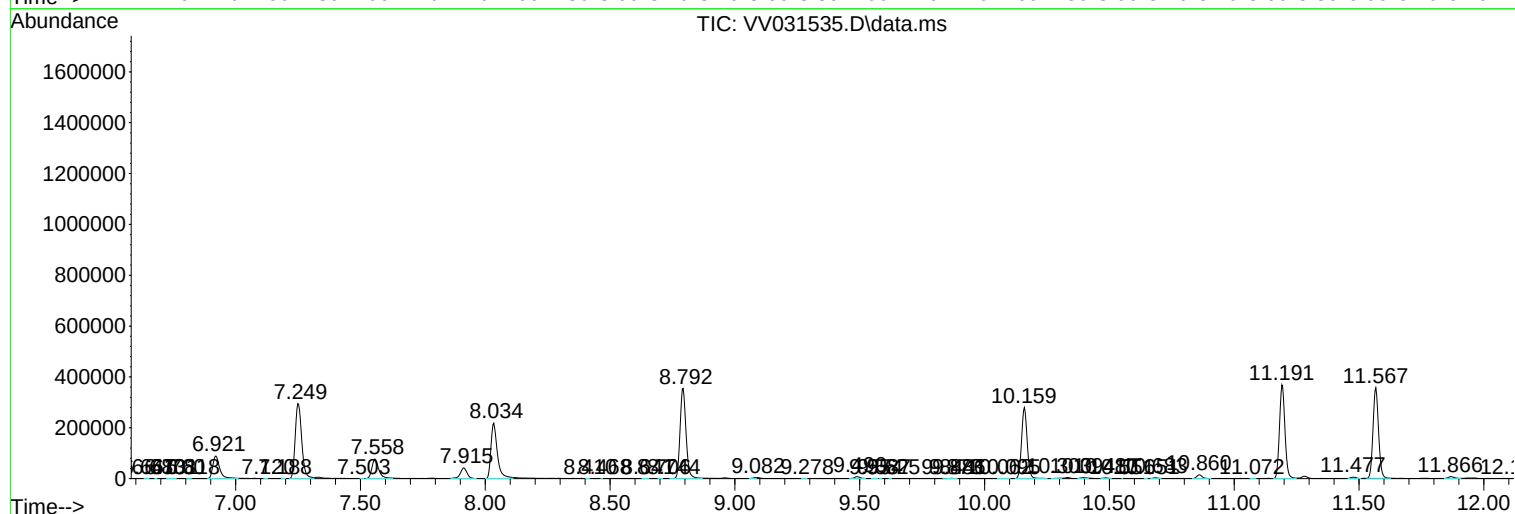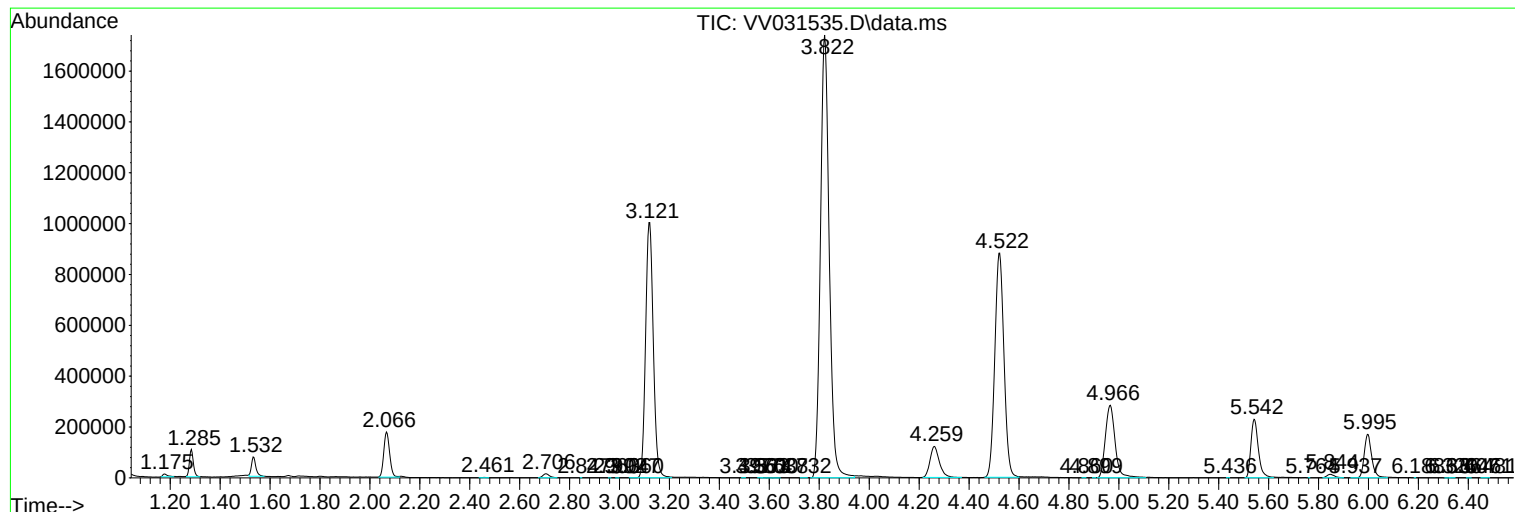

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031535.D
Acq On : 15 Jun 2023 16:46
Operator : SY/MD
Sample : 03249-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031535.D
Acq On : 15 Jun 2023 16:46
Operator : SY/MD
Sample : 03249-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------