

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031538.D
 Acq On : 15 Jun 2023 17:56
 Operator : SY/MD
 Sample : 03249-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	88	rVB	75874	82128	4.04%	0.865%
2	1.536	148	154	167	rVB	77030	91096	4.49%	0.959%
3	2.066	310	319	334	rBV2	178585	279534	13.77%	2.943%
4	2.391	418	420	422	rBV	358	185	0.01%	0.002%
5	2.458	436	441	450	rVB4	1424	1843	0.09%	0.019%
6	2.510	454	457	459	rBV	172	120	0.01%	0.001%
7	2.526	460	462	465	rBV3	332	199	0.01%	0.002%
8	2.610	485	488	492	rBV	259	215	0.01%	0.002%
9	2.706	514	518	523	rBV2	1538	1538	0.08%	0.016%
10	2.774	537	539	541	rBV	112	76	0.00%	0.001%
11	2.925	583	586	590	rBV2	158	168	0.01%	0.002%
12	2.970	598	600	602	rVB	347	178	0.01%	0.002%
13	2.986	602	605	610	rBV3	327	246	0.01%	0.003%
14	3.018	610	615	618	rBV2	267	286	0.01%	0.003%
15	3.121	633	647	673	rBV3	39062	81812	4.03%	0.861%
16	3.249	683	687	694	rBB3	298	345	0.02%	0.004%
17	3.288	694	699	702	rBV4	333	321	0.02%	0.003%
18	3.336	708	714	721	rBV3	512	578	0.03%	0.006%
19	3.471	753	756	759	rBV3	253	193	0.01%	0.002%
20	3.494	760	763	764	rBV2	144	87	0.00%	0.001%
21	3.565	781	785	788	rBV2	312	267	0.01%	0.003%
22	3.626	801	804	808	rVB2	328	227	0.01%	0.002%
23	3.645	808	810	811	rBV2	270	110	0.01%	0.001%
24	3.741	839	840	843	rBV	221	75	0.00%	0.001%
25	3.819	846	864	901	rBV3	98581	334990	16.50%	3.527%
26	4.259	985	1001	1034	rBV	125390	332745	16.39%	3.504%
27	4.523	1064	1083	1114	rBV	791946	2030687	100.00%	21.381%
28	4.966	1203	1221	1246	rBV2	291942	778192	38.32%	8.194%
29	5.253	1308	1310	1314	rVB3	404	169	0.01%	0.002%
30	5.272	1314	1316	1319	rVB2	338	173	0.01%	0.002%
31	5.452	1368	1372	1374	rBV2	266	181	0.01%	0.002%
32	5.542	1386	1400	1429	rBV	239399	493654	24.31%	5.198%
33	5.841	1481	1493	1515	rBV2	110574	229342	11.29%	2.415%
34	5.995	1528	1541	1564	rBV2	180802	372109	18.32%	3.918%
35	6.262	1622	1624	1628	rBV	206	128	0.01%	0.001%
36	6.346	1646	1650	1655	rVV3	352	303	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031538.D
 Acq On : 15 Jun 2023 17:56
 Operator : SY/MD
 Sample : 03249-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.371	1655	1658	1661	rBV2	286	202	0.01%	0.002%
38	6.400	1665	1667	1669	rBV	274	154	0.01%	0.002%
39	6.507	1697	1700	1702	rBV2	291	195	0.01%	0.002%
40	6.558	1712	1716	1719	rBV2	211	251	0.01%	0.003%
41	6.597	1725	1728	1729	rBV2	360	258	0.01%	0.003%
42	6.629	1735	1738	1744	rBV3	456	327	0.02%	0.003%
43	6.661	1744	1748	1750	rBV2	247	213	0.01%	0.002%
44	6.767	1777	1781	1784	rBV	388	339	0.02%	0.004%
45	6.802	1789	1792	1794	rBV2	302	195	0.01%	0.002%
46	6.921	1818	1829	1853	rBV	90849	171198	8.43%	1.803%
47	7.249	1920	1931	1954	rBV	313426	553409	27.25%	5.827%
48	7.461	1995	1997	2000	rBV3	355	147	0.01%	0.002%
49	7.500	2007	2009	2011	rBV2	207	108	0.01%	0.001%
50	7.561	2018	2028	2048	rBV	69196	123692	6.09%	1.302%
51	7.783	2091	2097	2106	rVB6	1490	2037	0.10%	0.021%
52	7.822	2106	2109	2110	rBV2	308	179	0.01%	0.002%
53	7.912	2118	2137	2164	rBV	506370	858731	42.29%	9.042%
54	8.034	2165	2175	2197	rBV	228064	402851	19.84%	4.242%
55	8.378	2280	2282	2283	rBV	332	134	0.01%	0.001%
56	8.461	2305	2308	2310	rBV3	203	121	0.01%	0.001%
57	8.523	2326	2327	2329	rBV	231	121	0.01%	0.001%
58	8.564	2338	2340	2341	rBV	278	136	0.01%	0.001%
59	8.580	2342	2345	2347	rVV	238	162	0.01%	0.002%
60	8.789	2399	2410	2438	rBV	363145	603309	29.71%	6.352%
61	9.085	2495	2502	2512	rBV5	3246	5441	0.27%	0.057%
62	9.278	2560	2562	2564	rBV	236	94	0.00%	0.001%
63	9.391	2594	2597	2601	rBV2	268	199	0.01%	0.002%
64	9.490	2622	2628	2638	rBV3	1421	2293	0.11%	0.024%
65	9.571	2651	2653	2655	rBV	198	124	0.01%	0.001%
66	9.638	2670	2674	2679	rBV2	352	342	0.02%	0.004%
67	9.661	2679	2681	2683	rVB2	213	90	0.00%	0.001%
68	9.686	2686	2689	2692	rBV3	261	272	0.01%	0.003%
69	9.744	2701	2707	2710	rBV	191	280	0.01%	0.003%
70	9.760	2710	2712	2715	rVB2	268	110	0.01%	0.001%
71	9.776	2715	2717	2722	rVB2	292	221	0.01%	0.002%
72	9.805	2722	2726	2728	rBV	134	111	0.01%	0.001%
73	9.908	2754	2758	2761	rBV3	328	215	0.01%	0.002%
74	9.937	2763	2767	2769	rVV2	203	148	0.01%	0.002%
75	10.030	2793	2796	2801	rVB3	316	264	0.01%	0.003%
76	10.101	2815	2818	2821	rBV3	384	216	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031538.D
 Acq On : 15 Jun 2023 17:56
 Operator : SY/MD
 Sample : 03249-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	10.159	2825	2836	2860	rVV	283112	441913	21.76%	4.653%
78	10.330	2874	2889	2900	rBV4	5592	9672	0.48%	0.102%
79	10.391	2903	2908	2913	rBV5	2145	2847	0.14%	0.030%
80	10.487	2930	2938	2946	rBV5	1444	2208	0.11%	0.023%
81	10.558	2957	2960	2966	rBV2	223	200	0.01%	0.002%
82	10.651	2986	2989	2991	rBV2	325	201	0.01%	0.002%
83	10.670	2992	2995	2996	rBV3	464	248	0.01%	0.003%
84	10.802	3034	3036	3039	rBV2	279	123	0.01%	0.001%
85	10.863	3044	3055	3065	rVB3	7162	10605	0.52%	0.112%
86	11.059	3114	3116	3118	rBV	302	151	0.01%	0.002%
87	11.104	3126	3130	3132	rBV3	391	283	0.01%	0.003%
88	11.191	3146	3157	3180	rBV	379524	574749	28.30%	6.052%
89	11.432	3229	3232	3235	rBV2	317	288	0.01%	0.003%
90	11.497	3245	3252	3263	rBV5	7553	14188	0.70%	0.149%
91	11.567	3264	3274	3296	rVB	379100	586717	28.89%	6.178%
92	11.690	3310	3312	3314	rBV2	603	276	0.01%	0.003%
93	11.870	3361	3368	3369	rBV3	1353	1437	0.07%	0.015%
94	11.937	3383	3389	3403	rVB9	1903	3091	0.15%	0.033%
95	12.931	3696	3698	3703	rBV2	459	345	0.02%	0.004%
96	13.056	3733	3737	3739	rBV2	407	359	0.02%	0.004%
97	13.194	3778	3780	3781	rBV2	343	101	0.00%	0.001%
98	13.407	3844	3846	3850	rBV2	412	267	0.01%	0.003%
99	13.452	3856	3860	3870	rVB4	2574	3614	0.18%	0.038%
100	13.860	3985	3987	3989	rBV	282	132	0.01%	0.001%




Sum of corrected areas: 9497404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031538.D
Acq On : 15 Jun 2023 17:56
Operator : SY/MD
Sample : 03249-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

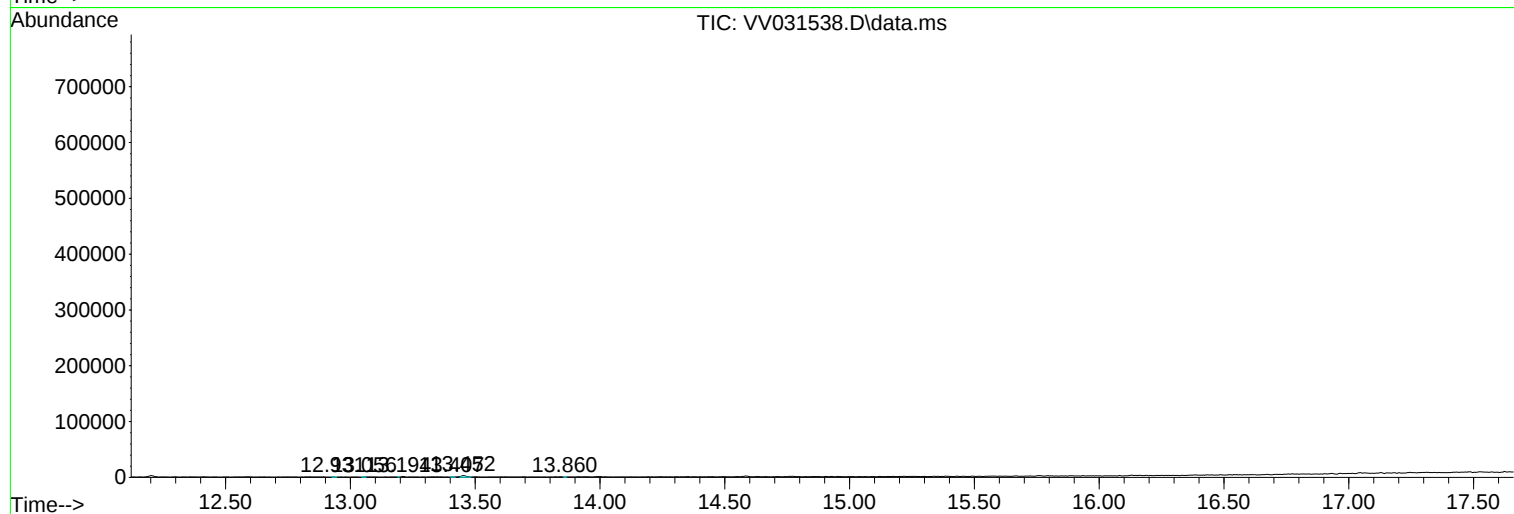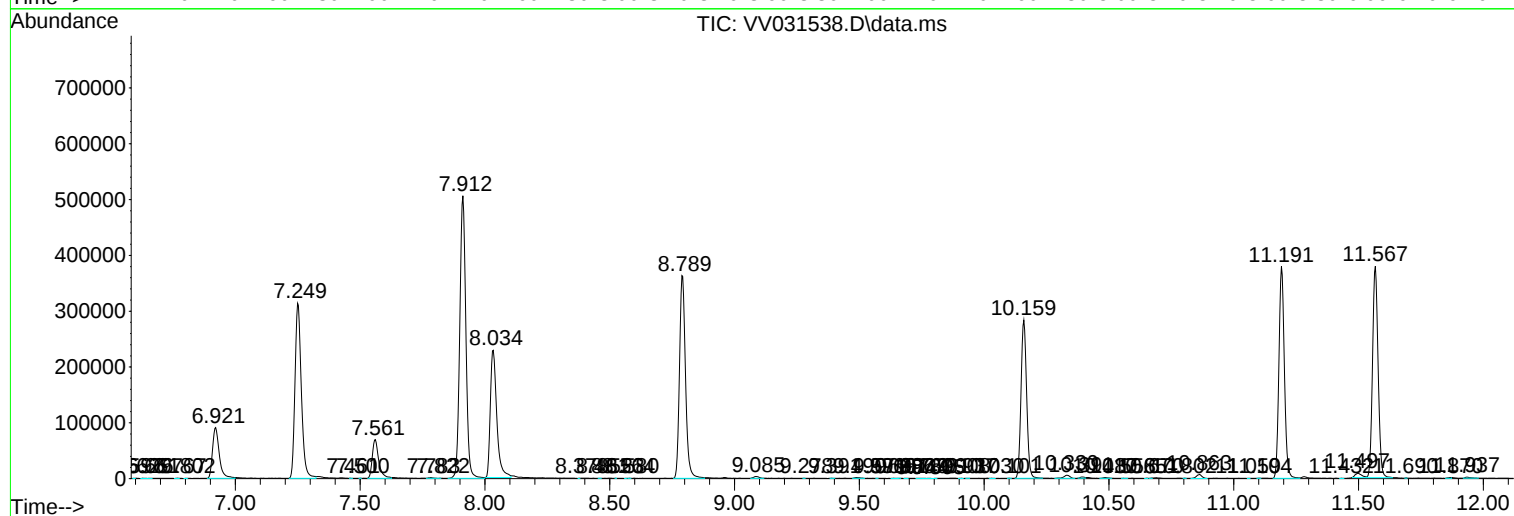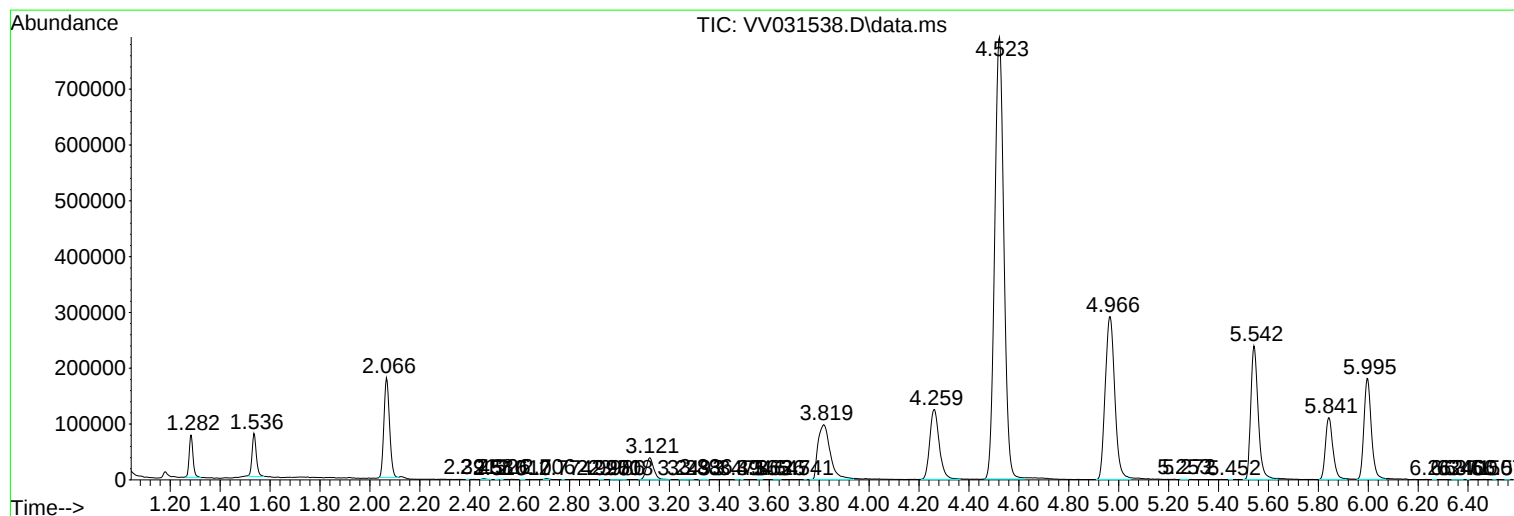

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031538.D
Acq On : 15 Jun 2023 17:56
Operator : SY/MD
Sample : 03249-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031538.D
Acq On : 15 Jun 2023 17:56
Operator : SY/MD
Sample : 03249-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------