

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031541.D
 Acq On : 15 Jun 2023 19:05
 Operator : SY/MD
 Sample : 03249-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	92	rVB	99065	105110	11.01%	1.236%
2	1.539	148	155	171	rVB	90320	111903	11.72%	1.316%
3	2.066	310	319	339	rVB2	207453	321104	33.64%	3.775%
4	2.455	435	440	448	rBV4	974	1186	0.12%	0.014%
5	2.661	503	504	508	rBV	199	136	0.01%	0.002%
6	2.706	508	518	533	rVV3	8806	16331	1.71%	0.192%
7	2.809	548	550	554	rVB	326	189	0.02%	0.002%
8	2.828	554	556	558	rBV	161	97	0.01%	0.001%
9	2.883	570	573	577	rVB2	211	156	0.02%	0.002%
10	2.908	578	581	583	rBV2	165	97	0.01%	0.001%
11	2.985	602	605	607	rBV	390	189	0.02%	0.002%
12	3.120	633	647	672	rBV	109976	231371	24.24%	2.720%
13	3.310	702	706	707	rBV	352	264	0.03%	0.003%
14	3.358	718	721	723	rBV2	280	163	0.02%	0.002%
15	3.465	751	754	755	rBV	162	87	0.01%	0.001%
16	3.619	801	802	806	rVB	199	105	0.01%	0.001%
17	3.648	809	811	813	rVV	191	77	0.01%	0.001%
18	3.670	816	818	822	rBV2	213	97	0.01%	0.001%
19	3.715	830	832	835	rBV2	154	83	0.01%	0.001%
20	3.809	849	861	888	rBV4	73833	246061	25.78%	2.893%
21	4.259	985	1001	1033	rBV	149642	394442	41.32%	4.637%
22	4.522	1065	1083	1109	rBV	373391	954496	100.00%	11.221%
23	4.821	1171	1176	1179	rBV2	274	272	0.03%	0.003%
24	4.899	1195	1200	1203	rBV2	401	416	0.04%	0.005%
25	4.966	1203	1221	1245	rBV2	343862	908856	95.22%	10.684%
26	5.255	1308	1311	1316	rBV3	268	198	0.02%	0.002%
27	5.419	1360	1362	1365	rBV2	306	202	0.02%	0.002%
28	5.455	1371	1373	1374	rBV2	383	120	0.01%	0.001%
29	5.542	1388	1400	1428	rBV	290396	596725	62.52%	7.015%
30	5.747	1461	1464	1466	rBV3	511	300	0.03%	0.004%
31	5.844	1484	1494	1509	rBV6	8882	18848	1.97%	0.222%
32	5.924	1516	1519	1522	rBV2	264	223	0.02%	0.003%
33	5.995	1528	1541	1564	rBV	209482	433037	45.37%	5.091%
34	6.407	1667	1669	1671	rBV	168	84	0.01%	0.001%
35	6.435	1675	1678	1680	rBV2	258	163	0.02%	0.002%
36	6.487	1691	1694	1698	rVB2	360	214	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031541.D
 Acq On : 15 Jun 2023 19:05
 Operator : SY/MD
 Sample : 03249-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.535	1707	1709	1710	rBV	135	33	0.00%	0.000%
38	6.628	1737	1738	1740	rBV	142	64	0.01%	0.001%
39	6.670	1749	1751	1754	rVB2	303	140	0.01%	0.002%
40	6.760	1778	1779	1781	rVB2	133	26	0.00%	0.000%
41	6.780	1781	1785	1788	rBV3	204	192	0.02%	0.002%
42	6.828	1798	1800	1802	rBV	112	53	0.01%	0.001%
43	6.921	1818	1829	1848	rBV2	104347	194553	20.38%	2.287%
44	7.207	1916	1918	1919	rBV2	283	140	0.01%	0.002%
45	7.249	1920	1931	1958	rVV	367146	656754	68.81%	7.721%
46	7.558	2017	2027	2051	rBV	81361	145584	15.25%	1.711%
47	7.783	2093	2097	2098	rBV2	1046	755	0.08%	0.009%
48	7.824	2109	2110	2113	rVB	344	87	0.01%	0.001%
49	7.915	2129	2138	2156	rVB3	69902	122639	12.85%	1.442%
50	8.033	2165	2175	2209	rBV	229985	423329	44.35%	4.977%
51	8.451	2304	2305	2308	rBV2	219	133	0.01%	0.002%
52	8.593	2347	2349	2350	rBV2	193	88	0.01%	0.001%
53	8.644	2361	2365	2367	rBV2	259	219	0.02%	0.003%
54	8.728	2389	2391	2397	rVB2	473	284	0.03%	0.003%
55	8.789	2399	2410	2442	rBV	439819	724603	75.91%	8.518%
56	9.095	2497	2505	2510	rBV4	920	1191	0.12%	0.014%
57	9.223	2543	2545	2547	rVB	148	39	0.00%	0.000%
58	9.239	2547	2550	2552	rBV3	297	183	0.02%	0.002%
59	9.310	2569	2572	2575	rVB2	237	122	0.01%	0.001%
60	9.445	2612	2614	2617	rBV	179	110	0.01%	0.001%
61	9.487	2624	2627	2628	rBV	437	241	0.03%	0.003%
62	9.619	2666	2668	2670	rBV	291	180	0.02%	0.002%
63	10.159	2824	2836	2854	rBV	313308	489777	51.31%	5.758%
64	10.329	2884	2889	2898	rVB5	3324	4636	0.49%	0.054%
65	10.484	2934	2937	2941	rBV2	396	325	0.03%	0.004%
66	10.631	2980	2983	2986	rBV	287	224	0.02%	0.003%
67	10.863	3048	3055	3066	rVB3	1420	2297	0.24%	0.027%
68	10.998	3094	3097	3101	rBV3	389	244	0.03%	0.003%
69	11.098	3126	3128	3130	rBV	207	104	0.01%	0.001%
70	11.152	3142	3145	3146	rBV	149	83	0.01%	0.001%
71	11.191	3146	3157	3181	rVV	460707	703165	73.67%	8.266%
72	11.500	3248	3253	3263	rBV6	2412	4646	0.49%	0.055%
73	11.567	3263	3274	3291	rVV	447075	682425	71.50%	8.022%
74	11.863	3364	3366	3369	rBV2	261	186	0.02%	0.002%
75	12.027	3411	3417	3422	rBV3	404	606	0.06%	0.007%
76	12.139	3448	3452	3456	rBV2	426	460	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031541.D
Acq On : 15 Jun 2023 19:05
Operator : SY/MD
Sample : 03249-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis

77	12.844	3668	3671	3675	rBV	454	317	0.03%	0.004%
78	13.075	3738	3743	3746	rBV2	408	429	0.04%	0.005%
79	13.593	3902	3904	3907	rBV	399	241	0.03%	0.003%
80	14.030	4036	4040	4046	rBV4	679	747	0.08%	0.009%
81	14.303	4122	4125	4128	rBV3	529	375	0.04%	0.004%




Sum of corrected areas: 8506431

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031541.D
Acq On : 15 Jun 2023 19:05
Operator : SY/MD
Sample : 03249-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

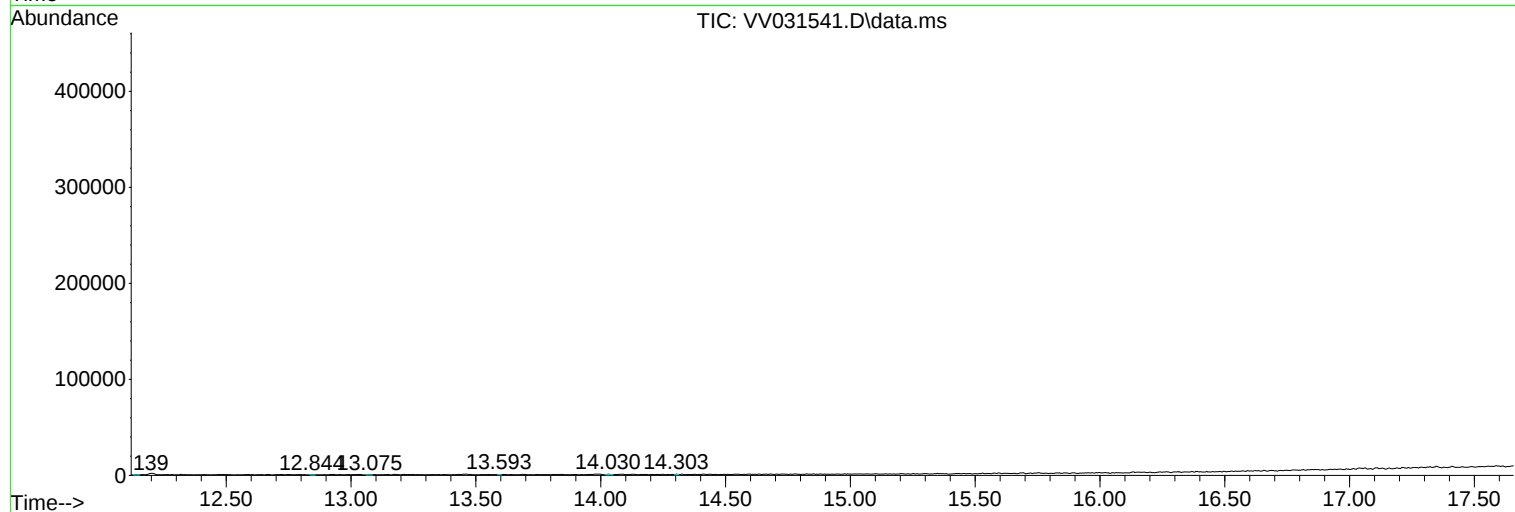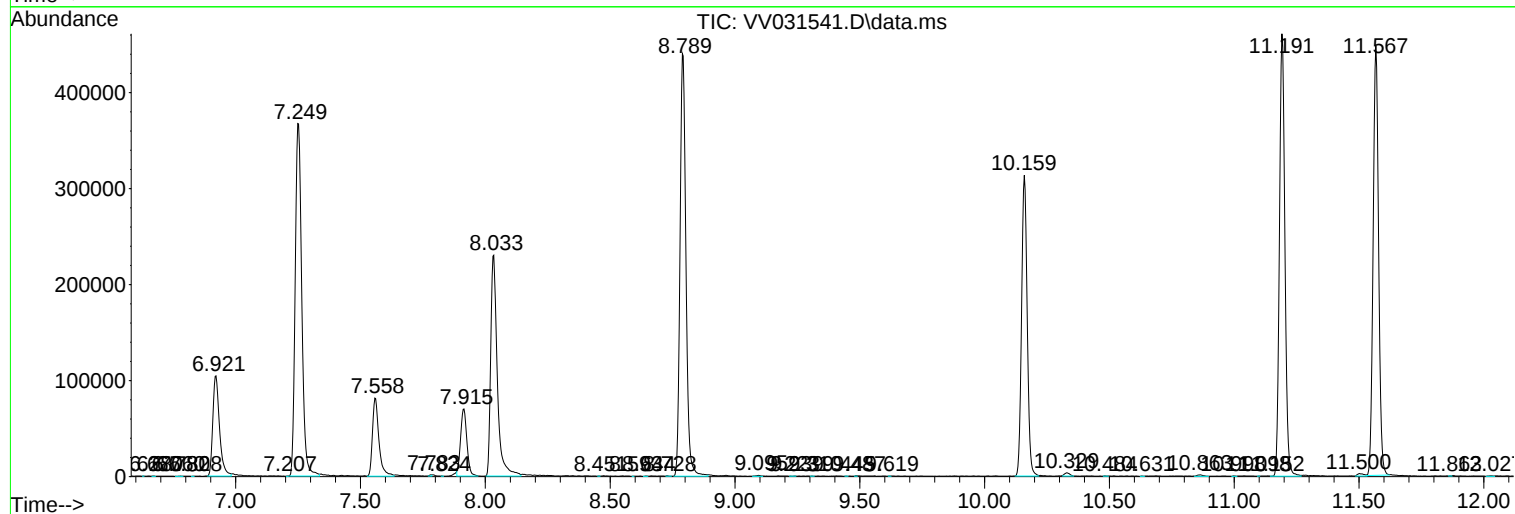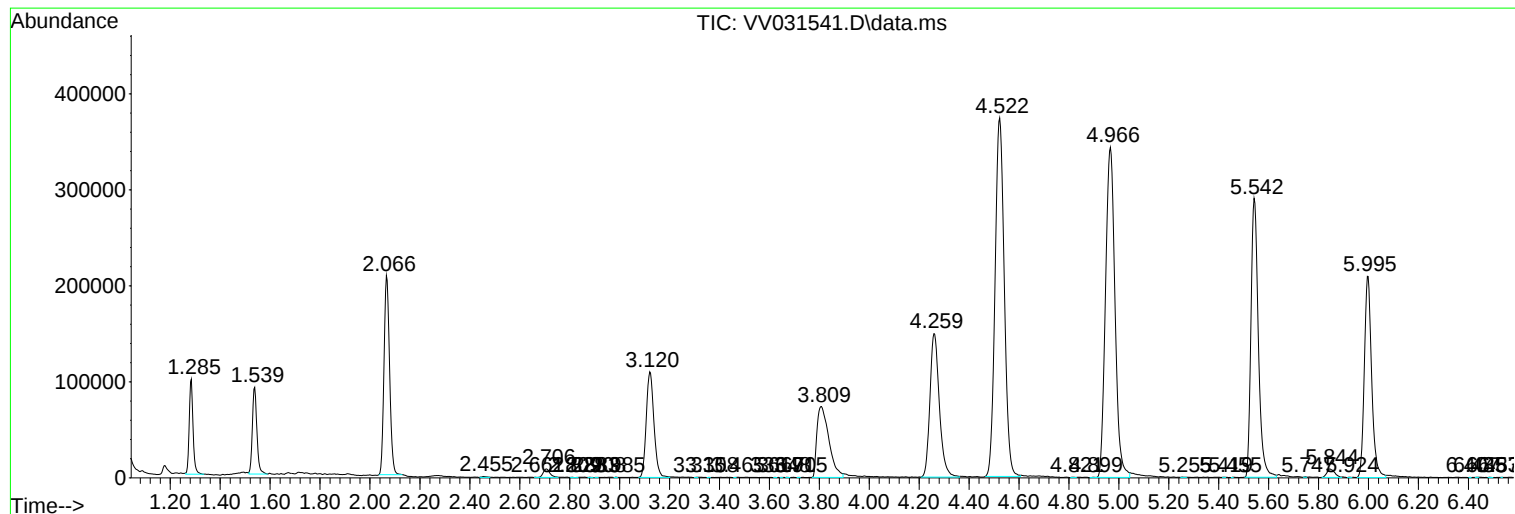

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031541.D
Acq On : 15 Jun 2023 19:05
Operator : SY/MD
Sample : 03249-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031541.D
Acq On : 15 Jun 2023 19:05
Operator : SY/MD
Sample : 03249-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------