

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031547.D
 Acq On : 15 Jun 2023 22:42
 Operator : SY/MD
 Sample : 03249-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	39	44	52	rBV	5072	6772	0.19%	0.041%
2	1.282	69	75	92	rVB	92582	98981	2.72%	0.605%
3	1.539	147	155	171	rVB	86754	105543	2.90%	0.646%
4	1.674	192	197	204	rBV	6935	7102	0.19%	0.043%
5	1.719	205	211	225	rVB2	12476	21029	0.58%	0.129%
6	2.076	309	322	347	rBV3	869186	1375293	37.76%	8.412%
7	2.458	434	441	452	rVB6	1137	1938	0.05%	0.012%
8	2.706	507	518	534	rBV2	17292	30177	0.83%	0.185%
9	2.822	547	554	559	rBV	220	300	0.01%	0.002%
10	3.121	626	647	677	rBV	455467	958536	26.32%	5.863%
11	3.281	695	697	702	rBV3	408	298	0.01%	0.002%
12	3.423	739	741	746	rVB2	452	285	0.01%	0.002%
13	3.693	816	825	829	rBV3	382	558	0.02%	0.003%
14	3.716	829	832	837	rVB	385	325	0.01%	0.002%
15	3.822	849	865	906	rBV2	527322	1386153	38.06%	8.478%
16	4.156	967	969	974	rVB3	665	411	0.01%	0.003%
17	4.259	984	1001	1035	rVV2	153607	439051	12.05%	2.685%
18	4.523	1062	1083	1113	rBV	1428200	3642170	100.00%	22.277%
19	4.844	1181	1183	1186	rVB2	535	296	0.01%	0.002%
20	4.870	1186	1191	1193	rBV3	395	372	0.01%	0.002%
21	4.963	1200	1220	1244	rBV2	343861	913740	25.09%	5.589%
22	5.159	1279	1281	1286	rVB2	1027	711	0.02%	0.004%
23	5.207	1293	1296	1301	rVB2	391	266	0.01%	0.002%
24	5.474	1375	1379	1381	rBV	332	300	0.01%	0.002%
25	5.542	1388	1400	1429	rBV	304072	624675	17.15%	3.821%
26	5.838	1479	1492	1519	rBV	683907	1365812	37.50%	8.354%
27	5.995	1529	1541	1566	rVB	214572	435597	11.96%	2.664%
28	6.175	1594	1597	1599	rVB2	696	428	0.01%	0.003%
29	6.301	1631	1636	1640	rVV3	299	300	0.01%	0.002%
30	6.330	1643	1645	1648	rVB2	456	306	0.01%	0.002%
31	6.355	1648	1653	1656	rBV	290	277	0.01%	0.002%
32	6.487	1690	1694	1700	rVV3	394	336	0.01%	0.002%
33	6.584	1720	1724	1727	rBV2	359	329	0.01%	0.002%
34	6.600	1727	1729	1733	rVB3	377	316	0.01%	0.002%
35	6.667	1744	1750	1753	rBV2	371	459	0.01%	0.003%
36	6.686	1753	1756	1759	rVV	287	273	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031547.D
 Acq On : 15 Jun 2023 22:42
 Operator : SY/MD
 Sample : 03249-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.828	1797	1800	1807	rVB3	251	314	0.01%	0.002%
38	6.921	1817	1829	1850	rBV	106263	197178	5.41%	1.206%
39	7.143	1896	1898	1901	rVB	638	319	0.01%	0.002%
40	7.249	1919	1931	1954	rBV	376507	657868	18.06%	4.024%
41	7.506	2009	2011	2017	rBV4	309	331	0.01%	0.002%
42	7.558	2017	2027	2058	rVV	77042	140921	3.87%	0.862%
43	7.738	2078	2083	2087	rBV3	425	379	0.01%	0.002%
44	7.780	2087	2096	2110	rBV2	18735	32849	0.90%	0.201%
45	7.912	2115	2137	2165	rBV	462354	797480	21.90%	4.878%
46	8.030	2165	2174	2198	rBV	230569	412195	11.32%	2.521%
47	8.265	2244	2247	2248	rBV2	396	253	0.01%	0.002%
48	8.545	2330	2334	2337	rBV2	339	361	0.01%	0.002%
49	8.606	2350	2353	2357	rVB3	442	330	0.01%	0.002%
50	8.789	2399	2410	2440	rBV	460557	756937	20.78%	4.630%
51	8.956	2459	2462	2467	rVB4	722	770	0.02%	0.005%
52	8.982	2468	2470	2475	rVB3	359	307	0.01%	0.002%
53	9.092	2502	2504	2508	rVB3	508	357	0.01%	0.002%
54	9.120	2510	2513	2517	rVB3	468	291	0.01%	0.002%
55	9.185	2529	2533	2535	rBV2	306	256	0.01%	0.002%
56	9.259	2550	2556	2559	rBV3	281	378	0.01%	0.002%
57	9.500	2629	2631	2643	rVB4	716	896	0.02%	0.005%
58	9.722	2695	2700	2702	rBV	443	384	0.01%	0.002%
59	9.764	2707	2713	2716	rBV2	382	307	0.01%	0.002%
60	9.873	2742	2747	2750	rBV	619	544	0.01%	0.003%
61	10.072	2805	2809	2812	rBV2	284	259	0.01%	0.002%
62	10.159	2824	2836	2857	rBV	301340	481635	13.22%	2.946%
63	10.333	2880	2890	2903	rBV2	6925	11973	0.33%	0.073%
64	10.571	2961	2964	2970	rVB2	478	495	0.01%	0.003%
65	10.606	2970	2975	2978	rBV2	469	389	0.01%	0.002%
66	10.792	3025	3033	3036	rBV2	417	416	0.01%	0.003%
67	10.857	3048	3053	3058	rBV4	712	693	0.02%	0.004%
68	10.927	3070	3075	3077	rVB2	408	297	0.01%	0.002%
69	11.133	3135	3139	3143	rVB4	939	633	0.02%	0.004%
70	11.191	3145	3157	3179	rBV	481376	729941	20.04%	4.465%
71	11.352	3205	3207	3212	rBV2	343	257	0.01%	0.002%
72	11.516	3250	3258	3262	rBV5	1281	1695	0.05%	0.010%
73	11.567	3262	3274	3292	rBV	436493	681147	18.70%	4.166%
74	11.789	3337	3343	3349	rBV3	336	500	0.01%	0.003%
75	11.828	3351	3355	3360	rBV3	335	409	0.01%	0.003%
76	12.062	3424	3428	3430	rBV2	315	265	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031547.D
 Acq On : 15 Jun 2023 22:42
 Operator : SY/MD
 Sample : 03249-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.204	3461	3472	3482	rBV2	2545	3832	0.11%	0.023%
78	12.394	3527	3531	3533	rBV2	422	381	0.01%	0.002%
79	12.738	3635	3638	3642	rBV3	382	407	0.01%	0.002%
80	12.828	3662	3666	3670	rBV2	393	364	0.01%	0.002%
81	12.870	3677	3679	3683	rVB2	511	293	0.01%	0.002%
82	13.214	3779	3786	3791	rBV4	1041	1443	0.04%	0.009%
83	13.323	3816	3820	3824	rBV3	413	386	0.01%	0.002%
84	13.451	3854	3860	3869	rVB2	1341	2076	0.06%	0.013%
85	13.654	3920	3923	3927	rVB2	294	258	0.01%	0.002%
86	13.689	3928	3934	3940	rBV5	964	1351	0.04%	0.008%
87	13.876	3986	3992	3994	rVB2	471	471	0.01%	0.003%
88	13.898	3994	3999	4002	rBV3	448	470	0.01%	0.003%
89	13.979	4022	4024	4027	rBV2	471	305	0.01%	0.002%
90	14.352	4137	4140	4143	rVV2	337	251	0.01%	0.002%
91	14.461	4172	4174	4179	rVB3	503	397	0.01%	0.002%
92	14.580	4209	4211	4217	rVB3	568	422	0.01%	0.003%
93	14.612	4217	4221	4224	rBV4	696	552	0.02%	0.003%
94	14.638	4227	4229	4232	rVV2	469	303	0.01%	0.002%
95	14.696	4244	4247	4250	rVV2	495	299	0.01%	0.002%
96	14.959	4326	4329	4331	rBV3	600	377	0.01%	0.002%
97	15.056	4357	4359	4362	rVB	689	418	0.01%	0.003%
98	15.120	4376	4379	4380	rBV	629	375	0.01%	0.002%
99	15.162	4389	4392	4395	rBV4	421	308	0.01%	0.002%
100	15.519	4500	4503	4506	rBV3	659	550	0.02%	0.003%

Sum of corrected areas: 16349213




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031547.D
Acq On : 15 Jun 2023 22:42
Operator : SY/MD
Sample : 03249-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

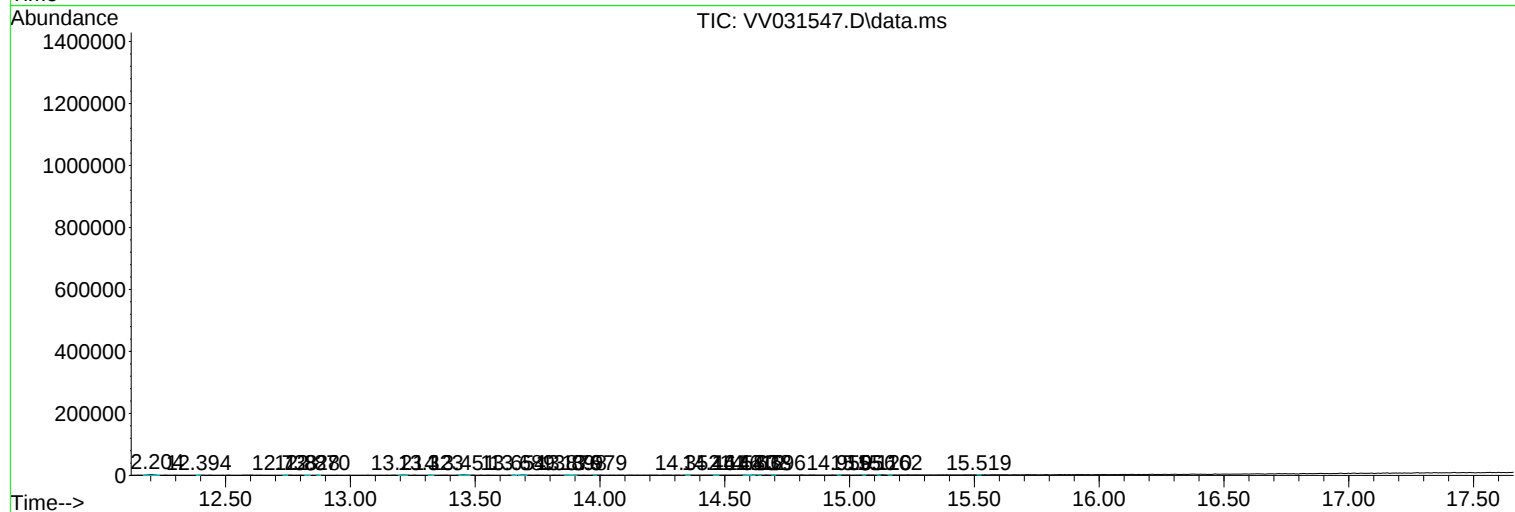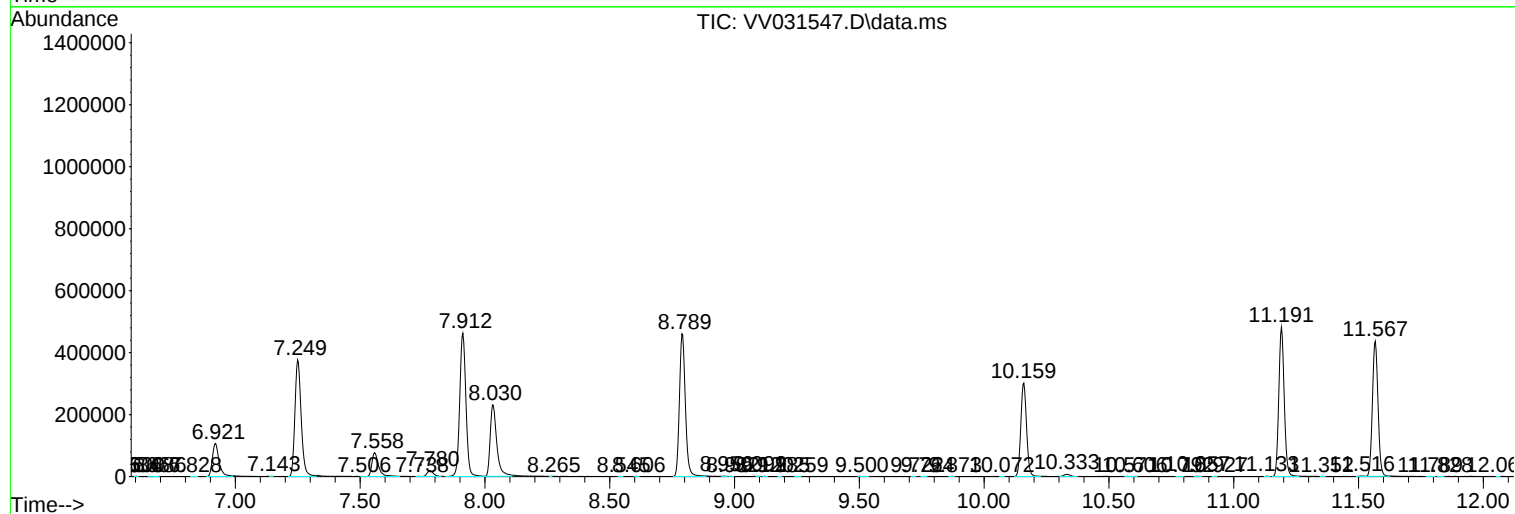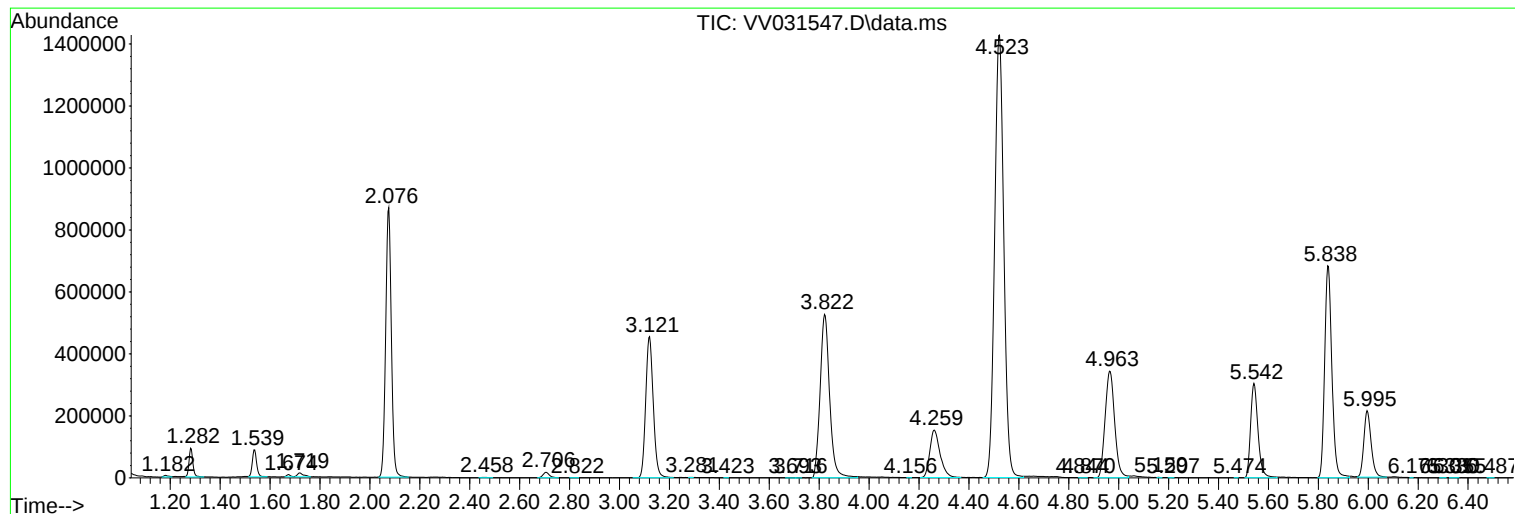

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031547.D
Acq On : 15 Jun 2023 22:42
Operator : SY/MD
Sample : 03249-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031547.D
Acq On : 15 Jun 2023 22:42
Operator : SY/MD
Sample : 03249-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------