

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031548.D
 Acq On : 15 Jun 2023 23:05
 Operator : SY/MD
 Sample : 03254-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	98695	107313	12.06%	1.461%
2	1.539	148	155	171	rVB	86900	104306	11.72%	1.420%
3	2.066	309	319	341	rVB	178629	260966	29.33%	3.552%
4	2.516	457	459	462	rBV	284	153	0.02%	0.002%
5	2.587	477	481	485	rBV3	420	307	0.03%	0.004%
6	2.632	492	495	498	rBV	320	213	0.02%	0.003%
7	2.709	509	519	532	rVB5	4207	8271	0.93%	0.113%
8	2.761	532	535	539	rBV3	504	449	0.05%	0.006%
9	2.995	605	608	611	rBV3	371	249	0.03%	0.003%
10	3.121	632	647	672	rBV	68525	147431	16.57%	2.007%
11	3.297	700	702	709	rVB2	342	347	0.04%	0.005%
12	3.368	721	724	729	rVB3	360	319	0.04%	0.004%
13	3.394	729	732	733	rBV	232	126	0.01%	0.002%
14	3.532	773	775	783	rVB2	373	321	0.04%	0.004%
15	3.564	783	785	787	rBV	250	166	0.02%	0.002%
16	3.667	814	817	818	rBV2	256	139	0.02%	0.002%
17	3.741	837	840	841	rBV	199	99	0.01%	0.001%
18	3.818	849	864	897	rBV2	121934	387612	43.57%	5.276%
19	4.259	985	1001	1030	rBV2	146729	384719	43.24%	5.236%
20	4.522	1064	1083	1106	rVB3	29398	77548	8.72%	1.055%
21	4.629	1113	1116	1120	rBV2	307	195	0.02%	0.003%
22	4.706	1138	1140	1144	rBV	206	172	0.02%	0.002%
23	4.754	1152	1155	1157	rBV	294	179	0.02%	0.002%
24	4.815	1171	1174	1180	rVB3	320	287	0.03%	0.004%
25	4.863	1187	1189	1192	rBV2	228	95	0.01%	0.001%
26	4.963	1203	1220	1249	rBV2	330000	889629	100.00%	12.109%
27	5.352	1339	1341	1344	rBV	323	220	0.02%	0.003%
28	5.445	1368	1370	1372	rVB	259	101	0.01%	0.001%
29	5.542	1388	1400	1428	rBV	287177	591533	66.49%	8.051%
30	5.847	1484	1495	1510	rVB7	10722	21791	2.45%	0.297%
31	5.995	1525	1541	1563	rBV	205903	423059	47.55%	5.758%
32	6.223	1610	1612	1613	rBV	146	58	0.01%	0.001%
33	6.407	1667	1669	1670	rVB	124	29	0.00%	0.000%
34	6.420	1671	1673	1675	rVV	168	69	0.01%	0.001%
35	6.577	1719	1722	1724	rBV	269	189	0.02%	0.003%
36	6.648	1741	1744	1747	rVB2	192	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031548.D
 Acq On : 15 Jun 2023 23:05
 Operator : SY/MD
 Sample : 03254-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.799	1789	1791	1794	rVB2	187	80	0.01%	0.001%
38	6.818	1794	1797	1800	rBV	252	177	0.02%	0.002%
39	6.918	1817	1828	1849	rBV2	102480	189429	21.29%	2.578%
40	7.124	1890	1892	1896	rBV3	543	334	0.04%	0.005%
41	7.162	1902	1904	1906	rVB	607	296	0.03%	0.004%
42	7.201	1913	1916	1919	rVB2	431	267	0.03%	0.004%
43	7.249	1919	1931	1967	rBV	364392	645829	72.60%	8.790%
44	7.558	2017	2027	2051	rBV	77012	137128	15.41%	1.866%
45	7.741	2081	2084	2086	rBV	399	240	0.03%	0.003%
46	7.786	2095	2098	2101	rBV2	404	287	0.03%	0.004%
47	8.030	2165	2174	2208	rBV	214654	396301	44.55%	5.394%
48	8.432	2293	2299	2301	rBV2	369	335	0.04%	0.005%
49	8.593	2347	2349	2352	rVB2	309	183	0.02%	0.002%
50	8.635	2360	2362	2365	rBV3	388	212	0.02%	0.003%
51	8.741	2391	2395	2399	rVB	360	306	0.03%	0.004%
52	8.789	2399	2410	2434	rBV	434885	716420	80.53%	9.751%
53	8.992	2470	2473	2476	rBV3	360	241	0.03%	0.003%
54	9.091	2502	2504	2508	rBV2	330	187	0.02%	0.003%
55	9.133	2515	2517	2519	rVB	268	109	0.01%	0.001%
56	9.149	2519	2522	2524	rBV2	245	178	0.02%	0.002%
57	9.207	2534	2540	2544	rBV2	559	627	0.07%	0.009%
58	9.381	2591	2594	2599	rVB3	361	300	0.03%	0.004%
59	9.407	2599	2602	2603	rBV	361	161	0.02%	0.002%
60	9.532	2639	2641	2643	rBV2	223	98	0.01%	0.001%
61	9.680	2685	2687	2690	rBV2	210	119	0.01%	0.002%
62	10.079	2808	2811	2814	rBB	223	139	0.02%	0.002%
63	10.159	2824	2836	2854	rBV	306265	480234	53.98%	6.536%
64	10.333	2880	2890	2905	rBV4	5218	9066	1.02%	0.123%
65	10.410	2911	2914	2919	rBV2	194	181	0.02%	0.002%
66	10.641	2984	2986	2988	rBV	179	127	0.01%	0.002%
67	10.924	3071	3074	3076	rBV	264	136	0.02%	0.002%
68	10.976	3087	3090	3091	rBV	204	103	0.01%	0.001%
69	11.133	3135	3139	3144	rVB2	601	476	0.05%	0.006%
70	11.191	3144	3157	3175	rBV	451361	687749	77.31%	9.361%
71	11.506	3253	3255	3257	rBV	353	197	0.02%	0.003%
72	11.567	3262	3274	3295	rVV	428320	668359	75.13%	9.097%
73	12.368	3521	3523	3526	rBV2	275	150	0.02%	0.002%
74	12.593	3589	3593	3595	rBV3	798	564	0.06%	0.008%
75	13.763	3955	3957	3958	rBV3	305	116	0.01%	0.002%
76	13.850	3981	3984	3989	rVB4	640	499	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031548.D
Acq On : 15 Jun 2023 23:05
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis

77	13.873	3989	3991	3993	rBV	369	181	0.02%	0.002%
78	14.249	4105	4108	4110	rBV	378	232	0.03%	0.003%




Sum of corrected areas: 7347123

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031548.D
Acq On : 15 Jun 2023 23:05
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

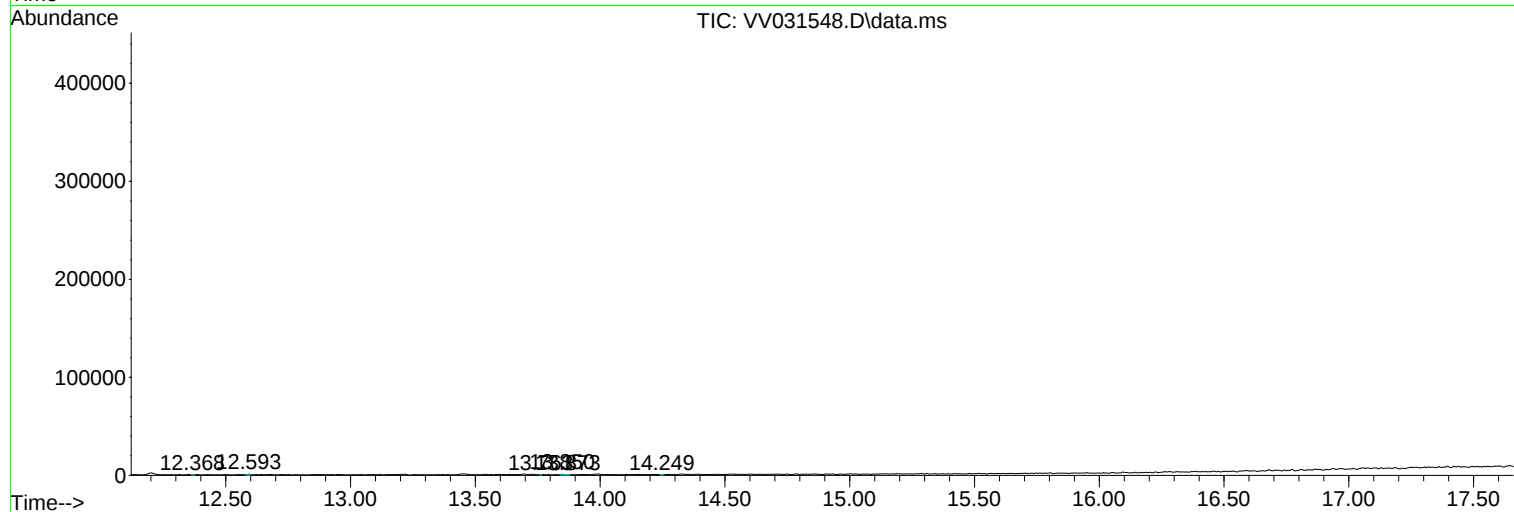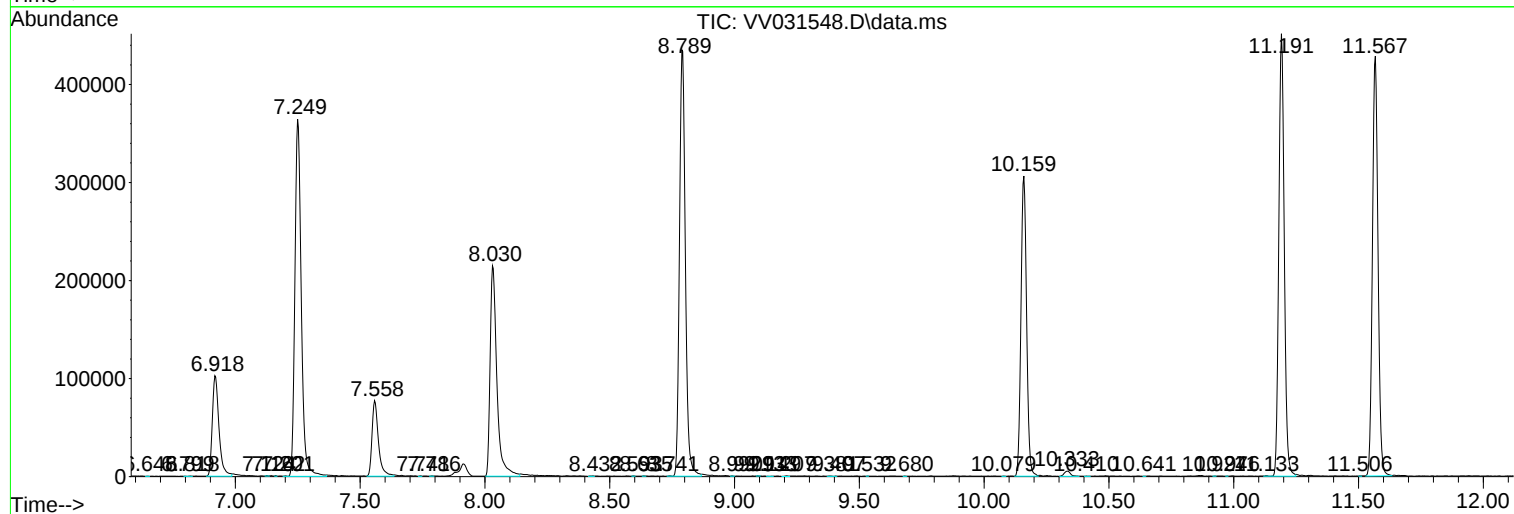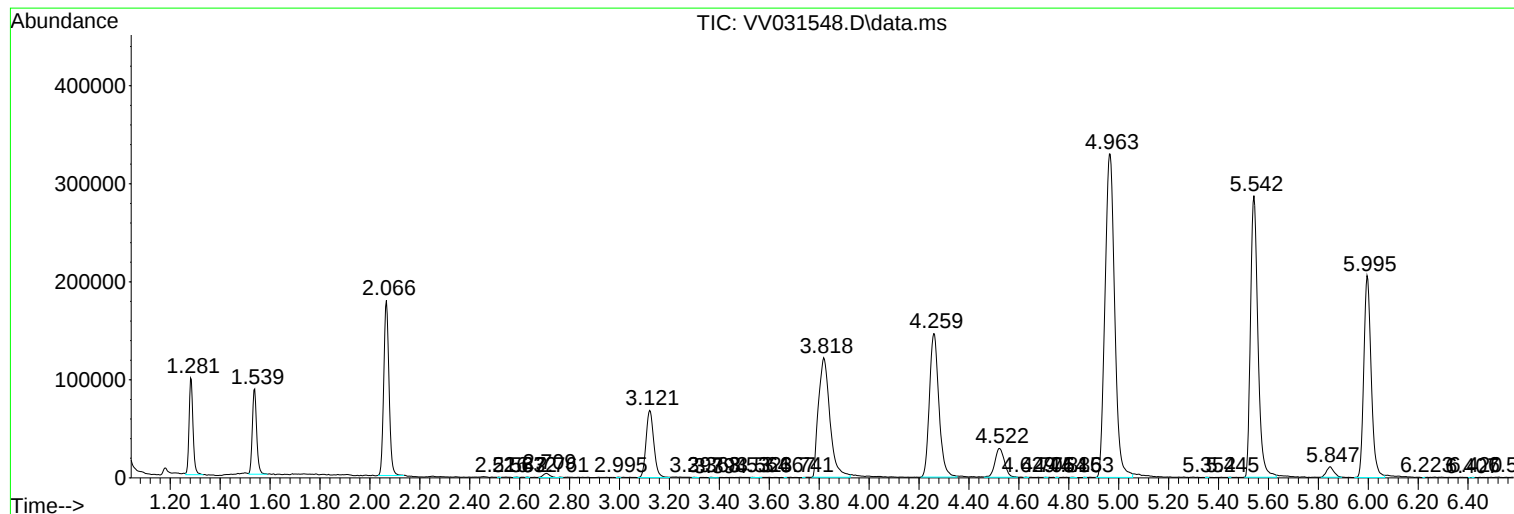

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031548.D
Acq On : 15 Jun 2023 23:05
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031548.D
Acq On : 15 Jun 2023 23:05
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc