

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031550.D
 Acq On : 15 Jun 2023 23:52
 Operator : SY/MD
 Sample : 03254-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VW031550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	94	rVB2	248143	271584	30.96%	3.589%
2	1.555	148	160	174	rVB2	182320	305181	34.79%	4.033%
3	2.066	309	319	333	rBV	177414	260718	29.72%	3.445%
4	2.407	422	425	427	rBV2	265	194	0.02%	0.003%
5	2.458	436	441	446	rVB5	923	1161	0.13%	0.015%
6	2.709	509	519	531	rBV4	3934	7197	0.82%	0.095%
7	2.867	563	568	570	rBV2	369	327	0.04%	0.004%
8	2.902	577	579	582	rBV	171	149	0.02%	0.002%
9	3.005	608	611	612	rBV	200	104	0.01%	0.001%
10	3.060	625	628	629	rBV	266	171	0.02%	0.002%
11	3.124	636	648	664	rBV3	6574	14157	1.61%	0.187%
12	3.314	702	707	711	rBV3	296	340	0.04%	0.004%
13	3.407	733	736	737	rBV2	213	122	0.01%	0.002%
14	3.433	740	744	748	rBV3	241	224	0.03%	0.003%
15	3.478	753	758	761	rBV	271	292	0.03%	0.004%
16	3.503	764	766	769	rBV2	266	187	0.02%	0.002%
17	3.748	840	842	845	rBV	189	110	0.01%	0.001%
18	3.822	849	865	890	rBV2	156343	473280	53.96%	6.254%
19	4.259	984	1001	1033	rBV	144257	381295	43.47%	5.039%
20	4.503	1074	1077	1079	rBV2	634	416	0.05%	0.005%
21	4.632	1113	1117	1120	rBV3	297	214	0.02%	0.003%
22	4.687	1131	1134	1136	rBV2	197	137	0.02%	0.002%
23	4.799	1164	1169	1170	rBV2	152	142	0.02%	0.002%
24	4.841	1180	1182	1185	rVB	460	221	0.03%	0.003%
25	4.963	1203	1220	1241	rBV2	327923	877158	100.00%	11.591%
26	5.320	1329	1331	1335	rVB	259	117	0.01%	0.002%
27	5.359	1341	1343	1348	rBV	358	198	0.02%	0.003%
28	5.391	1348	1353	1359	rBV3	362	418	0.05%	0.006%
29	5.468	1375	1377	1380	rVB2	415	224	0.03%	0.003%
30	5.487	1380	1383	1387	rBV	436	313	0.04%	0.004%
31	5.542	1387	1400	1432	rBV	288674	596843	68.04%	7.887%
32	5.844	1482	1494	1503	rVB9	1929	4022	0.46%	0.053%
33	5.905	1509	1513	1516	rVB	244	163	0.02%	0.002%
34	5.921	1516	1518	1524	rVB2	323	205	0.02%	0.003%
35	5.995	1528	1541	1567	rBV	203640	423271	48.25%	5.593%
36	6.178	1595	1598	1602	rVB2	752	440	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031550.D
 Acq On : 15 Jun 2023 23:52
 Operator : SY/MD
 Sample : 03254-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.230	1612	1614	1616	rBV	374	104	0.01%	0.001%
38	6.359	1644	1654	1657	rBV4	1568	2402	0.27%	0.032%
39	6.468	1686	1688	1691	rBV	201	104	0.01%	0.001%
40	6.584	1721	1724	1728	rBV	325	208	0.02%	0.003%
41	6.645	1740	1743	1745	rBV	341	156	0.02%	0.002%
42	6.744	1770	1774	1775	rBV	223	133	0.02%	0.002%
43	6.757	1775	1778	1780	rVV	209	135	0.02%	0.002%
44	6.838	1802	1803	1808	rBV2	163	121	0.01%	0.002%
45	6.918	1818	1828	1850	rBV2	101007	187101	21.33%	2.472%
46	7.191	1910	1913	1919	rVB3	373	319	0.04%	0.004%
47	7.249	1919	1931	1954	rBV	361941	635538	72.45%	8.398%
48	7.558	2017	2027	2051	rBV	77453	136389	15.55%	1.802%
49	7.786	2094	2098	2101	rVB2	251	203	0.02%	0.003%
50	7.805	2101	2104	2107	rBV	282	217	0.02%	0.003%
51	7.828	2107	2111	2113	rBV2	253	164	0.02%	0.002%
52	7.883	2120	2128	2134	rBV4	3459	5359	0.61%	0.071%
53	8.030	2164	2174	2202	rBV	216766	400578	45.67%	5.294%
54	8.458	2305	2307	2311	rBV2	215	156	0.02%	0.002%
55	8.558	2336	2338	2341	rBV2	298	136	0.02%	0.002%
56	8.789	2399	2410	2439	rBV	448250	720486	82.14%	9.521%
57	8.960	2460	2463	2464	rBV	356	201	0.02%	0.003%
58	9.014	2476	2480	2482	rBV	265	174	0.02%	0.002%
59	9.027	2482	2484	2491	rVV3	432	380	0.04%	0.005%
60	9.259	2552	2556	2562	rVB2	424	493	0.06%	0.007%
61	9.291	2562	2566	2569	rBV2	227	197	0.02%	0.003%
62	9.310	2569	2572	2574	rBV2	282	144	0.02%	0.002%
63	9.329	2574	2578	2582	rVB2	342	267	0.03%	0.004%
64	9.374	2589	2592	2594	rBV	165	108	0.01%	0.001%
65	9.490	2625	2628	2629	rBV2	355	253	0.03%	0.003%
66	9.696	2690	2692	2694	rBV	241	120	0.01%	0.002%
67	9.770	2713	2715	2718	rBV	267	180	0.02%	0.002%
68	10.027	2791	2795	2798	rBV	260	220	0.03%	0.003%
69	10.040	2798	2799	2802	rVB	254	112	0.01%	0.001%
70	10.098	2813	2817	2818	rBV2	276	169	0.02%	0.002%
71	10.159	2823	2836	2858	rVV	302072	480996	54.84%	6.356%
72	10.275	2869	2872	2874	rBV2	314	185	0.02%	0.002%
73	10.336	2880	2891	2902	rBV2	4808	8257	0.94%	0.109%
74	10.419	2915	2917	2919	rVB	327	138	0.02%	0.002%
75	10.616	2973	2978	2984	rBV2	351	452	0.05%	0.006%
76	10.673	2993	2996	2998	rBV	444	214	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031550.D
 Acq On : 15 Jun 2023 23:52
 Operator : SY/MD
 Sample : 03254-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	10.712	3005	3008	3011	rBV	243	210	0.02%	0.003%
78	10.799	3032	3035	3036	rBV	263	140	0.02%	0.002%
79	10.854	3049	3052	3053	rBV2	341	192	0.02%	0.003%
80	10.902	3064	3067	3070	rBV	293	253	0.03%	0.003%
81	11.191	3144	3157	3175	rBV	455900	691009	78.78%	9.132%
82	11.333	3199	3201	3206	rBV4	400	378	0.04%	0.005%
83	11.567	3262	3274	3290	rBV	428360	663343	75.62%	8.766%
84	11.747	3326	3330	3332	rBV2	601	482	0.05%	0.006%
85	11.789	3339	3343	3346	rBV2	200	182	0.02%	0.002%
86	11.808	3346	3349	3351	rBV	247	170	0.02%	0.002%
87	11.966	3396	3398	3401	rBV2	213	136	0.02%	0.002%
88	12.082	3431	3434	3437	rBV2	464	384	0.04%	0.005%
89	12.204	3458	3472	3478	rBV4	1629	3027	0.35%	0.040%
90	12.342	3513	3515	3520	rBV2	342	259	0.03%	0.003%
91	12.464	3551	3553	3554	rBV2	282	98	0.01%	0.001%
92	12.548	3576	3579	3581	rBV2	431	258	0.03%	0.003%
93	12.886	3682	3684	3688	rVB2	404	219	0.02%	0.003%
94	12.924	3693	3696	3699	rBV2	330	259	0.03%	0.003%
95	12.963	3706	3708	3711	rBV2	484	350	0.04%	0.005%
96	13.313	3814	3817	3821	rVB2	392	273	0.03%	0.004%
97	13.439	3854	3856	3858	rBV	456	199	0.02%	0.003%
98	13.480	3867	3869	3870	rBV	298	117	0.01%	0.002%
99	13.863	3986	3988	3990	rBV	377	254	0.03%	0.003%
100	14.757	4264	4266	4270	rBV3	654	553	0.06%	0.007%




Sum of corrected areas: 7567309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031550.D
Acq On : 15 Jun 2023 23:52
Operator : SY/MD
Sample : 03254-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

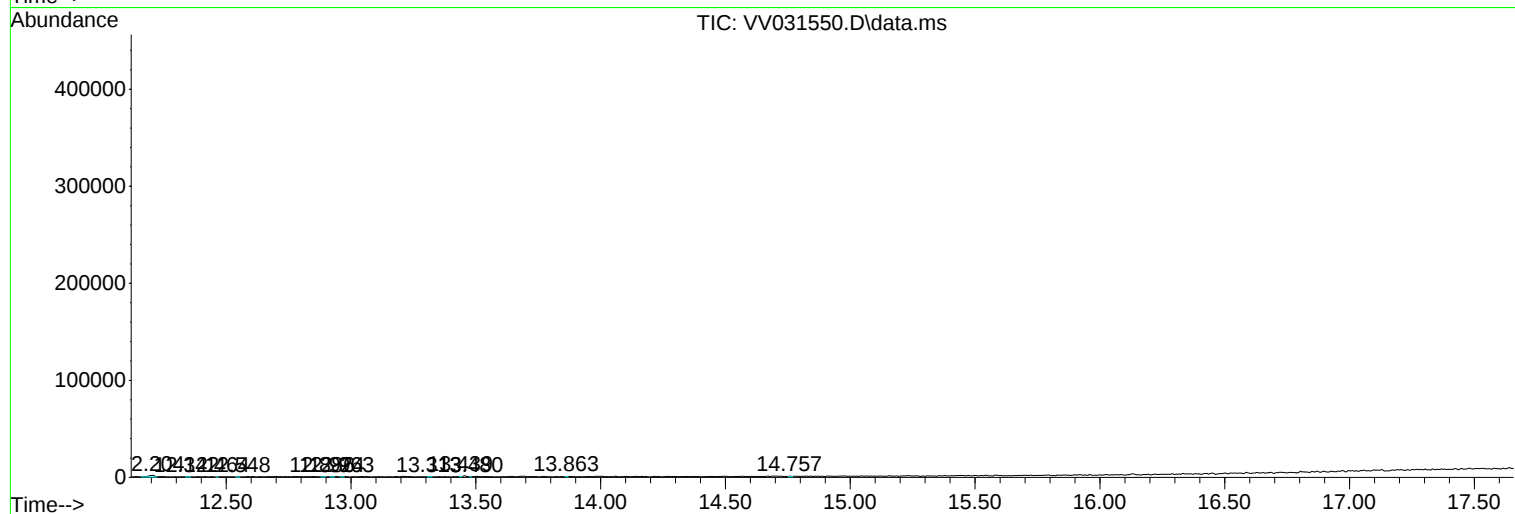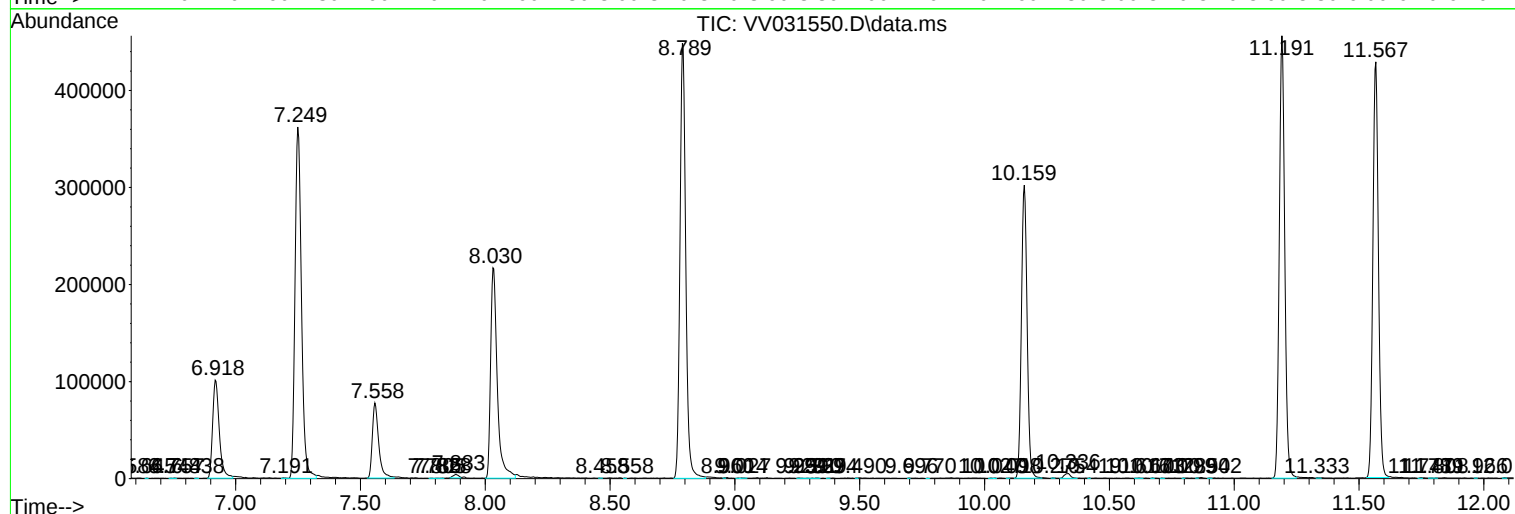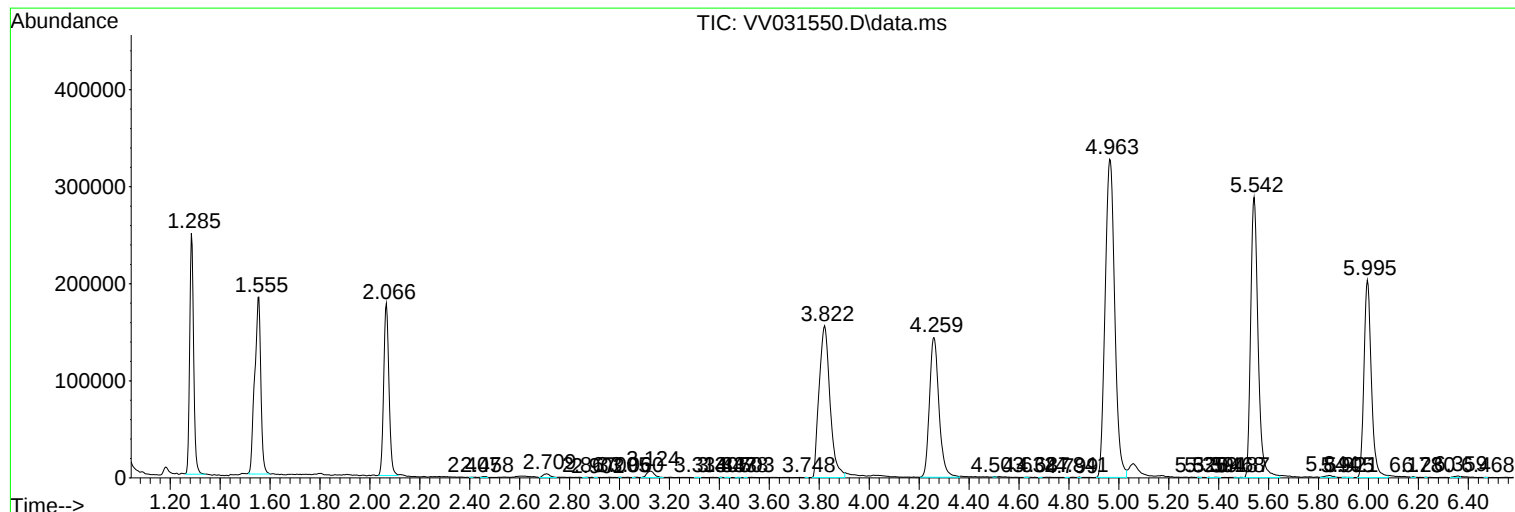

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031550.D
Acq On : 15 Jun 2023 23:52
Operator : SY/MD
Sample : 03254-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031550.D
Acq On : 15 Jun 2023 23:52
Operator : SY/MD
Sample : 03254-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------