

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031553.D
 Acq On : 16 Jun 2023 01:01
 Operator : SY/MD
 Sample : 03254-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.176	38	42	53	rVB	10747	12336	1.38%	0.155%
2	1.282	69	75	89	rVB	91411	96183	10.73%	1.208%
3	1.536	148	154	177	rVB	87133	113602	12.67%	1.427%
4	2.066	309	319	333	rBV	184768	269760	30.08%	3.388%
5	2.407	422	425	428	rBV2	480	356	0.04%	0.004%
6	2.651	497	501	508	rBV	219	315	0.04%	0.004%
7	2.706	509	518	531	rVV2	7914	14427	1.61%	0.181%
8	3.121	633	647	666	rBV	116585	246500	27.49%	3.096%
9	3.333	710	713	714	rBV	270	174	0.02%	0.002%
10	3.394	729	732	734	rBV	160	129	0.01%	0.002%
11	3.417	737	739	741	rVV	247	123	0.01%	0.002%
12	3.442	745	747	752	rVB2	303	207	0.02%	0.003%
13	3.593	792	794	797	rVB	293	137	0.02%	0.002%
14	3.690	822	824	826	rBV2	178	72	0.01%	0.001%
15	3.748	835	842	846	rBV2	242	397	0.04%	0.005%
16	3.819	848	864	900	rBV2	127213	424713	47.36%	5.334%
17	4.259	984	1001	1032	rBV	151294	388448	43.32%	4.878%
18	4.519	1067	1082	1105	rVB	180187	460038	51.30%	5.777%
19	4.880	1190	1194	1195	rBV	412	223	0.02%	0.003%
20	4.963	1203	1220	1245	rBV2	336148	896727	100.00%	11.261%
21	5.240	1304	1306	1307	rBV	409	132	0.01%	0.002%
22	5.397	1353	1355	1356	rBV	229	92	0.01%	0.001%
23	5.542	1387	1400	1425	rBV	295093	608092	67.81%	7.636%
24	5.847	1484	1495	1510	rVB5	10607	22983	2.56%	0.289%
25	5.925	1517	1519	1523	rBV2	245	133	0.01%	0.002%
26	5.995	1527	1541	1568	rBV	206819	429830	47.93%	5.398%
27	6.220	1604	1611	1616	rBV4	442	448	0.05%	0.006%
28	6.330	1644	1645	1648	rBV	213	109	0.01%	0.001%
29	6.542	1708	1711	1715	rBV2	242	265	0.03%	0.003%
30	6.625	1736	1737	1740	rVB	302	107	0.01%	0.001%
31	6.699	1758	1760	1764	rVB	269	121	0.01%	0.002%
32	6.732	1768	1770	1775	rVV	231	214	0.02%	0.003%
33	6.777	1779	1784	1787	rBV	406	293	0.03%	0.004%
34	6.918	1818	1828	1857	rBV	103197	191730	21.38%	2.408%
35	7.166	1902	1905	1906	rBV2	328	153	0.02%	0.002%
36	7.249	1919	1931	1959	rBV	367264	646810	72.13%	8.123%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031553.D
 Acq On : 16 Jun 2023 01:01
 Operator : SY/MD
 Sample : 03254-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.471	1997	2000	2005	rBV3	493	333	0.04%	0.004%
38	7.558	2017	2027	2048	rBV	74627	133713	14.91%	1.679%
39	7.879	2119	2127	2128	rBV2	2886	2785	0.31%	0.035%
40	8.031	2164	2174	2203	rBV	214120	392132	43.73%	4.924%
41	8.410	2286	2292	2293	rBV2	542	548	0.06%	0.007%
42	8.445	2300	2303	2304	rBV2	282	162	0.02%	0.002%
43	8.455	2304	2306	2307	rBV	206	57	0.01%	0.001%
44	8.548	2332	2335	2338	rBV	268	191	0.02%	0.002%
45	8.670	2369	2373	2376	rBV3	359	281	0.03%	0.004%
46	8.789	2398	2410	2437	rBV	457197	740896	82.62%	9.304%
47	9.159	2522	2525	2528	rBV	207	174	0.02%	0.002%
48	9.532	2638	2641	2643	rBV	225	140	0.02%	0.002%
49	9.712	2692	2697	2700	rBV2	348	356	0.04%	0.004%
50	9.773	2713	2716	2719	rBV	229	160	0.02%	0.002%
51	10.159	2824	2836	2859	rBV	301317	478936	53.41%	6.014%
52	10.259	2865	2867	2872	rVB3	438	262	0.03%	0.003%
53	10.497	2937	2941	2944	rBV	489	353	0.04%	0.004%
54	10.789	3028	3032	3034	rBV2	424	295	0.03%	0.004%
55	10.805	3034	3037	3042	rVB3	385	328	0.04%	0.004%
56	10.857	3048	3053	3066	rBV4	750	1467	0.16%	0.018%
57	10.982	3090	3092	3094	rVB2	181	60	0.01%	0.001%
58	11.191	3145	3157	3176	rBV	456002	708725	79.03%	8.900%
59	11.333	3199	3201	3203	rBV3	405	154	0.02%	0.002%
60	11.394	3217	3220	3222	rBV2	373	246	0.03%	0.003%
61	11.567	3262	3274	3294	rVB	425466	672718	75.02%	8.448%
62	11.966	3396	3398	3400	rBV	394	181	0.02%	0.002%
63	12.120	3444	3446	3448	rBV2	286	132	0.01%	0.002%
64	12.844	3668	3671	3674	rBV2	456	340	0.04%	0.004%
65	13.108	3750	3753	3755	rBV	351	222	0.02%	0.003%
66	14.288	4116	4120	4122	rBV3	445	393	0.04%	0.005%




Sum of corrected areas: 7963119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031553.D
Acq On : 16 Jun 2023 01:01
Operator : SY/MD
Sample : 03254-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

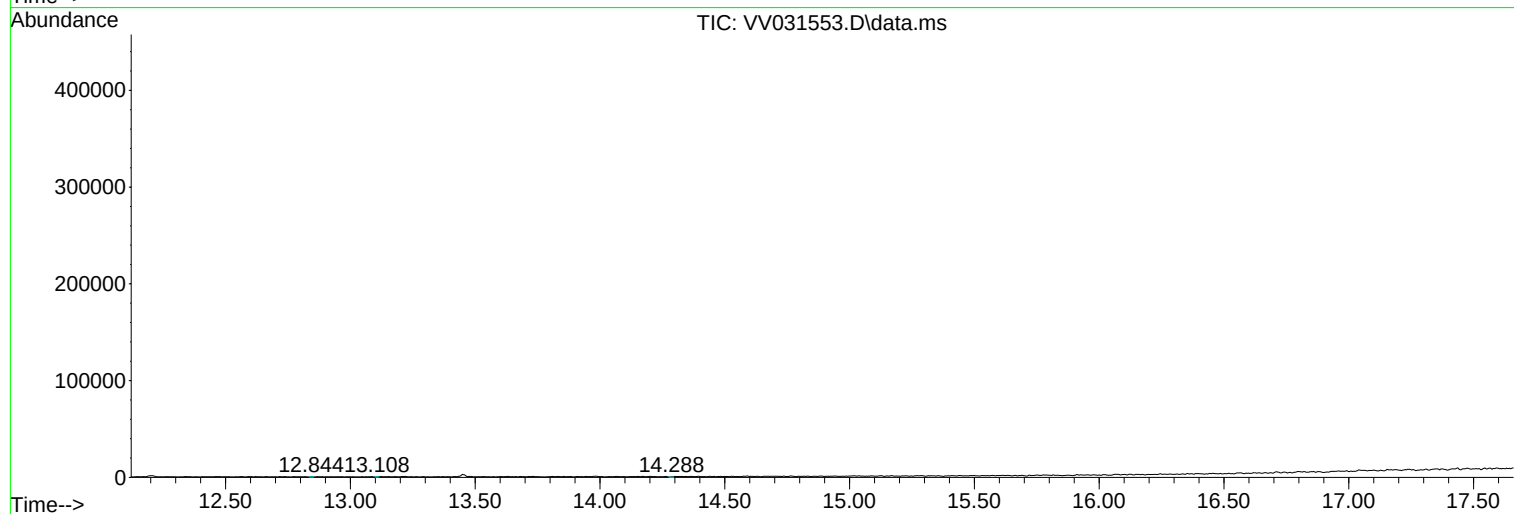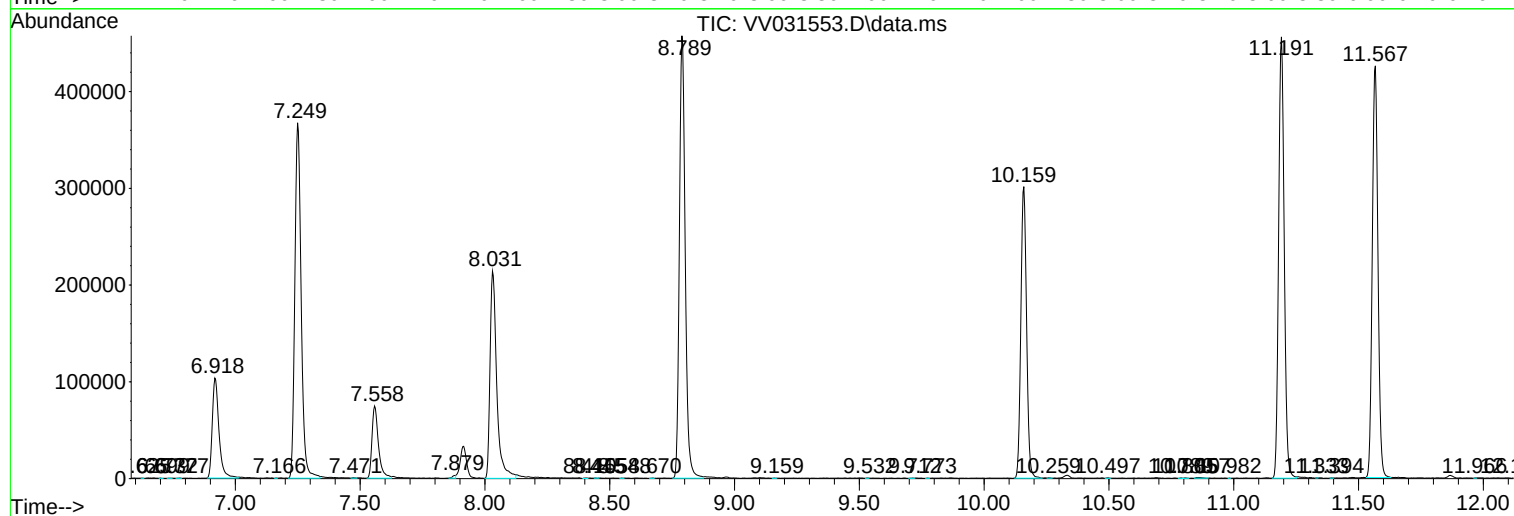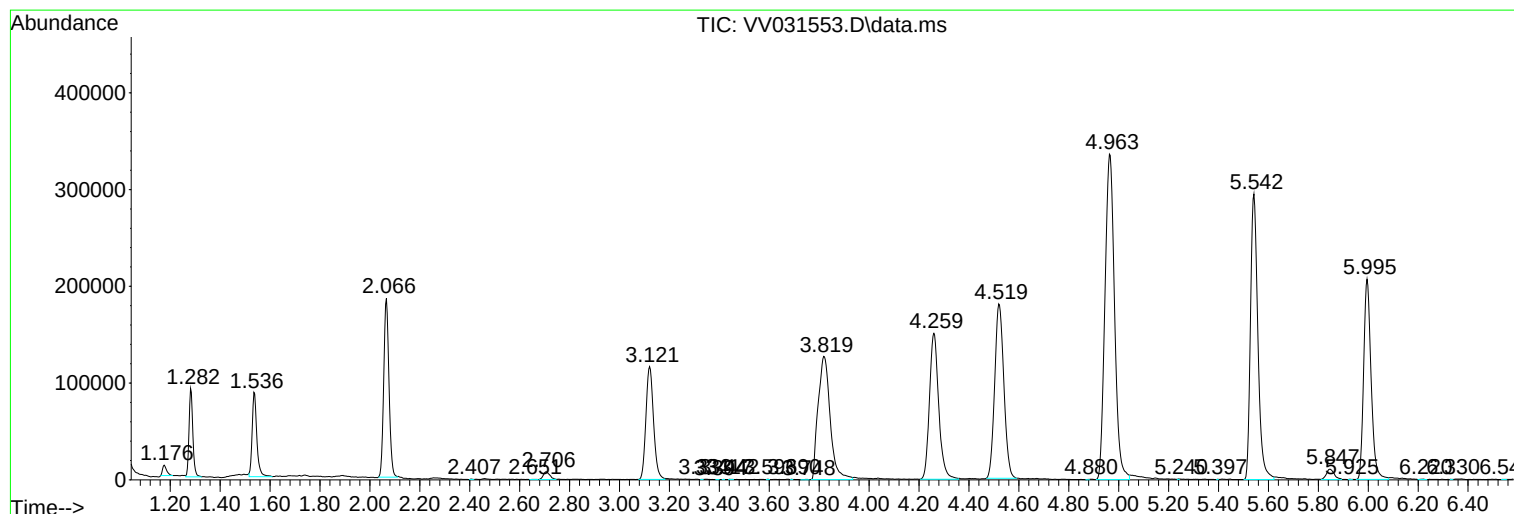

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031553.D
Acq On : 16 Jun 2023 01:01
Operator : SY/MD
Sample : 03254-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031553.D
Acq On : 16 Jun 2023 01:01
Operator : SY/MD
Sample : 03254-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------