

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031554.D
 Acq On : 16 Jun 2023 01:24
 Operator : SY/MD
 Sample : 03254-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	54	rBV	13056	19355	2.23%	0.248%
2	1.281	68	75	95	rVB	91503	101817	11.75%	1.306%
3	1.539	147	155	170	rVB	83266	104044	12.00%	1.335%
4	2.066	309	319	344	rVB3	196374	321994	37.14%	4.130%
5	2.252	369	377	385	rBV5	1447	2217	0.26%	0.028%
6	2.362	408	411	417	rBV2	321	268	0.03%	0.003%
7	2.455	436	440	442	rBV3	683	593	0.07%	0.008%
8	2.568	470	475	477	rBV4	630	598	0.07%	0.008%
9	2.584	477	480	482	rBV2	433	273	0.03%	0.004%
10	2.706	506	518	531	rVB5	5264	9548	1.10%	0.122%
11	2.777	537	540	546	rVB2	309	342	0.04%	0.004%
12	2.934	587	589	595	rVB2	220	223	0.03%	0.003%
13	3.121	632	647	670	rBV2	140255	292624	33.76%	3.753%
14	3.304	701	704	706	rBV2	355	269	0.03%	0.003%
15	3.407	732	736	739	rBV2	234	225	0.03%	0.003%
16	3.487	753	761	767	rBV2	287	510	0.06%	0.007%
17	3.645	808	810	816	rVB	278	245	0.03%	0.003%
18	3.815	848	863	893	rBV4	80704	282774	32.62%	3.627%
19	4.259	984	1001	1025	rBV	143857	376740	43.46%	4.832%
20	4.439	1055	1057	1060	rBV2	542	247	0.03%	0.003%
21	4.523	1065	1083	1108	rVV	104998	273185	31.51%	3.504%
22	4.654	1122	1124	1127	rBV2	314	214	0.02%	0.003%
23	4.693	1134	1136	1140	rBV2	326	249	0.03%	0.003%
24	4.886	1192	1196	1200	rBV3	255	247	0.03%	0.003%
25	4.963	1204	1220	1242	rBV2	322569	866883	100.00%	11.120%
26	5.365	1342	1345	1350	rVB2	334	234	0.03%	0.003%
27	5.542	1387	1400	1434	rBV	283069	586771	67.69%	7.527%
28	5.722	1453	1456	1460	rBV3	473	433	0.05%	0.006%
29	5.844	1483	1494	1517	rVV3	48005	101135	11.67%	1.297%
30	5.995	1527	1541	1568	rBV	202367	419345	48.37%	5.379%
31	6.201	1601	1605	1607	rBV	349	226	0.03%	0.003%
32	6.333	1641	1646	1647	rBV2	1324	981	0.11%	0.013%
33	6.410	1668	1670	1677	rVB4	393	416	0.05%	0.005%
34	6.786	1785	1787	1791	rVB	335	212	0.02%	0.003%
35	6.918	1817	1828	1854	rBV	98406	185788	21.43%	2.383%
36	7.034	1861	1864	1866	rVB3	549	294	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031554.D
 Acq On : 16 Jun 2023 01:24
 Operator : SY/MD
 Sample : 03254-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.092	1880	1882	1888	rVB2	414	310	0.04%	0.004%
38	7.140	1894	1897	1900	rVB2	397	227	0.03%	0.003%
39	7.198	1912	1915	1919	rBV2	348	200	0.02%	0.003%
40	7.249	1919	1931	1955	rBV	357853	623994	71.98%	8.004%
41	7.558	2017	2027	2045	rBV	73651	129479	14.94%	1.661%
42	7.677	2058	2064	2065	rBV2	331	318	0.04%	0.004%
43	7.783	2093	2097	2103	rVB3	635	649	0.07%	0.008%
44	7.911	2118	2137	2158	rBV	110637	192301	22.18%	2.467%
45	8.030	2164	2174	2202	rBV	206681	376902	43.48%	4.835%
46	8.188	2221	2223	2226	rVB3	679	382	0.04%	0.005%
47	8.346	2269	2272	2275	rBV2	430	233	0.03%	0.003%
48	8.374	2278	2281	2283	rVB2	471	244	0.03%	0.003%
49	8.487	2314	2316	2322	rVB2	309	258	0.03%	0.003%
50	8.609	2349	2354	2356	rBV	456	380	0.04%	0.005%
51	8.789	2398	2410	2435	rBV	441783	710697	81.98%	9.116%
52	8.895	2441	2443	2448	rVB5	1089	937	0.11%	0.012%
53	9.098	2505	2506	2509	rVB2	503	218	0.03%	0.003%
54	9.416	2603	2605	2610	rVB2	382	240	0.03%	0.003%
55	9.526	2635	2639	2641	rBV2	393	341	0.04%	0.004%
56	9.603	2660	2663	2666	rBV2	339	261	0.03%	0.003%
57	9.712	2691	2697	2702	rBV3	451	527	0.06%	0.007%
58	9.744	2702	2707	2710	rBV2	306	303	0.03%	0.004%
59	9.808	2721	2727	2732	rBV2	299	378	0.04%	0.005%
60	9.966	2772	2776	2778	rVV2	371	269	0.03%	0.003%
61	10.104	2814	2819	2820	rBV	271	245	0.03%	0.003%
62	10.159	2824	2836	2864	rVB	297589	468226	54.01%	6.006%
63	10.336	2880	2891	2900	rBV4	2952	4802	0.55%	0.062%
64	10.535	2948	2953	2956	rBV3	345	325	0.04%	0.004%
65	10.599	2970	2973	2978	rVB3	254	266	0.03%	0.003%
66	10.677	2994	2997	3001	rBV2	261	262	0.03%	0.003%
67	10.728	3011	3013	3017	rBV	284	203	0.02%	0.003%
68	10.850	3049	3051	3053	rBV3	425	251	0.03%	0.003%
69	10.953	3077	3083	3086	rBV2	207	236	0.03%	0.003%
70	10.979	3087	3091	3094	rBV	303	222	0.03%	0.003%
71	11.191	3145	3157	3173	rBV	441071	668749	77.14%	8.578%
72	11.567	3261	3274	3294	rBV	414521	649175	74.89%	8.327%
73	11.709	3315	3318	3321	rBV3	579	326	0.04%	0.004%
74	11.773	3331	3338	3340	rBV2	582	513	0.06%	0.007%
75	11.866	3363	3367	3369	rVB3	339	215	0.02%	0.003%
76	11.927	3383	3386	3389	rBV	290	218	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031554.D
 Acq On : 16 Jun 2023 01:24
 Operator : SY/MD
 Sample : 03254-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.085	3432	3435	3440	rVB3	279	243	0.03%	0.003%
78	12.117	3441	3445	3449	rBV3	424	506	0.06%	0.006%
79	12.197	3462	3470	3478	rBV4	1413	1995	0.23%	0.026%
80	12.471	3550	3555	3559	rBV2	265	261	0.03%	0.003%
81	12.805	3655	3659	3662	rVB	418	300	0.03%	0.004%
82	12.824	3662	3665	3668	rBV	354	261	0.03%	0.003%
83	13.088	3744	3747	3749	rBV	311	228	0.03%	0.003%
84	13.213	3783	3786	3789	rVB	558	276	0.03%	0.004%
85	13.390	3838	3841	3850	rVB3	376	487	0.06%	0.006%
86	13.439	3850	3856	3857	rBV4	576	469	0.05%	0.006%
87	13.770	3956	3959	3962	rBV3	512	384	0.04%	0.005%
88	13.995	4021	4029	4033	rVV5	611	753	0.09%	0.010%
89	14.014	4033	4035	4039	rVB3	421	268	0.03%	0.003%
90	14.040	4039	4043	4045	rBV	337	225	0.03%	0.003%
91	14.069	4048	4052	4053	rBV2	456	276	0.03%	0.004%
92	14.371	4144	4146	4149	rBV2	530	340	0.04%	0.004%
93	14.442	4165	4168	4172	rBV2	408	331	0.04%	0.004%
94	14.467	4173	4176	4178	rBV	300	221	0.03%	0.003%
95	14.992	4336	4339	4340	rBV	379	226	0.03%	0.003%
96	15.181	4396	4398	4400	rBV	415	235	0.03%	0.003%
97	15.297	4431	4434	4437	rBV2	431	246	0.03%	0.003%
98	15.332	4442	4445	4447	rBV2	757	457	0.05%	0.006%
99	15.458	4482	4484	4489	rBV4	601	497	0.06%	0.006%
100	15.805	4590	4592	4596	rBV5	833	768	0.09%	0.010%




Sum of corrected areas: 7796054

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031554.D
Acq On : 16 Jun 2023 01:24
Operator : SY/MD
Sample : 03254-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

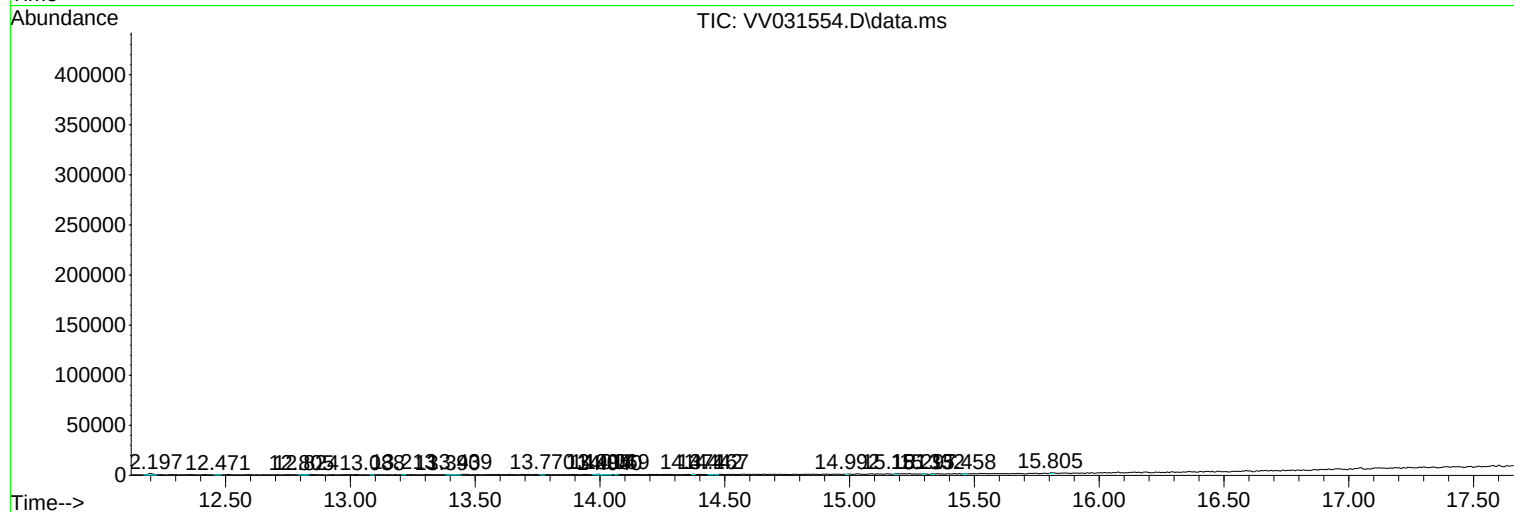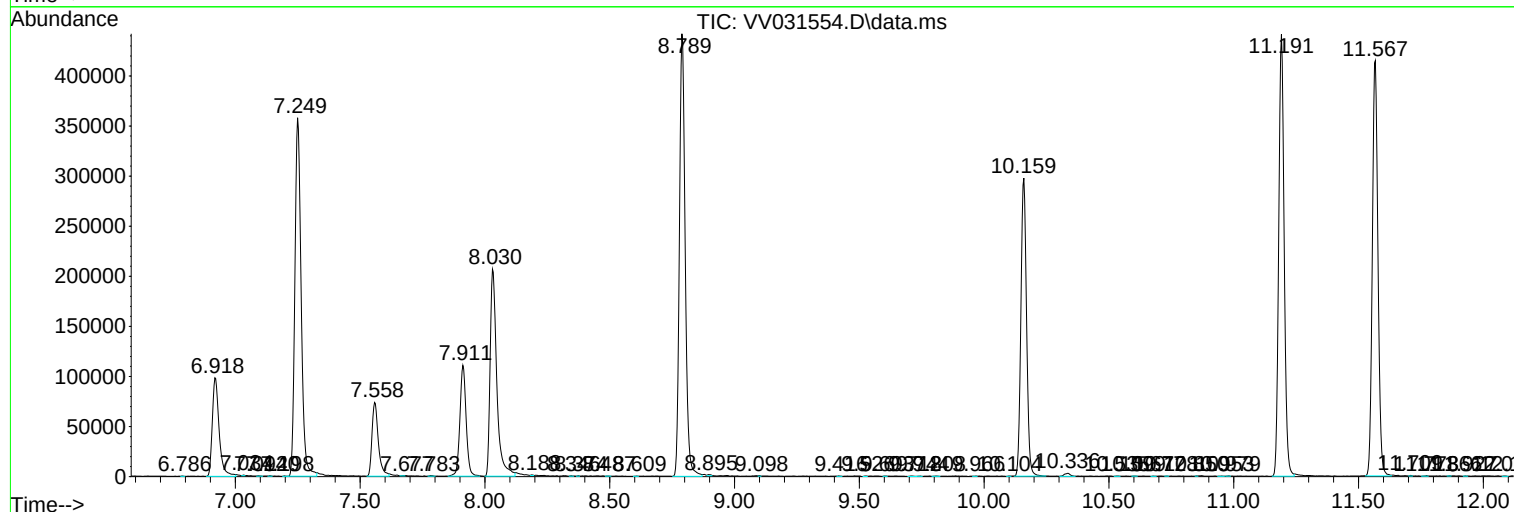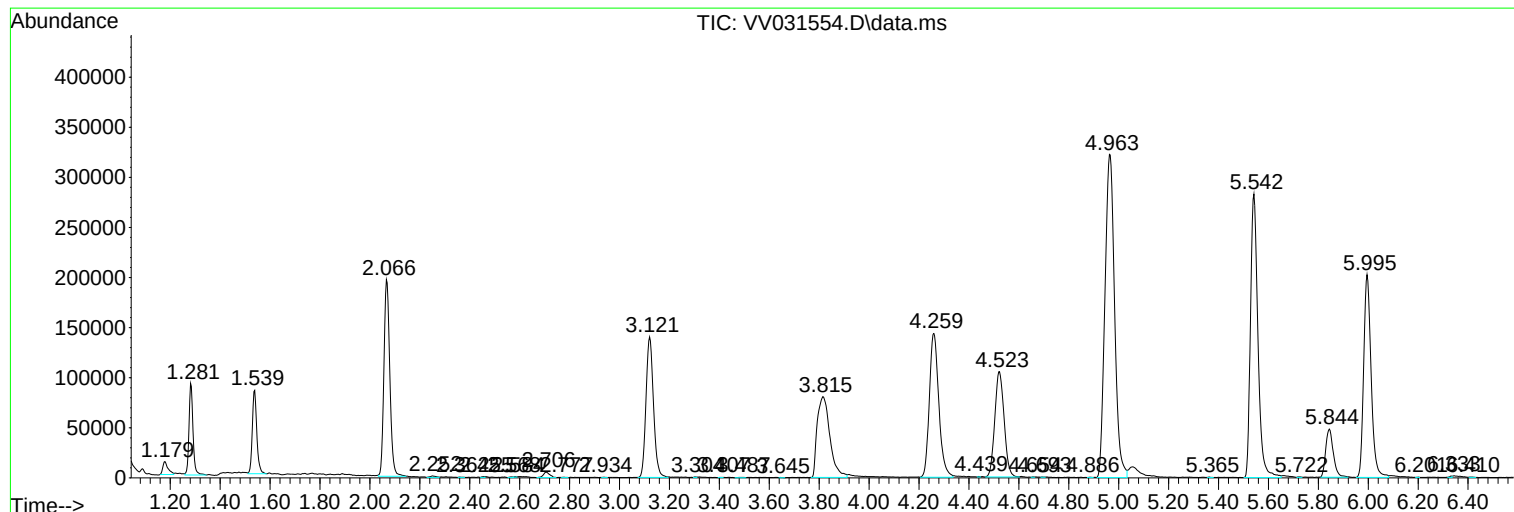

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031554.D
Acq On : 16 Jun 2023 01:24
Operator : SY/MD
Sample : 03254-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031554.D
Acq On : 16 Jun 2023 01:24
Operator : SY/MD
Sample : 03254-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------