

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031555.D
 Acq On : 16 Jun 2023 01:47
 Operator : SY/MD
 Sample : 03254-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	63	rBV	13384	20014	2.29%	0.283%
2	1.282	69	75	97	rVB	88060	93999	10.78%	1.328%
3	1.536	147	154	168	rVB	85488	103801	11.90%	1.467%
4	2.066	308	319	335	rBV2	182414	271234	31.09%	3.832%
5	2.246	370	375	376	rBV3	922	729	0.08%	0.010%
6	2.355	404	409	411	rBV3	542	459	0.05%	0.006%
7	2.452	433	439	445	rVV5	737	784	0.09%	0.011%
8	2.535	462	465	471	rVB3	333	311	0.04%	0.004%
9	2.574	474	477	483	rVV	231	241	0.03%	0.003%
10	2.709	512	519	525	rVB3	387	568	0.07%	0.008%
11	2.738	525	528	534	rVB3	395	404	0.05%	0.006%
12	2.777	535	540	542	rBV	354	233	0.03%	0.003%
13	2.860	564	566	568	rBV	372	255	0.03%	0.004%
14	2.995	606	608	615	rVB2	426	340	0.04%	0.005%
15	3.121	637	647	663	rVB2	3407	7342	0.84%	0.104%
16	3.359	714	721	723	rBV3	520	645	0.07%	0.009%
17	3.519	766	771	775	rVB2	291	288	0.03%	0.004%
18	3.799	848	858	898	rBV	58408	172455	19.77%	2.437%
19	4.259	984	1001	1026	rBV	144555	374761	42.96%	5.295%
20	4.519	1066	1082	1106	rBV2	108542	279859	32.08%	3.954%
21	4.670	1126	1129	1134	rBV3	526	540	0.06%	0.008%
22	4.748	1150	1153	1156	rBV2	329	280	0.03%	0.004%
23	4.963	1203	1220	1247	rBV3	328265	872336	100.00%	12.325%
24	5.314	1326	1329	1333	rBV3	247	241	0.03%	0.003%
25	5.542	1388	1400	1423	rBV	285150	576380	66.07%	8.144%
26	5.751	1462	1465	1471	rVB3	516	518	0.06%	0.007%
27	5.802	1478	1481	1484	rVB2	329	226	0.03%	0.003%
28	5.822	1484	1487	1488	rBV2	1042	588	0.07%	0.008%
29	5.847	1488	1495	1505	rVB8	3146	5972	0.68%	0.084%
30	5.889	1505	1508	1513	rVB	382	312	0.04%	0.004%
31	5.995	1527	1541	1570	rBV	200026	418077	47.93%	5.907%
32	6.191	1598	1602	1607	rBV3	429	407	0.05%	0.006%
33	6.587	1718	1725	1728	rBV2	335	436	0.05%	0.006%
34	6.629	1734	1738	1741	rVB3	436	250	0.03%	0.004%
35	6.706	1759	1762	1767	rBV	301	252	0.03%	0.004%
36	6.918	1817	1828	1859	rBV	96360	184153	21.11%	2.602%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031555.D
 Acq On : 16 Jun 2023 01:47
 Operator : SY/MD
 Sample : 03254-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.198	1911	1915	1919	rBV2	372	359	0.04%	0.005%
38	7.249	1919	1931	1954	rBV	350979	622362	71.34%	8.793%
39	7.429	1984	1987	1989	rBV3	410	218	0.02%	0.003%
40	7.558	2017	2027	2047	rBV	72241	128039	14.68%	1.809%
41	7.751	2082	2087	2090	rBV2	402	354	0.04%	0.005%
42	7.879	2119	2127	2129	rVV5	2568	2893	0.33%	0.041%
43	7.915	2129	2138	2154	rVB3	13907	25517	2.93%	0.361%
44	8.030	2164	2174	2204	rBV	203981	375202	43.01%	5.301%
45	8.542	2329	2333	2338	rBV4	329	405	0.05%	0.006%
46	8.645	2362	2365	2367	rVV2	315	227	0.03%	0.003%
47	8.789	2398	2410	2440	rBV	430267	709800	81.37%	10.029%
48	8.966	2459	2465	2471	rBV5	653	835	0.10%	0.012%
49	8.995	2471	2474	2479	rVB2	390	328	0.04%	0.005%
50	9.082	2496	2501	2505	rBV3	667	724	0.08%	0.010%
51	9.317	2571	2574	2582	rVV3	321	463	0.05%	0.007%
52	9.487	2624	2627	2629	rBV2	447	344	0.04%	0.005%
53	9.635	2666	2673	2675	rBV	272	244	0.03%	0.003%
54	9.876	2744	2748	2750	rBV3	445	267	0.03%	0.004%
55	9.895	2750	2754	2758	rVB2	319	253	0.03%	0.004%
56	10.159	2823	2836	2855	rBV	294396	465154	53.32%	6.572%
57	10.333	2880	2890	2899	rBV3	3253	5115	0.59%	0.072%
58	10.551	2952	2958	2959	rBV2	338	297	0.03%	0.004%
59	10.583	2966	2968	2974	rVB2	442	319	0.04%	0.005%
60	10.738	3014	3016	3020	rVB	293	230	0.03%	0.003%
61	10.786	3026	3031	3033	rBV2	395	263	0.03%	0.004%
62	10.860	3050	3054	3059	rBV3	800	676	0.08%	0.010%
63	10.924	3070	3074	3078	rBV2	416	340	0.04%	0.005%
64	11.062	3112	3117	3121	rBV2	376	361	0.04%	0.005%
65	11.130	3134	3138	3140	rBV	378	332	0.04%	0.005%
66	11.191	3145	3157	3176	rBV	437434	673699	77.23%	9.519%
67	11.513	3252	3257	3261	rBV4	639	717	0.08%	0.010%
68	11.567	3262	3274	3296	rVB	415347	655969	75.20%	9.268%
69	11.648	3296	3299	3302	rBV3	545	340	0.04%	0.005%
70	11.744	3327	3329	3332	rBV2	376	245	0.03%	0.003%
71	12.017	3410	3414	3416	rBV	258	236	0.03%	0.003%
72	12.201	3462	3471	3481	rVV5	1359	2344	0.27%	0.033%
73	12.365	3516	3522	3525	rBV3	411	422	0.05%	0.006%
74	12.513	3562	3568	3572	rBV3	293	329	0.04%	0.005%
75	12.596	3591	3594	3596	rVV	500	334	0.04%	0.005%
76	12.898	3685	3688	3690	rBV	351	252	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031555.D
 Acq On : 16 Jun 2023 01:47
 Operator : SY/MD
 Sample : 03254-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	13.098	3748	3750	3754	rBV2	289	302	0.03%	0.004%
78	13.136	3760	3762	3766	rVB2	557	308	0.04%	0.004%
79	13.159	3766	3769	3776	rBV3	271	271	0.03%	0.004%
80	13.458	3855	3862	3872	rVB4	852	1512	0.17%	0.021%
81	13.545	3885	3889	3891	rBV3	454	305	0.03%	0.004%
82	13.583	3897	3901	3904	rBV2	351	361	0.04%	0.005%
83	13.599	3904	3906	3909	rVV2	618	366	0.04%	0.005%
84	13.664	3923	3926	3929	rVV2	477	375	0.04%	0.005%
85	13.689	3929	3934	3937	rVB4	603	558	0.06%	0.008%
86	13.712	3937	3941	3948	rBV3	382	484	0.06%	0.007%
87	13.831	3974	3978	3982	rBV3	439	371	0.04%	0.005%
88	13.879	3989	3993	3996	rBV3	244	230	0.03%	0.003%
89	13.979	4021	4024	4027	rBV3	558	405	0.05%	0.006%
90	14.021	4033	4037	4042	rVB4	668	701	0.08%	0.010%
91	14.258	4109	4111	4114	rVB4	697	361	0.04%	0.005%
92	14.400	4153	4155	4158	rVB3	518	298	0.03%	0.004%
93	14.467	4172	4176	4178	rBV2	322	281	0.03%	0.004%
94	14.522	4187	4193	4198	rBV4	550	824	0.09%	0.012%
95	14.574	4207	4209	4213	rVB2	435	271	0.03%	0.004%
96	14.869	4298	4301	4303	rVB3	650	301	0.03%	0.004%
97	15.287	4426	4431	4434	rBV5	565	600	0.07%	0.008%
98	15.426	4472	4474	4480	rVB4	797	606	0.07%	0.009%
99	15.455	4480	4483	4485	rBV3	688	451	0.05%	0.006%
100	15.606	4526	4530	4533	rBV3	687	653	0.07%	0.009%




Sum of corrected areas: 7077693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031555.D
Acq On : 16 Jun 2023 01:47
Operator : SY/MD
Sample : 03254-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

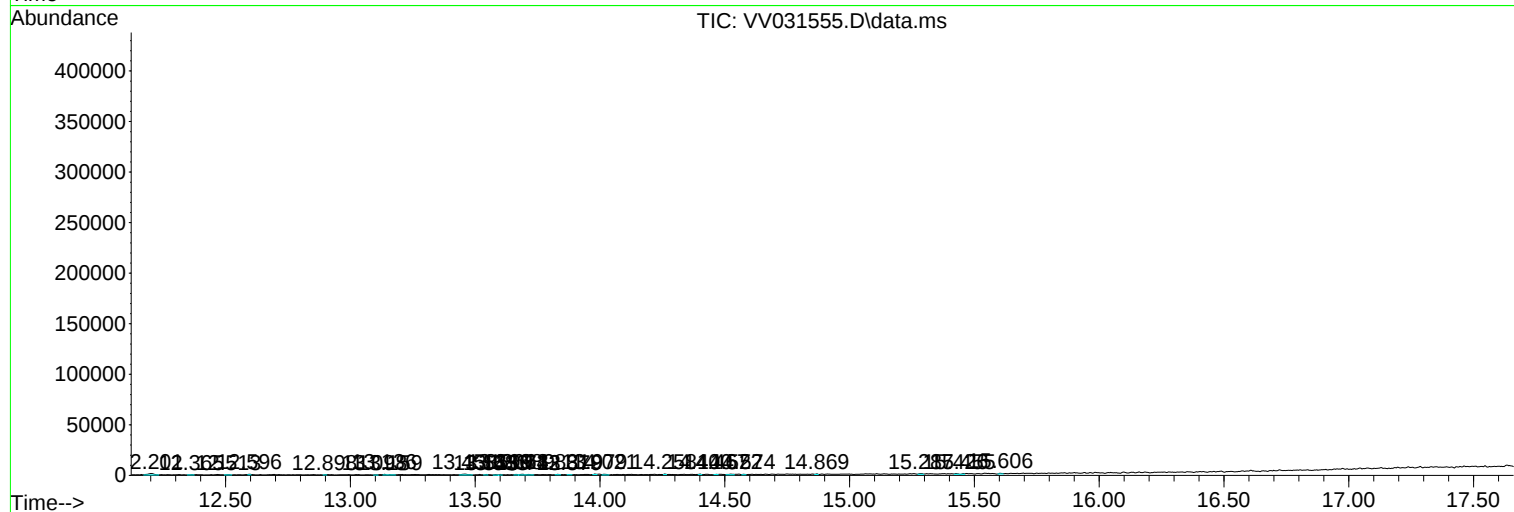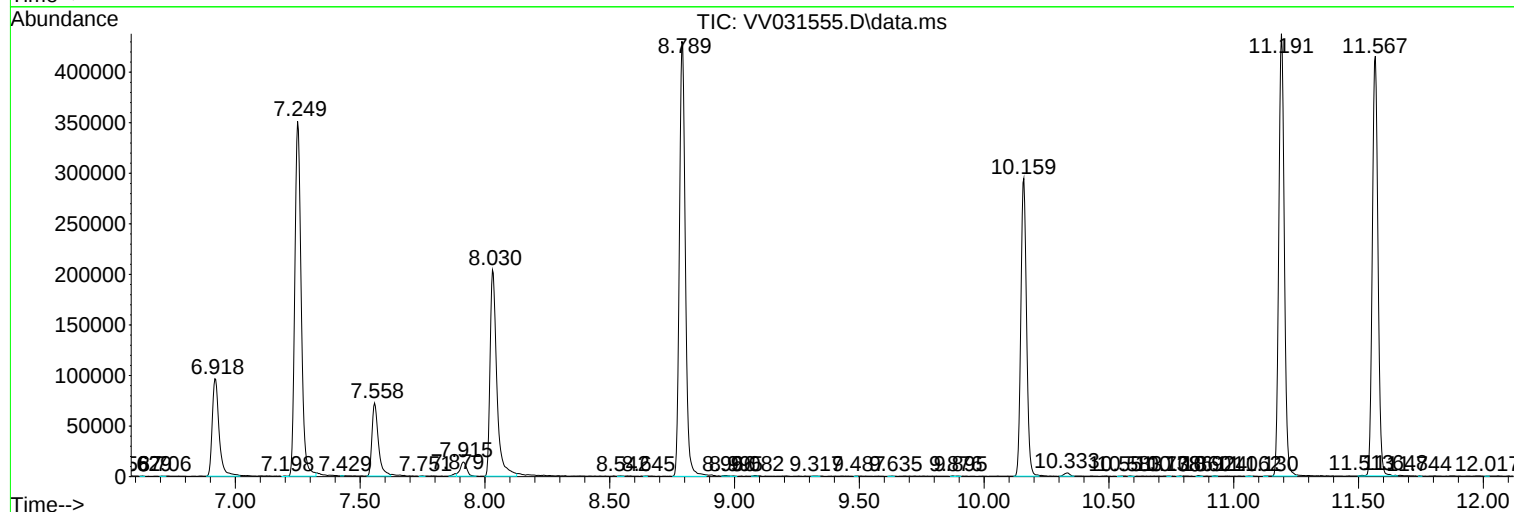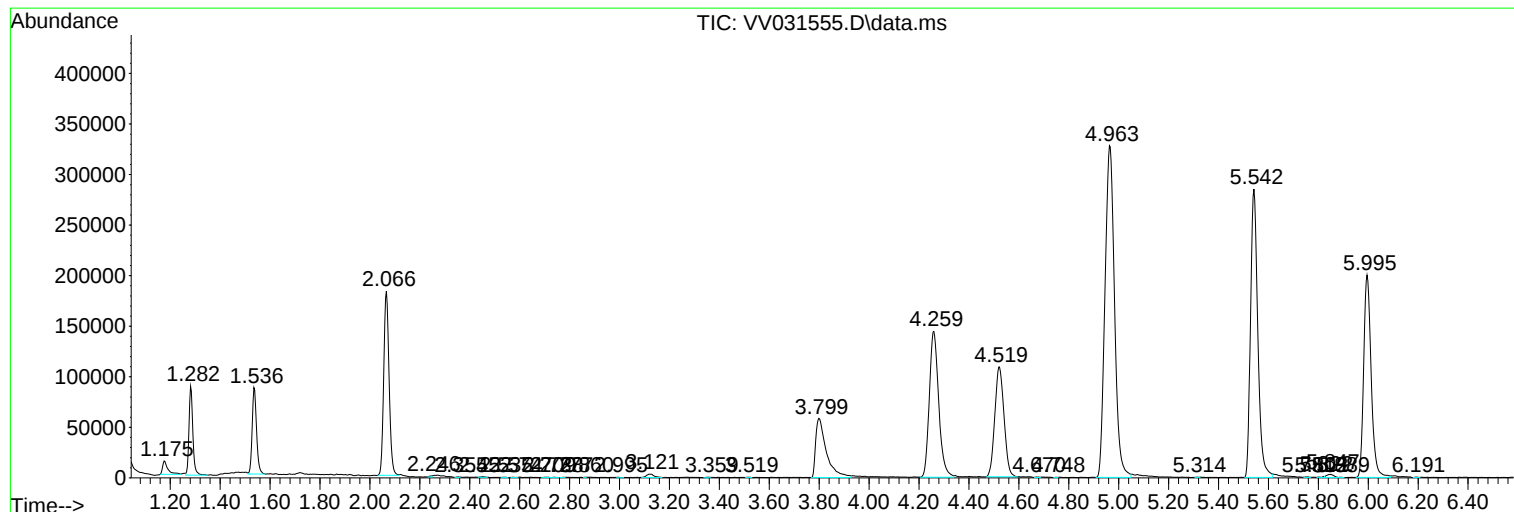

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031555.D
Acq On : 16 Jun 2023 01:47
Operator : SY/MD
Sample : 03254-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031555.D
Acq On : 16 Jun 2023 01:47
Operator : SY/MD
Sample : 03254-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc