

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031556.D
 Acq On : 16 Jun 2023 02:11
 Operator : SY/MD
 Sample : 03254-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	52	rBV	10733	13501	1.00%	0.196%
2	1.281	69	75	88	rVB	67100	71228	5.27%	1.036%
3	1.539	148	155	171	rVB	66360	81903	6.06%	1.191%
4	2.066	310	319	334	rBV3	150202	236782	17.53%	3.445%
5	2.387	416	419	421	rBV2	476	359	0.03%	0.005%
6	2.706	509	518	529	rBV6	2535	4891	0.36%	0.071%
7	2.796	542	546	551	rBV2	232	328	0.02%	0.005%
8	2.928	584	587	590	rBV	349	204	0.02%	0.003%
9	3.121	635	647	670	rBV	25348	52188	3.86%	0.759%
10	3.246	684	686	687	rBV	169	70	0.01%	0.001%
11	3.294	699	701	706	rBV2	124	99	0.01%	0.001%
12	3.416	738	739	740	rBV2	121	35	0.00%	0.001%
13	3.474	749	757	763	rBV2	297	557	0.04%	0.008%
14	3.542	773	778	780	rBV2	379	248	0.02%	0.004%
15	3.629	802	805	806	rBV2	154	99	0.01%	0.001%
16	3.712	828	831	834	rBV2	193	133	0.01%	0.002%
17	3.735	834	838	839	rBV	197	131	0.01%	0.002%
18	3.757	843	845	846	rBV	145	76	0.01%	0.001%
19	3.802	849	859	898	rBV2	58016	192070	14.22%	2.794%
20	4.259	986	1001	1029	rBV	113848	295647	21.88%	4.301%
21	4.519	1063	1082	1115	rBV	526215	1350956	100.00%	19.653%
22	4.838	1176	1181	1187	rVB3	471	593	0.04%	0.009%
23	4.866	1187	1190	1193	rBV2	287	232	0.02%	0.003%
24	4.966	1204	1221	1246	rBV2	253407	680762	50.39%	9.903%
25	5.259	1308	1312	1314	rBV2	304	224	0.02%	0.003%
26	5.333	1332	1335	1336	rBV	226	111	0.01%	0.002%
27	5.378	1347	1349	1355	rBV2	193	133	0.01%	0.002%
28	5.542	1385	1400	1427	rBV	215383	447256	33.11%	6.507%
29	5.847	1485	1495	1507	rBV9	5253	12014	0.89%	0.175%
30	5.995	1528	1541	1567	rBV	160597	331987	24.57%	4.830%
31	6.281	1627	1630	1631	rBV	201	101	0.01%	0.001%
32	6.577	1721	1722	1723	rBV	150	41	0.00%	0.001%
33	6.590	1723	1726	1729	rBV2	308	265	0.02%	0.004%
34	6.638	1737	1741	1742	rBV	350	211	0.02%	0.003%
35	6.921	1818	1829	1861	rBV2	73847	143769	10.64%	2.092%
36	7.088	1877	1881	1889	rBV3	338	506	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031556.D
 Acq On : 16 Jun 2023 02:11
 Operator : SY/MD
 Sample : 03254-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.153	1899	1901	1902	rBV	330	138	0.01%	0.002%
38	7.188	1908	1912	1914	rBV2	467	375	0.03%	0.005%
39	7.249	1919	1931	1950	rBV	266988	470120	34.80%	6.839%
40	7.471	1997	2000	2001	rBV	355	190	0.01%	0.003%
41	7.558	2018	2027	2060	rBV	57503	105196	7.79%	1.530%
42	7.754	2086	2088	2090	rBV	271	180	0.01%	0.003%
43	7.783	2090	2097	2100	rBV2	2014	2533	0.19%	0.037%
44	7.911	2118	2137	2154	rBV5	28961	54679	4.05%	0.795%
45	8.030	2164	2174	2204	rBV	186845	347663	25.73%	5.058%
46	8.355	2271	2275	2277	rBV	309	275	0.02%	0.004%
47	8.683	2375	2377	2381	rBV2	186	87	0.01%	0.001%
48	8.792	2398	2411	2436	rBV	331273	551070	40.79%	8.017%
49	8.960	2460	2463	2470	rBV3	1283	1293	0.10%	0.019%
50	9.034	2484	2486	2490	rVB	339	157	0.01%	0.002%
51	9.088	2497	2503	2511	rBV3	1324	1991	0.15%	0.029%
52	9.358	2579	2587	2589	rBV2	453	520	0.04%	0.008%
53	9.471	2619	2622	2623	rBV	266	152	0.01%	0.002%
54	9.612	2664	2666	2669	rBV	181	99	0.01%	0.001%
55	9.667	2679	2683	2684	rBV2	535	389	0.03%	0.006%
56	9.853	2739	2741	2742	rBV	205	106	0.01%	0.002%
57	9.879	2745	2749	2754	rVV3	1061	1183	0.09%	0.017%
58	9.905	2754	2757	2759	rVB2	282	138	0.01%	0.002%
59	10.066	2803	2807	2810	rBV2	312	326	0.02%	0.005%
60	10.159	2825	2836	2856	rBV	253860	398429	29.49%	5.796%
61	10.262	2866	2868	2871	rBV2	169	100	0.01%	0.001%
62	10.291	2875	2877	2879	rVV2	343	185	0.01%	0.003%
63	10.329	2882	2889	2900	rVB3	3536	5527	0.41%	0.080%
64	10.487	2927	2938	2948	rBV4	946	1722	0.13%	0.025%
65	10.567	2960	2963	2966	rBV2	176	172	0.01%	0.003%
66	10.648	2986	2988	2989	rBV	201	61	0.00%	0.001%
67	10.696	2999	3003	3006	rBV2	517	466	0.03%	0.007%
68	10.744	3014	3018	3020	rVB2	355	276	0.02%	0.004%
69	10.757	3020	3022	3023	rBV2	111	43	0.00%	0.001%
70	10.783	3023	3030	3036	rBV3	333	553	0.04%	0.008%
71	10.863	3050	3055	3063	rVB5	1618	1979	0.15%	0.029%
72	10.979	3089	3091	3094	rBV5	171	112	0.01%	0.002%
73	11.059	3114	3116	3121	rVB2	351	166	0.01%	0.002%
74	11.191	3146	3157	3181	rBV	332067	510583	37.79%	7.428%
75	11.567	3262	3274	3293	rBV	312122	489749	36.25%	7.125%
76	11.812	3346	3350	3354	rBV2	425	386	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031556.D
 Acq On : 16 Jun 2023 02:11
 Operator : SY/MD
 Sample : 03254-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.021	3413	3415	3422	rBV2	275	292	0.02%	0.004%
78	12.133	3448	3450	3451	rBV	309	116	0.01%	0.002%
79	12.365	3520	3522	3524	rBV	289	110	0.01%	0.002%
80	12.590	3589	3592	3597	rBV3	785	887	0.07%	0.013%
81	12.709	3627	3629	3630	rBV3	268	96	0.01%	0.001%
82	12.818	3660	3663	3667	rBV2	358	317	0.02%	0.005%
83	13.088	3744	3747	3750	rBV2	435	244	0.02%	0.004%
84	13.204	3780	3783	3791	rVB5	1134	1157	0.09%	0.017%
85	13.294	3807	3811	3814	rBV3	472	457	0.03%	0.007%
86	13.721	3940	3944	3947	rBV3	376	335	0.02%	0.005%
87	13.792	3963	3966	3967	rBV	342	192	0.01%	0.003%
88	13.924	4004	4007	4008	rBV	343	176	0.01%	0.003%
89	14.127	4066	4070	4071	rBV2	392	268	0.02%	0.004%
90	14.188	4086	4089	4090	rBV3	390	228	0.02%	0.003%




Sum of corrected areas: 6873954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031556.D
Acq On : 16 Jun 2023 02:11
Operator : SY/MD
Sample : 03254-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

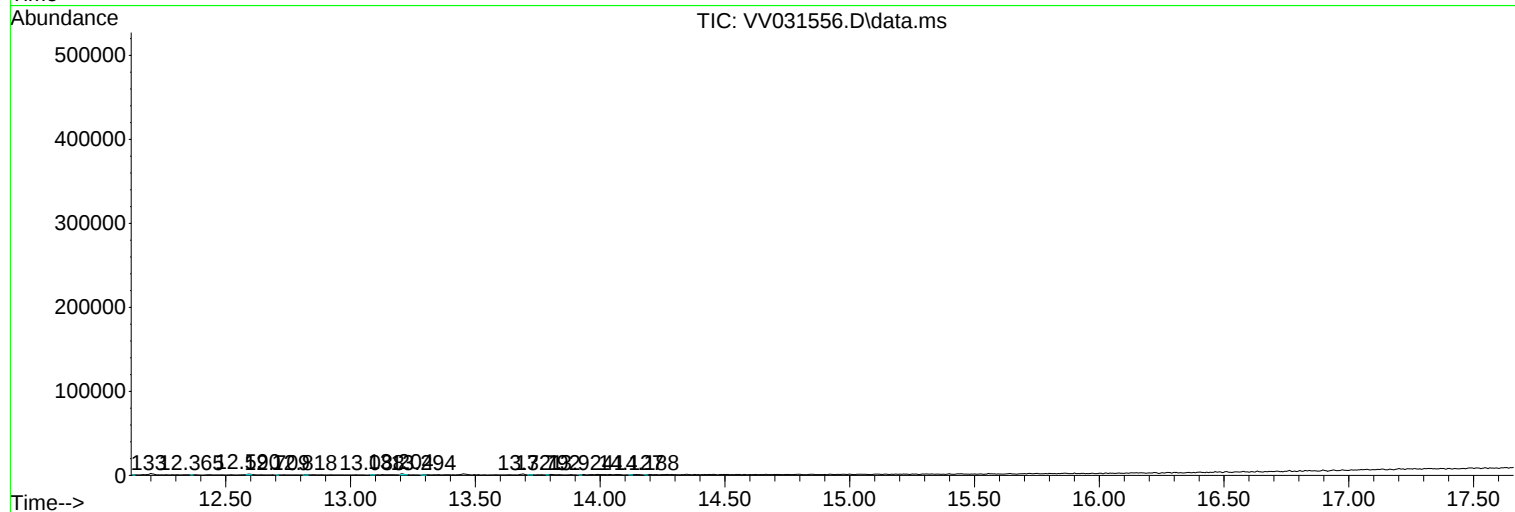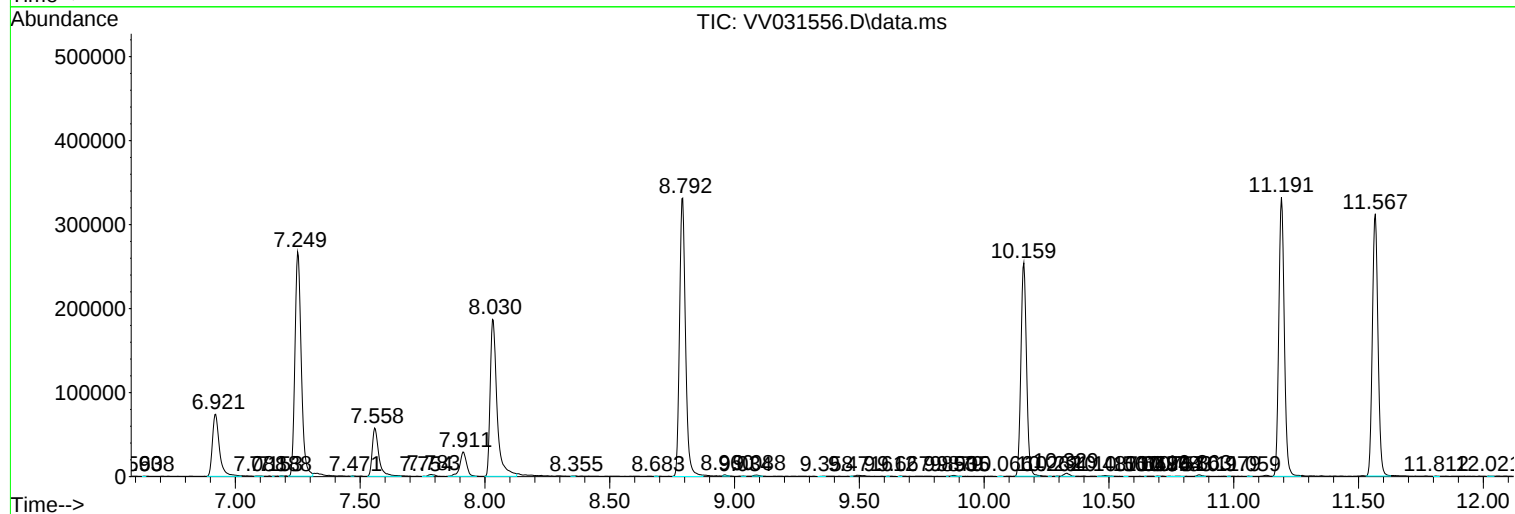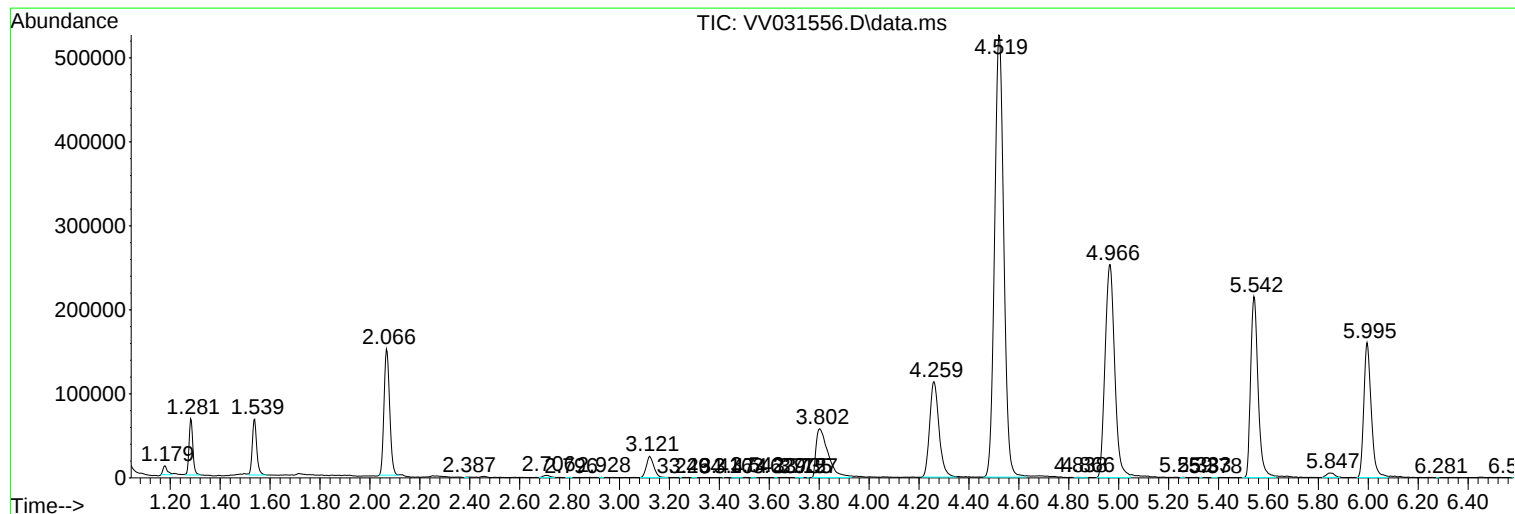

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031556.D
Acq On : 16 Jun 2023 02:11
Operator : SY/MD
Sample : 03254-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031556.D
Acq On : 16 Jun 2023 02:11
Operator : SY/MD
Sample : 03254-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc