

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031557.D
 Acq On : 16 Jun 2023 02:34
 Operator : SY/MD
 Sample : 03254-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	94483	102161	5.91%	1.166%
2	1.536	148	154	171	rVB	85822	108715	6.29%	1.241%
3	2.066	309	319	334	rVB	177974	260909	15.09%	2.977%
4	2.359	407	410	412	rBV	341	275	0.02%	0.003%
5	2.462	435	442	447	rBV3	909	1024	0.06%	0.012%
6	2.532	461	464	467	rBV2	291	248	0.01%	0.003%
7	2.651	498	501	507	rVB2	230	285	0.02%	0.003%
8	2.677	507	509	510	rBV2	249	118	0.01%	0.001%
9	2.712	511	520	533	rVB6	3886	7457	0.43%	0.085%
10	2.786	541	543	546	rBV	176	111	0.01%	0.001%
11	2.864	565	567	571	rBV	283	182	0.01%	0.002%
12	2.931	585	588	590	rBV	152	96	0.01%	0.001%
13	3.063	623	629	633	rBV2	444	463	0.03%	0.005%
14	3.121	634	647	668	rBV	63422	133865	7.74%	1.528%
15	3.285	695	698	700	rBV2	196	145	0.01%	0.002%
16	3.298	700	702	704	rVV	219	102	0.01%	0.001%
17	3.355	718	720	721	rBV	143	64	0.00%	0.001%
18	3.368	721	724	725	rVV	166	76	0.00%	0.001%
19	3.439	743	746	753	rBV2	357	465	0.03%	0.005%
20	3.677	817	820	824	rBV	338	290	0.02%	0.003%
21	3.802	847	859	889	rBV2	63025	214348	12.40%	2.446%
22	4.259	983	1001	1036	rBV	147010	380092	21.99%	4.338%
23	4.519	1064	1082	1114	rBV	672515	1728611	100.00%	19.726%
24	4.844	1181	1183	1187	rBV	161	125	0.01%	0.001%
25	4.863	1187	1189	1190	rBV	297	146	0.01%	0.002%
26	4.963	1203	1220	1251	rBV2	319725	867147	50.16%	9.896%
27	5.343	1335	1338	1343	rVB2	386	267	0.02%	0.003%
28	5.368	1343	1346	1348	rBV	203	177	0.01%	0.002%
29	5.439	1363	1368	1372	rBV3	296	310	0.02%	0.004%
30	5.474	1377	1379	1380	rVB3	272	74	0.00%	0.001%
31	5.542	1388	1400	1435	rBV	278243	577255	33.39%	6.587%
32	5.847	1484	1495	1517	rVB4	18209	39329	2.28%	0.449%
33	5.995	1527	1541	1564	rBV	201478	416407	24.09%	4.752%
34	6.207	1604	1607	1610	rBV2	350	234	0.01%	0.003%
35	6.227	1610	1613	1616	rBV3	493	261	0.02%	0.003%
36	6.265	1622	1625	1628	rBV	246	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031557.D
 Acq On : 16 Jun 2023 02:34
 Operator : SY/MD
 Sample : 03254-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.297	1633	1635	1638	rVV2	283	139	0.01%	0.002%
38	6.330	1642	1645	1648	rVB2	351	208	0.01%	0.002%
39	6.558	1713	1716	1719	rBV2	281	177	0.01%	0.002%
40	6.593	1724	1727	1729	rBV	198	134	0.01%	0.002%
41	6.629	1736	1738	1740	rBV	384	108	0.01%	0.001%
42	6.799	1788	1791	1792	rBV	183	93	0.01%	0.001%
43	6.825	1798	1799	1800	rBV	151	47	0.00%	0.001%
44	6.860	1807	1810	1812	rBV2	189	114	0.01%	0.001%
45	6.918	1817	1828	1853	rBV2	95914	181790	10.52%	2.075%
46	7.162	1902	1904	1906	rBV2	278	121	0.01%	0.001%
47	7.249	1920	1931	1959	rBV	349230	615449	35.60%	7.023%
48	7.477	2000	2002	2007	rVB3	342	257	0.01%	0.003%
49	7.558	2017	2027	2051	rBV	74566	132836	7.68%	1.516%
50	7.915	2119	2138	2154	rBV5	35259	66575	3.85%	0.760%
51	8.031	2164	2174	2213	rBV	204413	380962	22.04%	4.347%
52	8.333	2266	2268	2273	rVB3	419	261	0.02%	0.003%
53	8.432	2296	2299	2308	rVB4	378	334	0.02%	0.004%
54	8.545	2331	2334	2338	rVB3	280	197	0.01%	0.002%
55	8.622	2355	2358	2359	rBV	168	75	0.00%	0.001%
56	8.789	2398	2410	2434	rBV	430097	700463	40.52%	7.994%
57	8.960	2459	2463	2465	rBV2	712	635	0.04%	0.007%
58	9.082	2499	2501	2502	rBV	384	155	0.01%	0.002%
59	9.548	2644	2646	2647	rBV	194	93	0.01%	0.001%
60	9.622	2666	2669	2670	rBV	287	187	0.01%	0.002%
61	9.645	2671	2676	2684	rVB6	1458	2036	0.12%	0.023%
62	9.744	2701	2707	2710	rBV2	677	703	0.04%	0.008%
63	9.963	2774	2775	2776	rBV2	125	29	0.00%	0.000%
64	9.989	2776	2783	2787	rVV	376	473	0.03%	0.005%
65	10.069	2804	2808	2810	rBV3	606	519	0.03%	0.006%
66	10.117	2820	2823	2824	rBV	260	133	0.01%	0.002%
67	10.159	2824	2836	2857	rVV	299401	470221	27.20%	5.366%
68	10.329	2884	2889	2898	rVB4	4074	5796	0.34%	0.066%
69	10.487	2930	2938	2947	rVB3	1670	2148	0.12%	0.025%
70	10.683	2993	2999	3007	rVB5	1513	2258	0.13%	0.026%
71	10.863	3048	3055	3064	rVB4	4259	6021	0.35%	0.069%
72	10.921	3064	3073	3076	rBV2	310	534	0.03%	0.006%
73	10.985	3091	3093	3094	rBV2	283	95	0.01%	0.001%
74	11.137	3137	3140	3146	rVB2	588	708	0.04%	0.008%
75	11.191	3146	3157	3176	rBV	448580	683181	39.52%	7.796%
76	11.567	3263	3274	3298	rVB	419981	659401	38.15%	7.525%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031557.D
 Acq On : 16 Jun 2023 02:34
 Operator : SY/MD
 Sample : 03254-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.715	3318	3320	3324	rBV4	396	223	0.01%	0.003%
78	11.863	3359	3366	3370	rBV4	986	1482	0.09%	0.017%
79	12.095	3435	3438	3440	rBV3	525	344	0.02%	0.004%
80	12.191	3463	3468	3470	rBV3	1262	1110	0.06%	0.013%
81	12.529	3570	3573	3576	rVB3	323	185	0.01%	0.002%
82	12.590	3589	3592	3597	rBV3	645	639	0.04%	0.007%
83	12.902	3688	3689	3691	rVB3	344	86	0.00%	0.001%
84	13.519	3878	3881	3884	rBV2	574	405	0.02%	0.005%
85	13.673	3927	3929	3932	rBV	325	203	0.01%	0.002%
86	13.863	3986	3988	3990	rBV	351	100	0.01%	0.001%
87	14.178	4084	4086	4089	rBV	437	269	0.02%	0.003%
88	14.194	4089	4091	4092	rBV	346	157	0.01%	0.002%




Sum of corrected areas: 8762894

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031557.D
Acq On : 16 Jun 2023 02:34
Operator : SY/MD
Sample : 03254-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

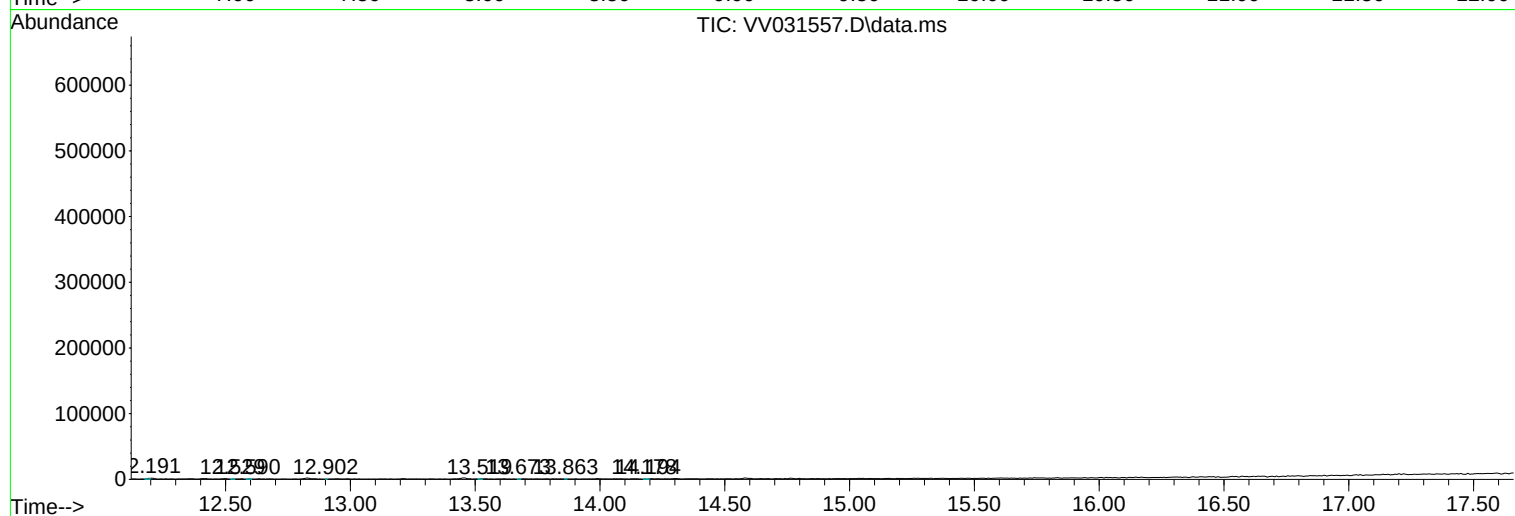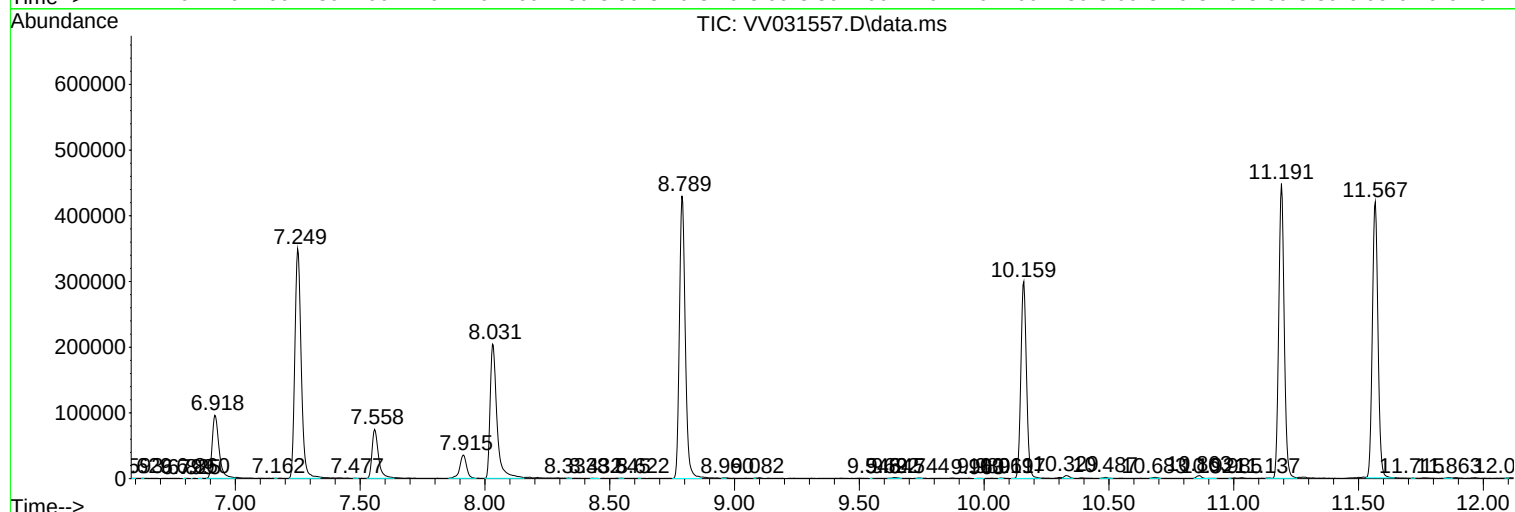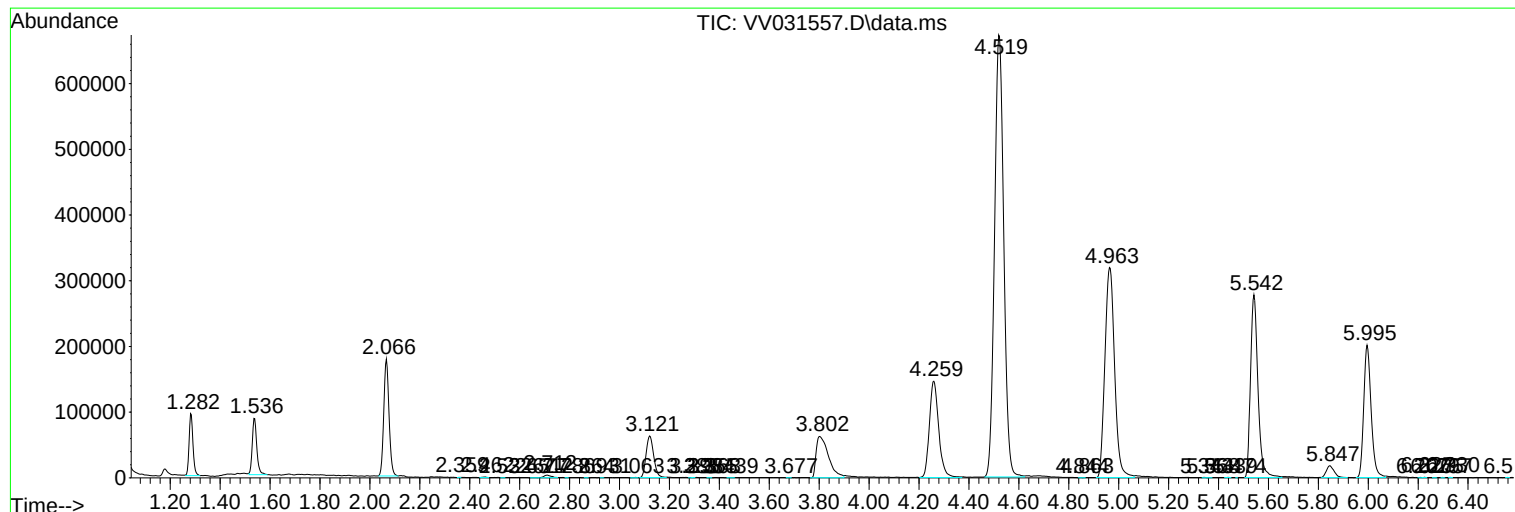

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031557.D
Acq On : 16 Jun 2023 02:34
Operator : SY/MD
Sample : 03254-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031557.D
Acq On : 16 Jun 2023 02:34
Operator : SY/MD
Sample : 03254-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc