

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031558.D
 Acq On : 16 Jun 2023 02:57
 Operator : SY/MD
 Sample : 03254-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	53	rBV	11455	17576	1.92%	0.219%
2	1.282	69	75	88	rVB	93619	99856	10.93%	1.243%
3	1.536	147	154	170	rVB	89418	108760	11.90%	1.354%
4	2.066	308	319	338	rBV3	207588	332560	36.39%	4.140%
5	2.259	369	379	383	rBV6	1829	3386	0.37%	0.042%
6	2.397	420	422	428	rVB3	437	350	0.04%	0.004%
7	2.452	434	439	441	rBV4	649	591	0.06%	0.007%
8	2.606	477	487	491	rBV5	875	1399	0.15%	0.017%
9	2.706	511	518	530	rVB4	5117	8815	0.96%	0.110%
10	2.793	541	545	548	rBV2	387	351	0.04%	0.004%
11	2.957	592	596	599	rBV2	298	270	0.03%	0.003%
12	2.999	604	609	613	rVB2	226	289	0.03%	0.004%
13	3.121	630	647	670	rBV	137752	294972	32.28%	3.672%
14	3.240	681	684	692	rVB2	369	428	0.05%	0.005%
15	3.536	772	776	779	rVB2	360	308	0.03%	0.004%
16	3.564	779	785	788	rBV2	404	364	0.04%	0.005%
17	3.812	848	862	891	rBV3	81557	296882	32.49%	3.696%
18	4.259	984	1001	1031	rBV	152084	394990	43.22%	4.918%
19	4.523	1065	1083	1105	rBV2	106499	271050	29.66%	3.374%
20	4.699	1135	1138	1142	rVB3	375	301	0.03%	0.004%
21	4.886	1190	1196	1200	rBV	245	257	0.03%	0.003%
22	4.963	1203	1220	1243	rBV2	339183	913843	100.00%	11.377%
23	5.227	1299	1302	1305	rVB2	563	308	0.03%	0.004%
24	5.542	1387	1400	1428	rBV	284911	588266	64.37%	7.324%
25	5.744	1461	1463	1468	rVB3	488	251	0.03%	0.003%
26	5.844	1482	1494	1515	rBV3	50480	104185	11.40%	1.297%
27	5.921	1515	1518	1523	rVB4	936	824	0.09%	0.010%
28	5.995	1527	1541	1563	rBV	213081	439473	48.09%	5.471%
29	6.198	1601	1604	1610	rBV3	558	409	0.04%	0.005%
30	6.336	1641	1647	1648	rBV3	1821	1769	0.19%	0.022%
31	6.918	1817	1828	1854	rBV2	100806	190114	20.80%	2.367%
32	7.249	1920	1931	1951	rBV	367233	649400	71.06%	8.085%
33	7.465	1996	1998	2002	rVB2	521	378	0.04%	0.005%
34	7.558	2017	2027	2050	rBV	77452	137823	15.08%	1.716%
35	7.658	2056	2058	2064	rVB3	585	455	0.05%	0.006%
36	7.712	2072	2075	2077	rBV	458	258	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061523\
 Data File : VW031558.D
 Acq On : 16 Jun 2023 02:57
 Operator : SY/MD
 Sample : 03254-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.741	2082	2084	2090	rVB3	557	439	0.05%	0.005%
38	7.786	2090	2098	2108	rBV5	934	1308	0.14%	0.016%
39	7.912	2115	2137	2163	rVB	114818	199667	21.85%	2.486%
40	8.031	2164	2174	2200	rBV	219665	402169	44.01%	5.007%
41	8.394	2285	2287	2294	rVB4	517	486	0.05%	0.006%
42	8.484	2310	2315	2319	rBV3	342	285	0.03%	0.004%
43	8.606	2350	2353	2357	rVB2	419	347	0.04%	0.004%
44	8.635	2357	2362	2366	rBV3	370	389	0.04%	0.005%
45	8.789	2397	2410	2435	rBV	431729	710964	77.80%	8.851%
46	8.982	2468	2470	2477	rVB3	591	565	0.06%	0.007%
47	9.024	2478	2483	2490	rBV3	472	500	0.05%	0.006%
48	9.059	2490	2494	2498	rBV2	336	317	0.03%	0.004%
49	9.085	2500	2502	2511	rVB4	667	809	0.09%	0.010%
50	9.127	2511	2515	2518	rBV	457	413	0.05%	0.005%
51	9.198	2534	2537	2541	rBV	314	256	0.03%	0.003%
52	9.272	2558	2560	2568	rVB2	283	311	0.03%	0.004%
53	9.439	2607	2612	2613	rBV2	291	248	0.03%	0.003%
54	9.815	2722	2729	2733	rBV2	280	358	0.04%	0.004%
55	9.850	2734	2740	2744	rVB2	255	268	0.03%	0.003%
56	9.876	2744	2748	2749	rBV2	405	285	0.03%	0.004%
57	9.931	2762	2765	2769	rBV2	411	348	0.04%	0.004%
58	10.114	2817	2822	2824	rBV2	446	388	0.04%	0.005%
59	10.159	2824	2836	2861	rVV	318690	497789	54.47%	6.197%
60	10.297	2874	2879	2882	rBV3	373	400	0.04%	0.005%
61	10.333	2882	2890	2899	rVB2	3405	5092	0.56%	0.063%
62	10.863	3049	3055	3056	rBV2	524	410	0.04%	0.005%
63	10.924	3069	3074	3082	rVB2	375	495	0.05%	0.006%
64	10.969	3083	3088	3092	rBV	222	295	0.03%	0.004%
65	11.021	3099	3104	3106	rBV2	270	257	0.03%	0.003%
66	11.191	3146	3157	3180	rBV	430804	659509	72.17%	8.211%
67	11.294	3185	3189	3192	rVB2	332	303	0.03%	0.004%
68	11.352	3204	3207	3211	rBV2	486	466	0.05%	0.006%
69	11.513	3250	3257	3261	rBV4	1386	1796	0.20%	0.022%
70	11.567	3261	3274	3295	rVV	434605	669383	73.25%	8.334%
71	11.693	3311	3313	3318	rVB2	482	336	0.04%	0.004%
72	11.722	3318	3322	3328	rVB3	478	473	0.05%	0.006%
73	11.905	3376	3379	3384	rVB2	476	408	0.04%	0.005%
74	11.937	3384	3389	3396	rBV2	407	667	0.07%	0.008%
75	12.046	3418	3423	3428	rBV2	301	316	0.03%	0.004%
76	12.198	3468	3470	3482	rVB5	1035	981	0.11%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
 Data File : VV031558.D
 Acq On : 16 Jun 2023 02:57
 Operator : SY/MD
 Sample : 03254-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.275	3489	3494	3496	rBV3	304	271	0.03%	0.003%
78	12.342	3512	3515	3520	rBV3	275	259	0.03%	0.003%
79	12.651	3608	3611	3614	rBV2	409	273	0.03%	0.003%
80	12.792	3652	3655	3659	rBV2	359	341	0.04%	0.004%
81	12.812	3659	3661	3668	rVB2	301	281	0.03%	0.003%
82	12.982	3707	3714	3717	rBV2	457	599	0.07%	0.007%
83	13.152	3764	3767	3770	rBV	372	281	0.03%	0.003%
84	13.458	3853	3862	3868	rBV4	803	1332	0.15%	0.017%
85	13.484	3868	3870	3875	rVB	330	249	0.03%	0.003%
86	13.538	3884	3887	3891	rVB3	444	361	0.04%	0.004%
87	13.564	3891	3895	3899	rBV2	568	583	0.06%	0.007%
88	13.689	3930	3934	3941	rBV5	592	635	0.07%	0.008%
89	13.725	3942	3945	3949	rVB2	387	330	0.04%	0.004%
90	13.837	3977	3980	3983	rBV2	352	258	0.03%	0.003%
91	13.943	4010	4013	4015	rBV2	386	264	0.03%	0.003%
92	14.252	4106	4109	4112	rVB	536	343	0.04%	0.004%
93	14.297	4118	4123	4124	rBV	400	266	0.03%	0.003%
94	14.342	4134	4137	4139	rBV	420	277	0.03%	0.003%
95	14.567	4203	4207	4210	rBV3	489	456	0.05%	0.006%
96	14.805	4279	4281	4287	rVB2	392	327	0.04%	0.004%
97	14.876	4298	4303	4307	rBV3	505	604	0.07%	0.008%
98	15.043	4349	4355	4358	rBV3	609	765	0.08%	0.010%
99	15.149	4384	4388	4389	rBV2	898	609	0.07%	0.008%
100	15.313	4436	4439	4441	rBV2	561	347	0.04%	0.004%



Sum of corrected areas: 8032318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031558.D
Acq On : 16 Jun 2023 02:57
Operator : SY/MD
Sample : 03254-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

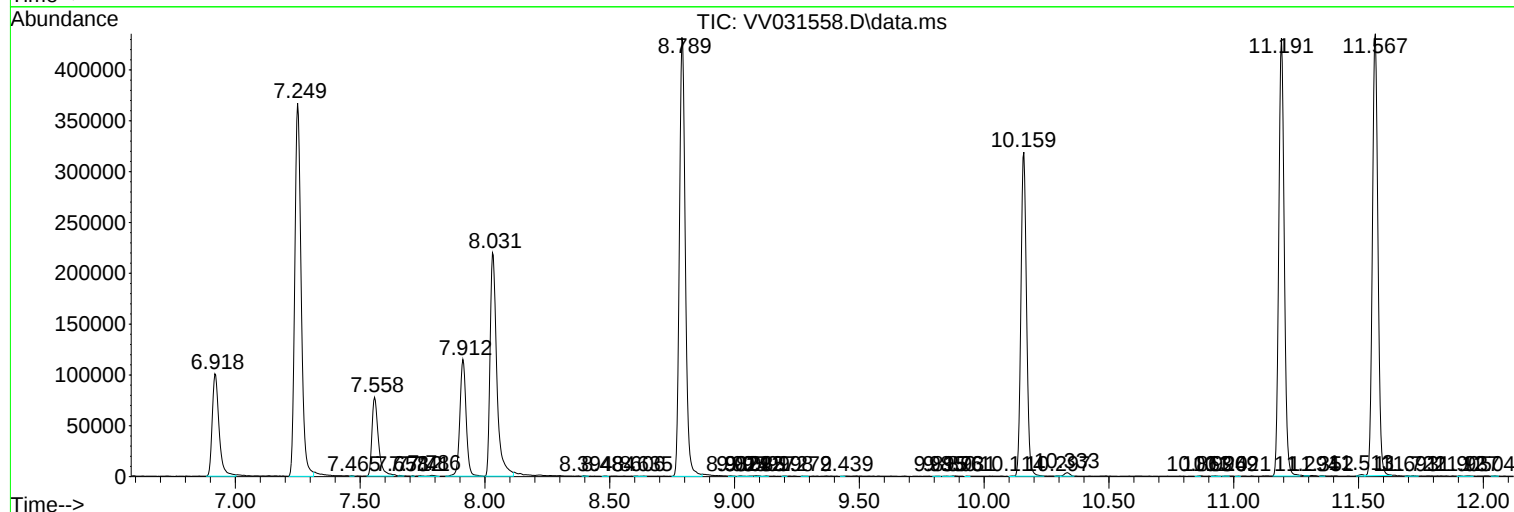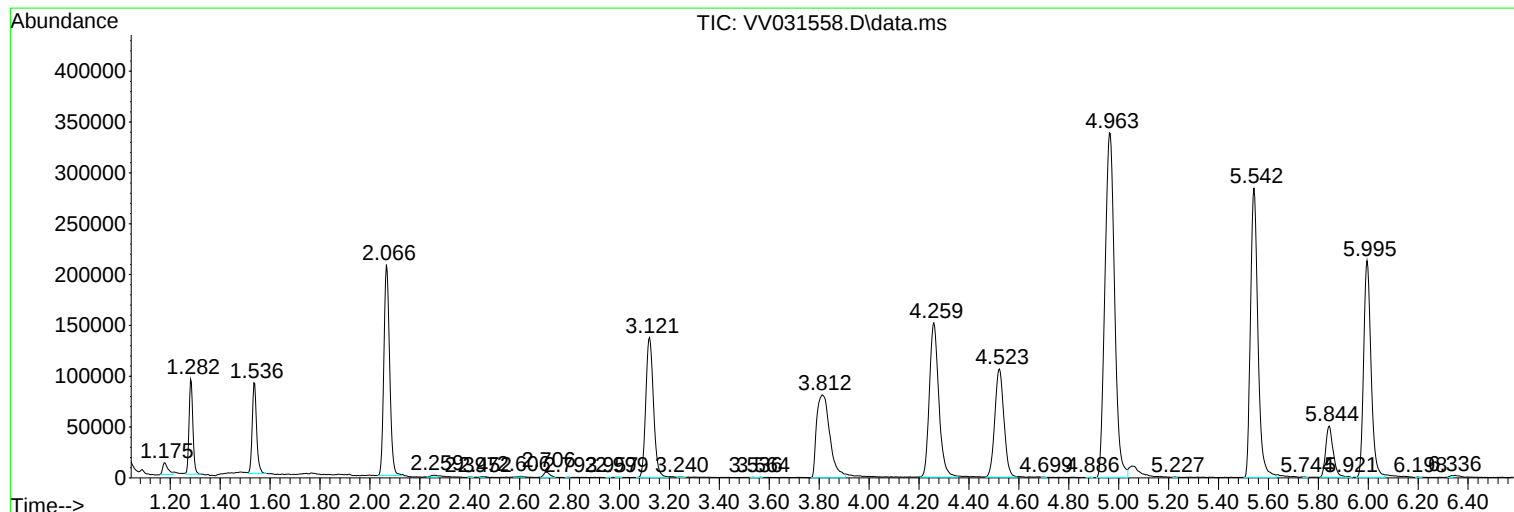

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031558.D
Acq On : 16 Jun 2023 02:57
Operator : SY/MD
Sample : 03254-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031558.D
Acq On : 16 Jun 2023 02:57
Operator : SY/MD
Sample : 03254-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------