
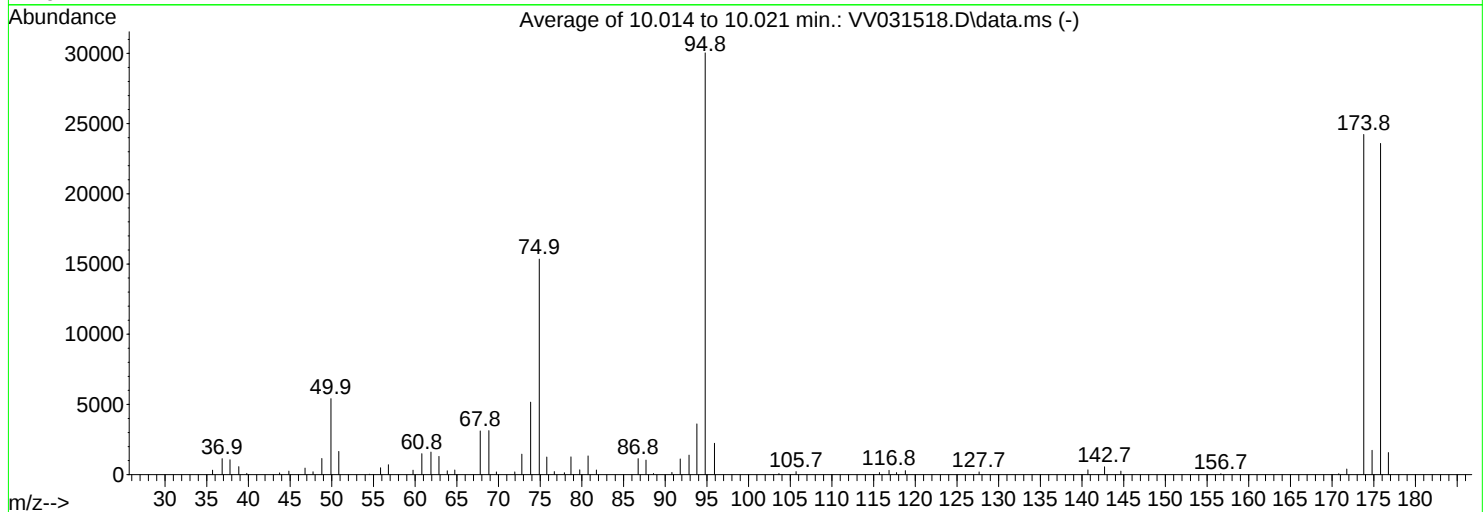


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061523\
Data File : VV031518.D
Acq On : 15 Jun 2023 09:12
Operator : SY/MD
Sample : BFB388
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB388

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Sat Jun 17 02:08:04 2023

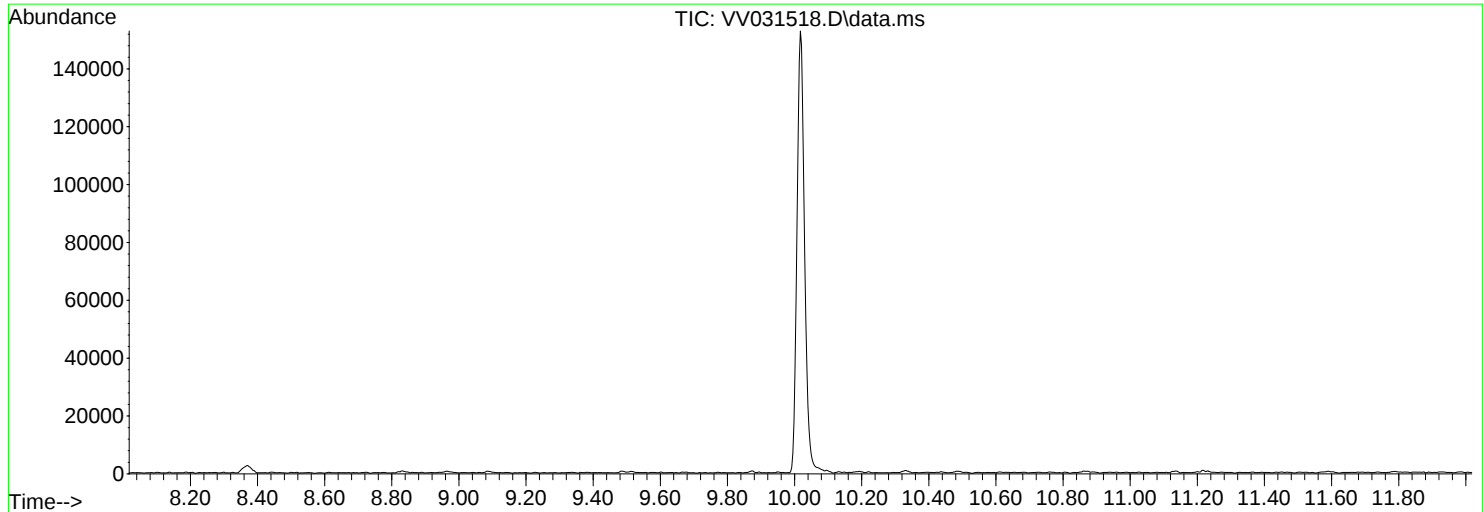

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	5414	PASS
75	95	30	80	51.1	15352	PASS
95	95	100	100	100.0	30040	PASS
96	95	5	9	7.4	2236	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.6	24227	PASS
175	174	5	9	7.2	1737	PASS
176	174	95	105	97.4	23589	PASS
177	176	5	10	6.7	1576	PASS

m/z	Abundance
39.80	107.0
43.80	336.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
35.70	373.0
36.90	1182.0
37.80	1001.0
38.90	607.0
39.80	188.0
43.70	347.0
44.90	273.0
46.80	425.0
47.70	183.0
48.80	1044.0
49.90	5402.0
50.80	1634.0
55.80	500.0
56.80	738.0
59.80	264.0
60.80	1473.0
61.90	1558.0
62.90	1208.0
63.90	266.0
64.70	348.0
67.80	3105.0
68.90	3066.0
69.70	177.0
72.00	138.0
72.80	1388.0
73.80	5228.0
74.90	14636.0
75.80	1277.0
76.70	244.0
77.90	145.0
78.70	1138.0
79.80	325.0
80.80	1351.0
81.80	301.0
86.70	1038.0
87.70	997.0
88.60	108.0
90.80	142.0
91.80	1043.0
92.90	1348.0
93.80	3546.0
94.80	29040.0
95.90	2093.0
105.70	203.0
115.70	143.0
116.90	302.0
117.70	153.0
118.80	268.0
127.70	163.0
140.70	353.0
142.70	538.0
144.70	302.0
170.80	104.0
171.70	425.0
173.80	23272.0
174.80	1716.0
175.80	22256.0
176.80	1580.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
35.70	346.0
36.80	1168.0
37.80	1074.0
38.80	599.0
39.80	189.0
43.80	436.0
44.90	247.0
46.80	493.0
47.80	214.0
48.80	1193.0
49.90	5650.0
50.80	1711.0
54.50	102.0
55.90	515.0
56.80	714.0
59.70	334.0
60.80	1553.0
61.90	1702.0
62.80	1348.0
63.80	277.0
64.80	346.0
67.80	3190.0
68.80	3265.0
69.70	186.0
71.90	194.0
72.80	1527.0
73.80	5255.0
74.90	15901.0
75.80	1315.0
76.70	221.0
77.90	137.0
78.70	1323.0
79.80	323.0
80.80	1417.0
81.70	357.0
86.80	1172.0
87.70	1086.0
88.60	129.0
90.80	177.0
91.80	1175.0
92.90	1444.0
93.80	3739.0
94.80	31144.0
95.90	2340.0
103.60	107.0
105.70	237.0
115.70	157.0
116.90	327.0
117.80	155.0
118.80	286.0
127.60	216.0
140.70	356.0
142.70	565.0
144.70	243.0
156.60	110.0
170.80	105.0
171.70	386.0
173.80	24832.0
174.80	1762.0
175.80	24376.0
176.80	1627.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
35.70	251.0
36.90	1081.0
37.80	1103.0
38.80	501.0
39.80	201.0
43.80	590.0
44.80	223.0
46.80	484.0
47.80	213.0
48.80	1218.0
49.90	5191.0
50.90	1612.0
55.90	458.0
56.80	670.0
59.70	370.0
60.80	1439.0
61.90	1549.0
62.90	1327.0
63.80	283.0
64.80	299.0
67.80	3027.0
68.80	3086.0
69.80	215.0
71.90	239.0
72.80	1458.0
73.90	4987.0
74.90	15518.0
75.80	1165.0
76.70	173.0
77.90	126.0
78.70	1348.0
79.70	388.0
80.70	1220.0
81.70	325.0
86.80	1207.0
87.70	1044.0
90.80	174.0
91.80	1143.0
92.80	1390.0
93.80	3545.0
94.80	29936.0
95.90	2276.0
103.70	122.0
105.70	209.0
115.70	157.0
116.80	298.0
117.70	134.0
118.80	301.0
127.60	211.0
140.70	312.0
142.70	586.0
144.60	208.0
156.70	106.0
171.80	382.0
173.80	24576.0
174.80	1734.0
175.80	24136.0
176.70	1521.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388