
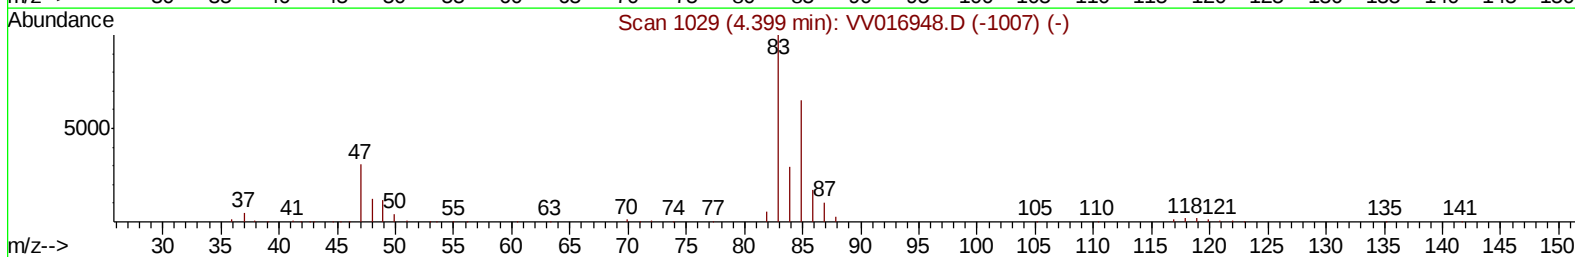
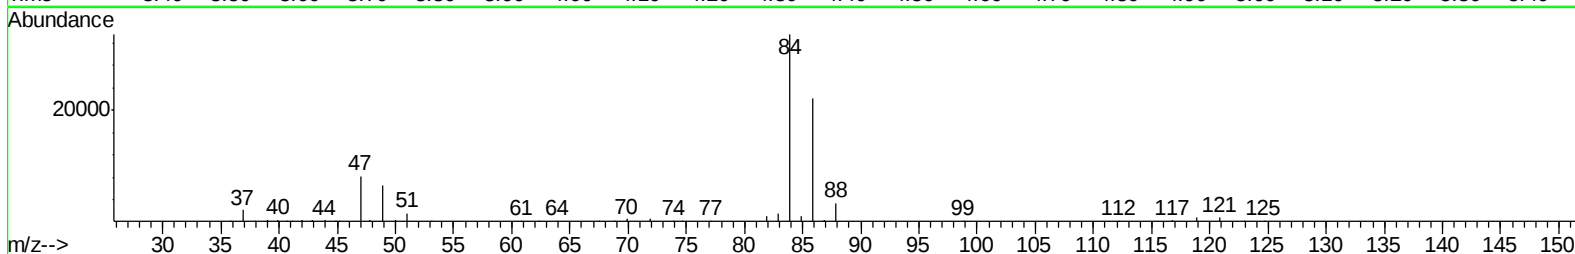


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061620\
Data File : VV016949.D
Acq On : 16 Jun 2020 10:12
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 17 00:57:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 17 00:55:26 2020
Response via : Initial Calibration

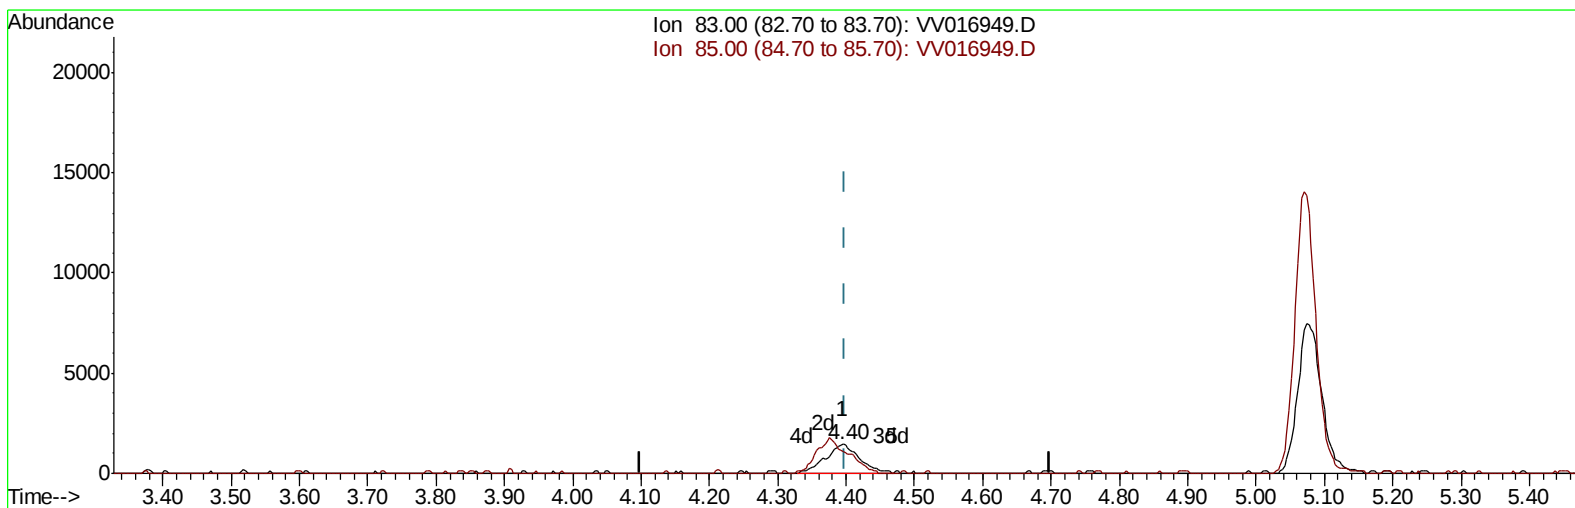

TIC: VV016949.D

(25) Chloroform (T)

4.396min (-0.003) 1.11ug/L m

response 4978

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	76.31
0.00	0.00	0.00
0.00	0.00	0.00