
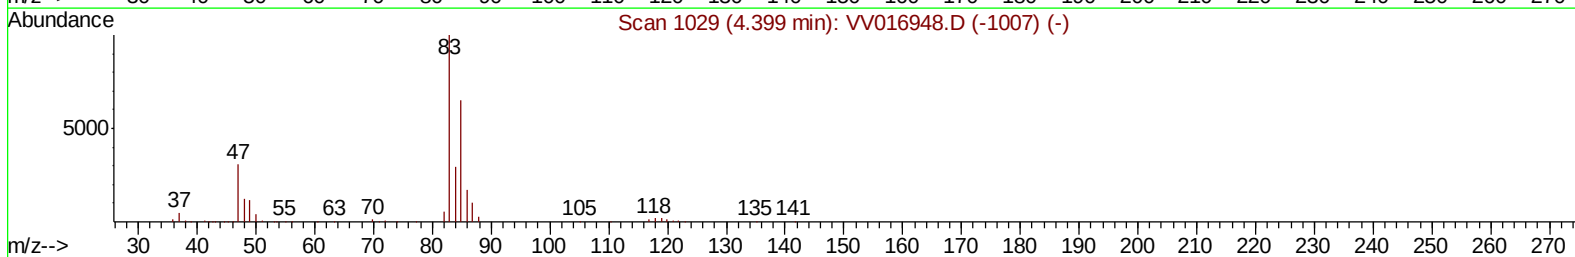
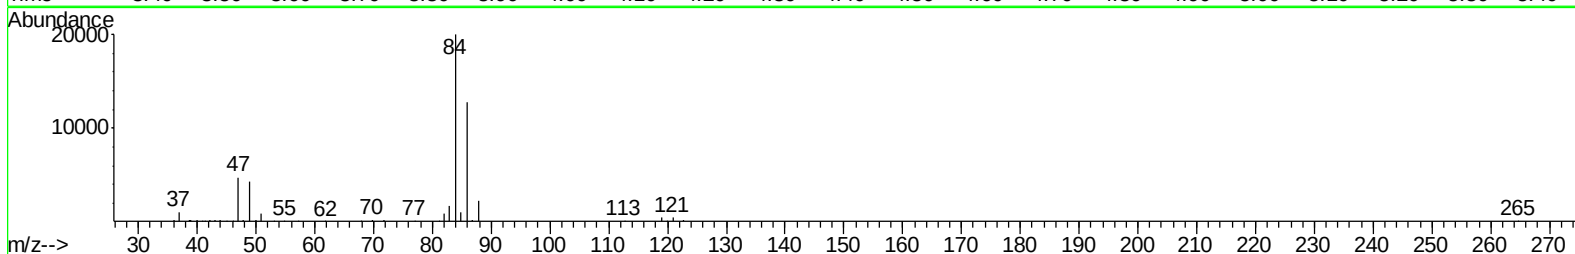


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061620\
 Data File : VV016951.D
 Acq On : 16 Jun 2020 11:02
 Operator : SY/MD
 Sample : L2913-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 17 00:57:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 17 00:55:26 2020
 Response via : Initial Calibration

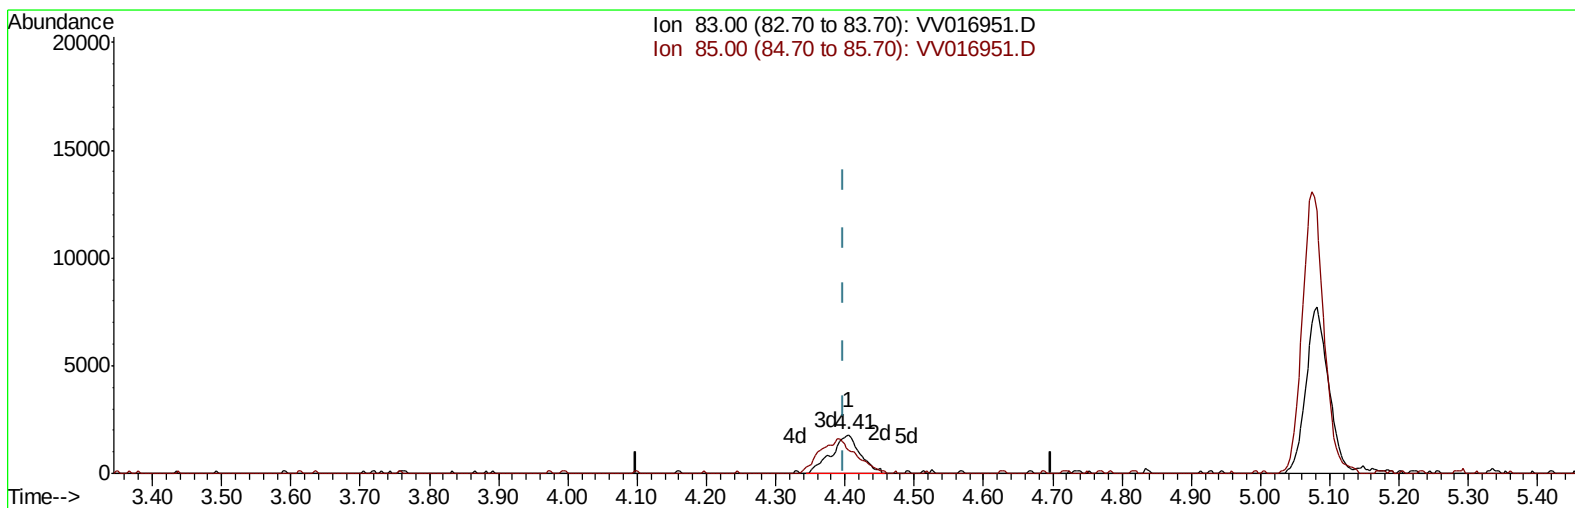

TIC: VV016951.D

(25) Chloroform (T)

4.405min (+0.007) 1.14ug/L m

response 5167

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	60.73
0.00	0.00	0.00
0.00	0.00	0.00