

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
 Data File : VV016949.D
 Acq On : 16 Jun 2020 10:12
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	166832	166081	11.79%	1.535%
2	1.576	144	151	160	rVB	131003	141998	10.08%	1.313%
3	2.119	311	320	341	rVB	280794	424281	30.12%	3.922%
4	2.556	453	456	462	rVB7	2021	1831	0.13%	0.017%
5	2.720	503	507	512	rVB8	1689	1232	0.09%	0.011%
6	2.762	517	520	521	rBV2	1732	937	0.07%	0.009%
7	2.833	538	542	545	rBV5	1164	1067	0.08%	0.010%
8	2.888	556	559	561	rBV4	2147	1205	0.09%	0.011%
9	2.942	570	576	579	rBV7	1579	1898	0.13%	0.018%
10	3.113	626	629	632	rVB3	1329	894	0.06%	0.008%
11	3.151	639	641	645	rBV4	1470	1294	0.09%	0.012%
12	3.203	653	657	658	rBV4	1270	937	0.07%	0.009%
13	3.212	658	660	664	rVV3	1492	1086	0.08%	0.010%
14	3.251	670	672	675	rBV4	1382	855	0.06%	0.008%
15	3.309	687	690	694	rBV5	1236	874	0.06%	0.008%
16	3.421	721	725	728	rBV5	1516	1375	0.10%	0.013%
17	3.460	732	737	739	rVB4	1514	1341	0.10%	0.012%
18	3.479	739	743	745	rBV5	1740	1223	0.09%	0.011%
19	3.531	757	759	763	rBV4	1126	749	0.05%	0.007%
20	3.743	820	825	829	rBV4	1249	1058	0.08%	0.010%
21	3.778	833	836	842	rBV6	1436	1194	0.08%	0.011%
22	3.894	857	872	904	rBV	113367	319679	22.70%	2.955%
23	4.373	1006	1021	1047	rBV2	233137	564829	40.10%	5.221%
24	4.601	1090	1092	1095	rVB4	1790	922	0.07%	0.009%
25	4.778	1144	1147	1150	rVB5	1495	755	0.05%	0.007%
26	4.833	1160	1164	1166	rBV5	1271	1011	0.07%	0.009%
27	4.894	1180	1183	1185	rBV3	1901	1387	0.10%	0.013%
28	4.962	1202	1204	1207	rBV3	1582	823	0.06%	0.008%
29	5.068	1220	1237	1265	rBV2	549507	1408425	100.00%	13.018%
30	5.354	1321	1326	1330	rBV7	2054	2285	0.16%	0.021%
31	5.476	1360	1364	1367	rBV5	1776	1518	0.11%	0.014%
32	5.637	1400	1414	1438	rBV	414654	832361	59.10%	7.694%
33	5.926	1495	1504	1520	rVB2	30398	64118	4.55%	0.593%
34	6.090	1542	1555	1576	rBV	317152	640732	45.49%	5.922%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
 Data File : VV016949.D
 Acq On : 16 Jun 2020 10:12
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.489	1674	1679	1685	rBV9	2749	2973	0.21%	0.027%
36	6.524	1687	1690	1693	rBV6	1401	1070	0.08%	0.010%
37	6.614	1716	1718	1723	rBV6	1025	936	0.07%	0.009%
38	6.720	1747	1751	1754	rBV3	1482	1314	0.09%	0.012%
39	6.752	1758	1761	1764	rVB4	977	789	0.06%	0.007%
40	7.006	1826	1840	1862	rBV	177393	331932	23.57%	3.068%
41	7.289	1926	1928	1930	rBV3	1534	834	0.06%	0.008%
42	7.334	1931	1942	1958	rVV	674288	1148177	81.52%	10.613%
43	7.588	2017	2021	2026	rBV7	2226	1982	0.14%	0.018%
44	7.640	2026	2037	2055	rBV	133689	229529	16.30%	2.122%
45	7.910	2118	2121	2125	rBV5	1325	1135	0.08%	0.010%
46	8.029	2155	2158	2160	rBV3	1164	817	0.06%	0.008%
47	8.106	2171	2182	2213	rBV2	316659	625375	44.40%	5.780%
48	8.604	2333	2337	2340	rBV6	1252	1229	0.09%	0.011%
49	8.685	2360	2362	2366	rVV4	1410	904	0.06%	0.008%
50	8.871	2409	2420	2436	rBV	625669	1013674	71.97%	9.370%
51	9.103	2490	2492	2495	rBV3	1442	789	0.06%	0.007%
52	9.354	2567	2570	2572	rBV4	1152	952	0.07%	0.009%
53	9.453	2598	2601	2605	rBV5	1548	1081	0.08%	0.010%
54	9.495	2609	2614	2617	rBV7	1688	1499	0.11%	0.014%
55	9.559	2631	2634	2637	rBV4	1830	1501	0.11%	0.014%
56	9.637	2654	2658	2660	rBV4	1433	1037	0.07%	0.010%
57	9.749	2690	2693	2695	rBV4	2093	1007	0.07%	0.009%
58	9.836	2716	2720	2723	rBV3	1443	1315	0.09%	0.012%
59	9.903	2738	2741	2744	rVV5	1473	853	0.06%	0.008%
60	9.926	2746	2748	2751	rVV3	1601	1130	0.08%	0.010%
61	9.955	2753	2757	2761	rBV5	2894	2755	0.20%	0.025%
62	9.990	2765	2768	2770	rVB4	1452	758	0.05%	0.007%
63	10.006	2770	2773	2776	rBV4	1769	1018	0.07%	0.009%
64	10.238	2833	2845	2858	rBV	381305	603962	42.88%	5.583%
65	10.646	2969	2972	2974	rBV3	1428	875	0.06%	0.008%
66	10.746	3000	3003	3005	rBV2	1473	1001	0.07%	0.009%
67	10.778	3009	3013	3016	rVV4	920	765	0.05%	0.007%
68	11.157	3126	3131	3133	rBV4	1186	970	0.07%	0.009%
69	11.183	3135	3139	3140	rBV4	1688	1101	0.08%	0.010%
70	11.270	3155	3166	3183	rBV	674612	1017632	72.25%	9.406%
71	11.431	3212	3216	3222	rBV8	1319	1541	0.11%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
 Data File : VV016949.D
 Acq On : 16 Jun 2020 10:12
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3299	rBV	744452	1143828	81.21%	10.573%
73	11.788	3324	3327	3331	rVB6	1283	879	0.06%	0.008%
74	11.810	3331	3334	3338	rVB6	1240	1076	0.08%	0.010%
75	11.884	3353	3357	3360	rVV3	1014	915	0.06%	0.008%
76	11.907	3360	3364	3371	rVB9	2065	2622	0.19%	0.024%
77	11.939	3371	3374	3377	rBV5	2056	1743	0.12%	0.016%
78	12.042	3402	3406	3407	rBV4	1245	925	0.07%	0.009%
79	12.196	3451	3454	3456	rVB3	1383	832	0.06%	0.008%
80	12.318	3490	3492	3494	rBV3	1468	933	0.07%	0.009%
81	12.389	3511	3514	3516	rBV4	1594	863	0.06%	0.008%
82	12.627	3585	3588	3589	rBV3	1471	735	0.05%	0.007%
83	12.675	3589	3603	3609	rBV3	5465	10148	0.72%	0.094%
84	12.775	3631	3634	3637	rBV4	1371	1175	0.08%	0.011%
85	13.064	3721	3724	3726	rBV3	1417	998	0.07%	0.009%
86	13.189	3761	3763	3769	rBV5	1112	1270	0.09%	0.012%
87	13.286	3786	3793	3803	rVB9	7251	10534	0.75%	0.097%
88	13.530	3862	3869	3881	rBV3	8201	14802	1.05%	0.137%
89	13.710	3922	3925	3926	rBV2	1326	795	0.06%	0.007%
90	13.768	3939	3943	3952	rVB10	6922	10780	0.77%	0.100%
91	13.868	3969	3974	3976	rBV5	1590	1260	0.09%	0.012%
92	13.945	3995	3998	4000	rBV4	1831	1123	0.08%	0.010%
93	14.215	4076	4082	4085	rBV6	1108	1162	0.08%	0.011%
94	14.267	4094	4098	4101	rBV5	1067	1085	0.08%	0.010%
95	14.575	4191	4194	4198	rBV6	1430	1433	0.10%	0.013%
96	14.810	4264	4267	4269	rBV4	1391	797	0.06%	0.007%
97	14.881	4286	4289	4294	rVB6	1986	1481	0.11%	0.014%
98	15.328	4426	4428	4431	rBV4	1715	875	0.06%	0.008%
99	15.543	4492	4495	4497	rBV4	2164	1234	0.09%	0.011%
100	16.141	4678	4681	4686	rBV	6116	3953	0.28%	0.037%


Sum of corrected areas: 10818723

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
Data File : VV016949.D
Acq On : 16 Jun 2020 10:12
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

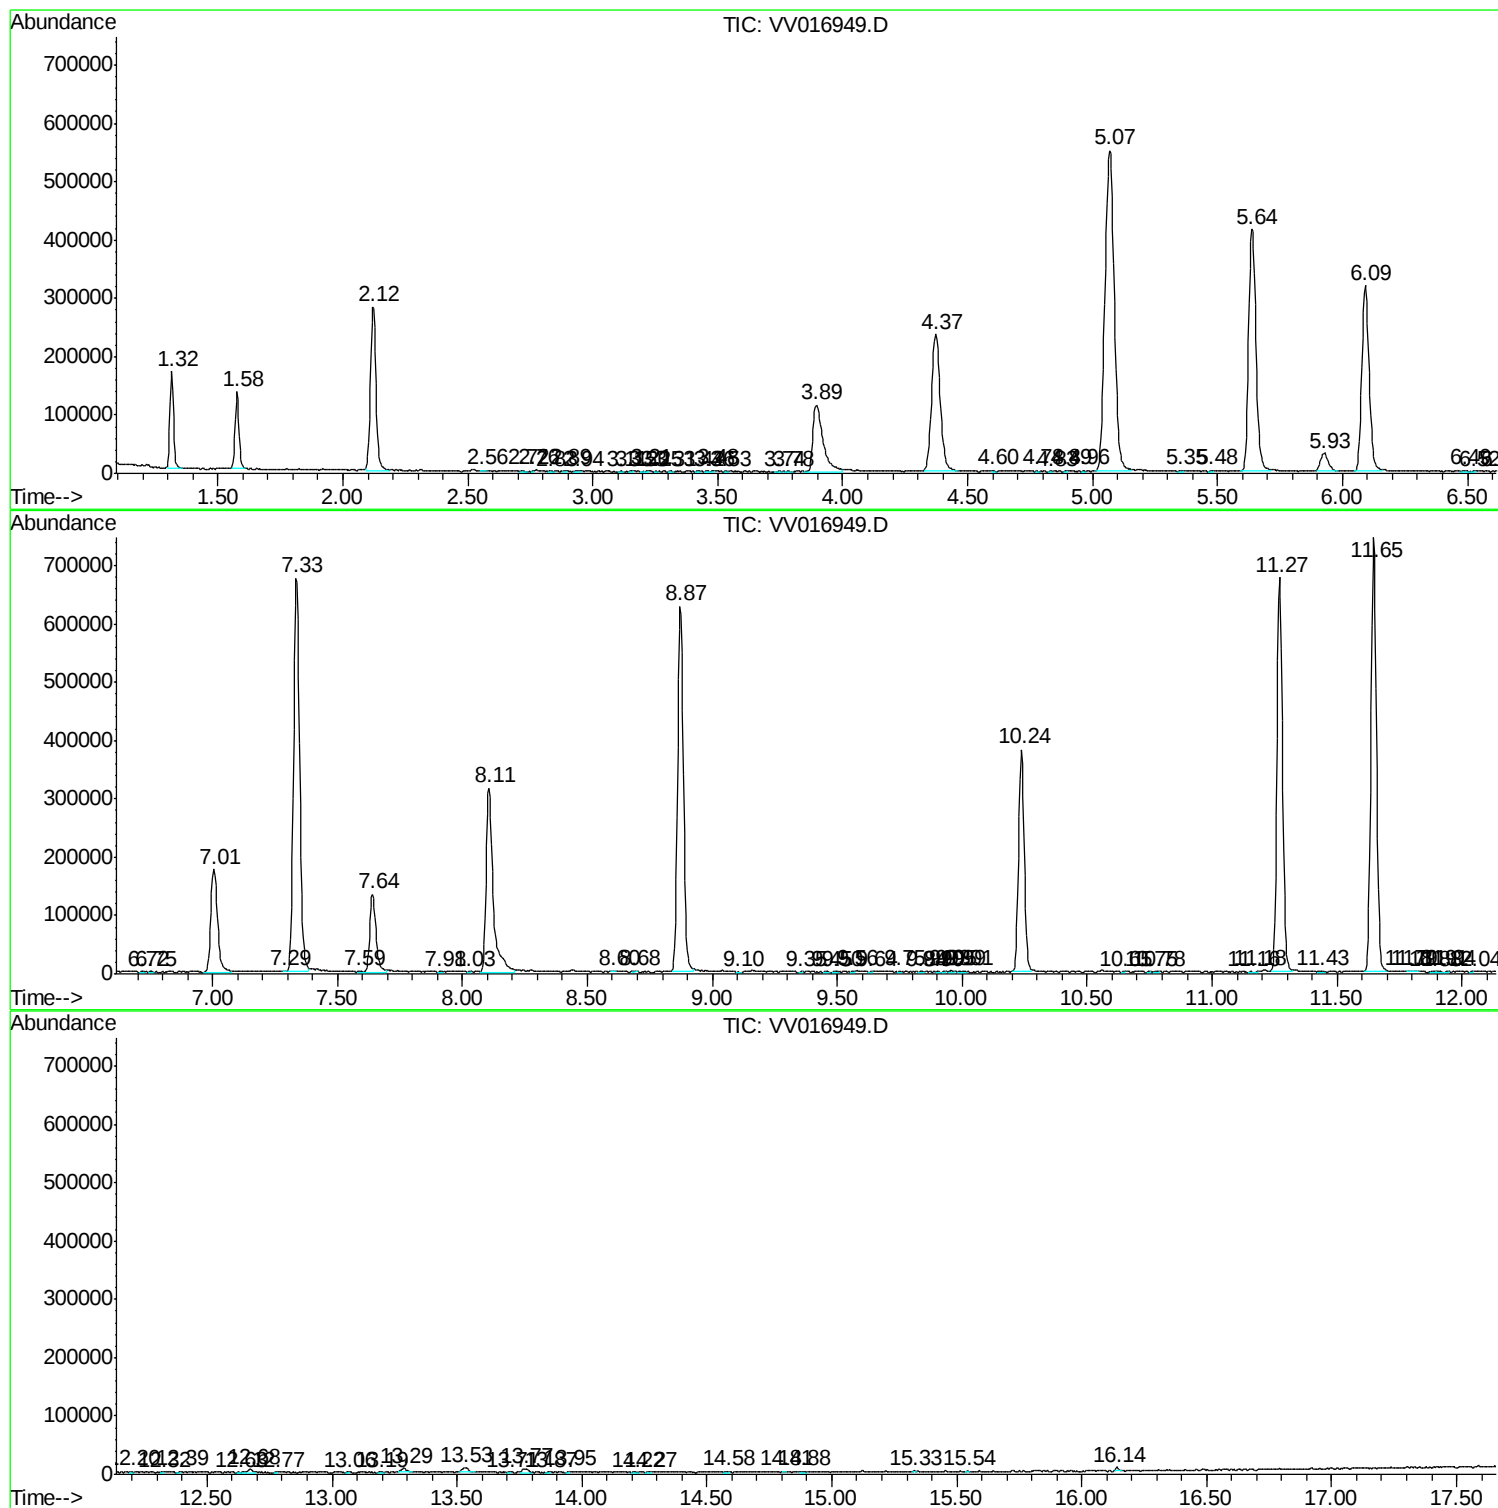

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
Data File : VV016949.D
Acq On : 16 Jun 2020 10:12
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK88

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061620\
Data File : VV016949.D
Acq On : 16 Jun 2020 10:12
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK88

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc