

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
 Data File : VV016951.D
 Acq On : 16 Jun 2020 11:02
 Operator : SY/MD
 Sample : L2913-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	86	rVB	158271	166465	12.08%	1.580%
2	1.576	144	151	162	rVB	123624	138627	10.06%	1.316%
3	2.123	312	321	341	rVB	266756	407793	29.60%	3.872%
4	2.968	583	584	585	rVB	1014	196	0.01%	0.002%
5	3.084	614	620	622	rBV6	1451	1385	0.10%	0.013%
6	3.274	677	679	684	rVB6	1033	647	0.05%	0.006%
7	3.299	684	687	688	rBV3	753	414	0.03%	0.004%
8	3.351	701	703	706	rBV5	1625	1089	0.08%	0.010%
9	3.666	799	801	803	rBV3	1003	501	0.04%	0.005%
10	3.682	803	806	811	rBV5	1567	1716	0.12%	0.016%
11	3.704	811	813	816	rVV4	1235	773	0.06%	0.007%
12	3.901	864	874	899	rBV	105436	279681	20.30%	2.655%
13	4.376	1007	1022	1043	rBV	224991	546710	39.68%	5.190%
14	4.595	1086	1090	1092	rBV4	2138	1701	0.12%	0.016%
15	5.071	1221	1238	1265	rBV2	536446	1377828	100.00%	13.081%
16	5.556	1388	1389	1392	rBV2	1199	741	0.05%	0.007%
17	5.640	1403	1415	1445	rBV	416806	828694	60.14%	7.867%
18	5.811	1466	1468	1472	rVB5	2461	1548	0.11%	0.015%
19	5.926	1497	1504	1521	rVB	33308	66119	4.80%	0.628%
20	6.032	1534	1537	1540	rBV4	2029	1275	0.09%	0.012%
21	6.093	1543	1556	1573	rBV2	308086	624582	45.33%	5.930%
22	6.380	1643	1645	1648	rBV4	1109	604	0.04%	0.006%
23	6.418	1655	1657	1659	rBV3	887	344	0.02%	0.003%
24	6.733	1753	1755	1758	rVB3	1164	637	0.05%	0.006%
25	6.749	1758	1760	1763	rVB4	1597	715	0.05%	0.007%
26	6.762	1763	1764	1766	rBV2	879	405	0.03%	0.004%
27	6.804	1775	1777	1780	rBV3	1558	526	0.04%	0.005%
28	7.007	1829	1840	1859	rBV	183684	328120	23.81%	3.115%
29	7.286	1925	1927	1930	rVB3	1344	837	0.06%	0.008%
30	7.338	1931	1943	1960	rBV	662757	1125139	81.66%	10.682%
31	7.643	2028	2038	2054	rBV	132988	224960	16.33%	2.136%
32	8.032	2157	2159	2161	rBV3	1195	455	0.03%	0.004%
33	8.106	2170	2182	2218	rBV2	304675	608012	44.13%	5.772%
34	8.479	2296	2298	2299	rBV2	1930	718	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
 Data File : VV016951.D
 Acq On : 16 Jun 2020 11:02
 Operator : SY/MD
 Sample : L2913-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.601	2334	2336	2337	rBV	1089	475	0.03%	0.005%
36	8.740	2377	2379	2383	rVB5	1659	1025	0.07%	0.010%
37	8.871	2408	2420	2447	rBV	621075	1022722	74.23%	9.710%
38	9.122	2496	2498	2503	rVB6	1984	1308	0.09%	0.012%
39	9.283	2545	2548	2552	rBV5	2129	1497	0.11%	0.014%
40	9.354	2568	2570	2573	rBV4	1263	833	0.06%	0.008%
41	9.434	2592	2595	2600	rVB7	1644	934	0.07%	0.009%
42	9.498	2612	2615	2617	rBV4	1104	709	0.05%	0.007%
43	9.560	2630	2634	2635	rBV3	1700	1063	0.08%	0.010%
44	9.598	2645	2646	2651	rVB5	2047	1474	0.11%	0.014%
45	9.682	2670	2672	2673	rBV2	960	441	0.03%	0.004%
46	9.810	2709	2712	2714	rBV3	1010	596	0.04%	0.006%
47	10.010	2770	2774	2775	rBV4	1672	898	0.07%	0.009%
48	10.032	2779	2781	2784	rBV4	1096	732	0.05%	0.007%
49	10.238	2833	2845	2861	rBV	377054	588782	42.73%	5.590%
50	10.434	2904	2906	2908	rBV3	1049	551	0.04%	0.005%
51	10.643	2968	2971	2973	rBV2	1475	858	0.06%	0.008%
52	10.736	2997	3000	3001	rBV3	1526	726	0.05%	0.007%
53	10.785	3012	3015	3017	rBV3	1404	792	0.06%	0.008%
54	10.820	3023	3026	3028	rBV4	964	690	0.05%	0.007%
55	10.907	3051	3053	3055	rBV3	1211	534	0.04%	0.005%
56	11.058	3098	3100	3103	rVB4	1325	816	0.06%	0.008%
57	11.080	3105	3107	3108	rBV2	1323	563	0.04%	0.005%
58	11.138	3123	3125	3126	rBV2	1167	462	0.03%	0.004%
59	11.270	3154	3166	3184	rBV	668296	1030574	74.80%	9.784%
60	11.498	3236	3237	3239	rBV2	1195	661	0.05%	0.006%
61	11.646	3269	3283	3299	rBV	712500	1115147	80.94%	10.587%
62	11.842	3341	3344	3345	rBV3	1142	593	0.04%	0.006%
63	11.855	3345	3348	3350	rVV3	1588	857	0.06%	0.008%
64	11.900	3360	3362	3363	rBV2	1079	338	0.02%	0.003%
65	11.955	3376	3379	3383	rBV5	1344	1028	0.07%	0.010%
66	12.360	3504	3505	3506	rBV	1115	353	0.03%	0.003%
67	12.521	3551	3555	3557	rBV4	2032	1484	0.11%	0.014%
68	12.556	3563	3566	3570	rVV4	1315	1094	0.08%	0.010%
69	12.576	3570	3572	3577	rVB5	1036	713	0.05%	0.007%
70	12.656	3595	3597	3598	rBV2	2111	853	0.06%	0.008%
71	12.733	3619	3621	3623	rBV3	1565	836	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
Data File : VV016951.D
Acq On : 16 Jun 2020 11:02
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Title : VOC Analysis

72	12.849	3652	3657	3660	rBV8	1893	2082	0.15%	0.020%
73	13.035	3713	3715	3716	rBV2	1091	376	0.03%	0.004%
74	13.437	3836	3840	3844	rBV6	1756	1808	0.13%	0.017%
75	13.884	3976	3979	3982	rBV4	1434	1074	0.08%	0.010%
76	14.090	4039	4043	4045	rBV5	1674	1241	0.09%	0.012%
77	14.280	4097	4102	4107	rBV8	1366	1625	0.12%	0.015%
78	15.270	4408	4410	4415	rBV6	1845	1029	0.07%	0.010%


Sum of corrected areas: 10533204

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
Data File : VV016951.D
Acq On : 16 Jun 2020 11:02
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

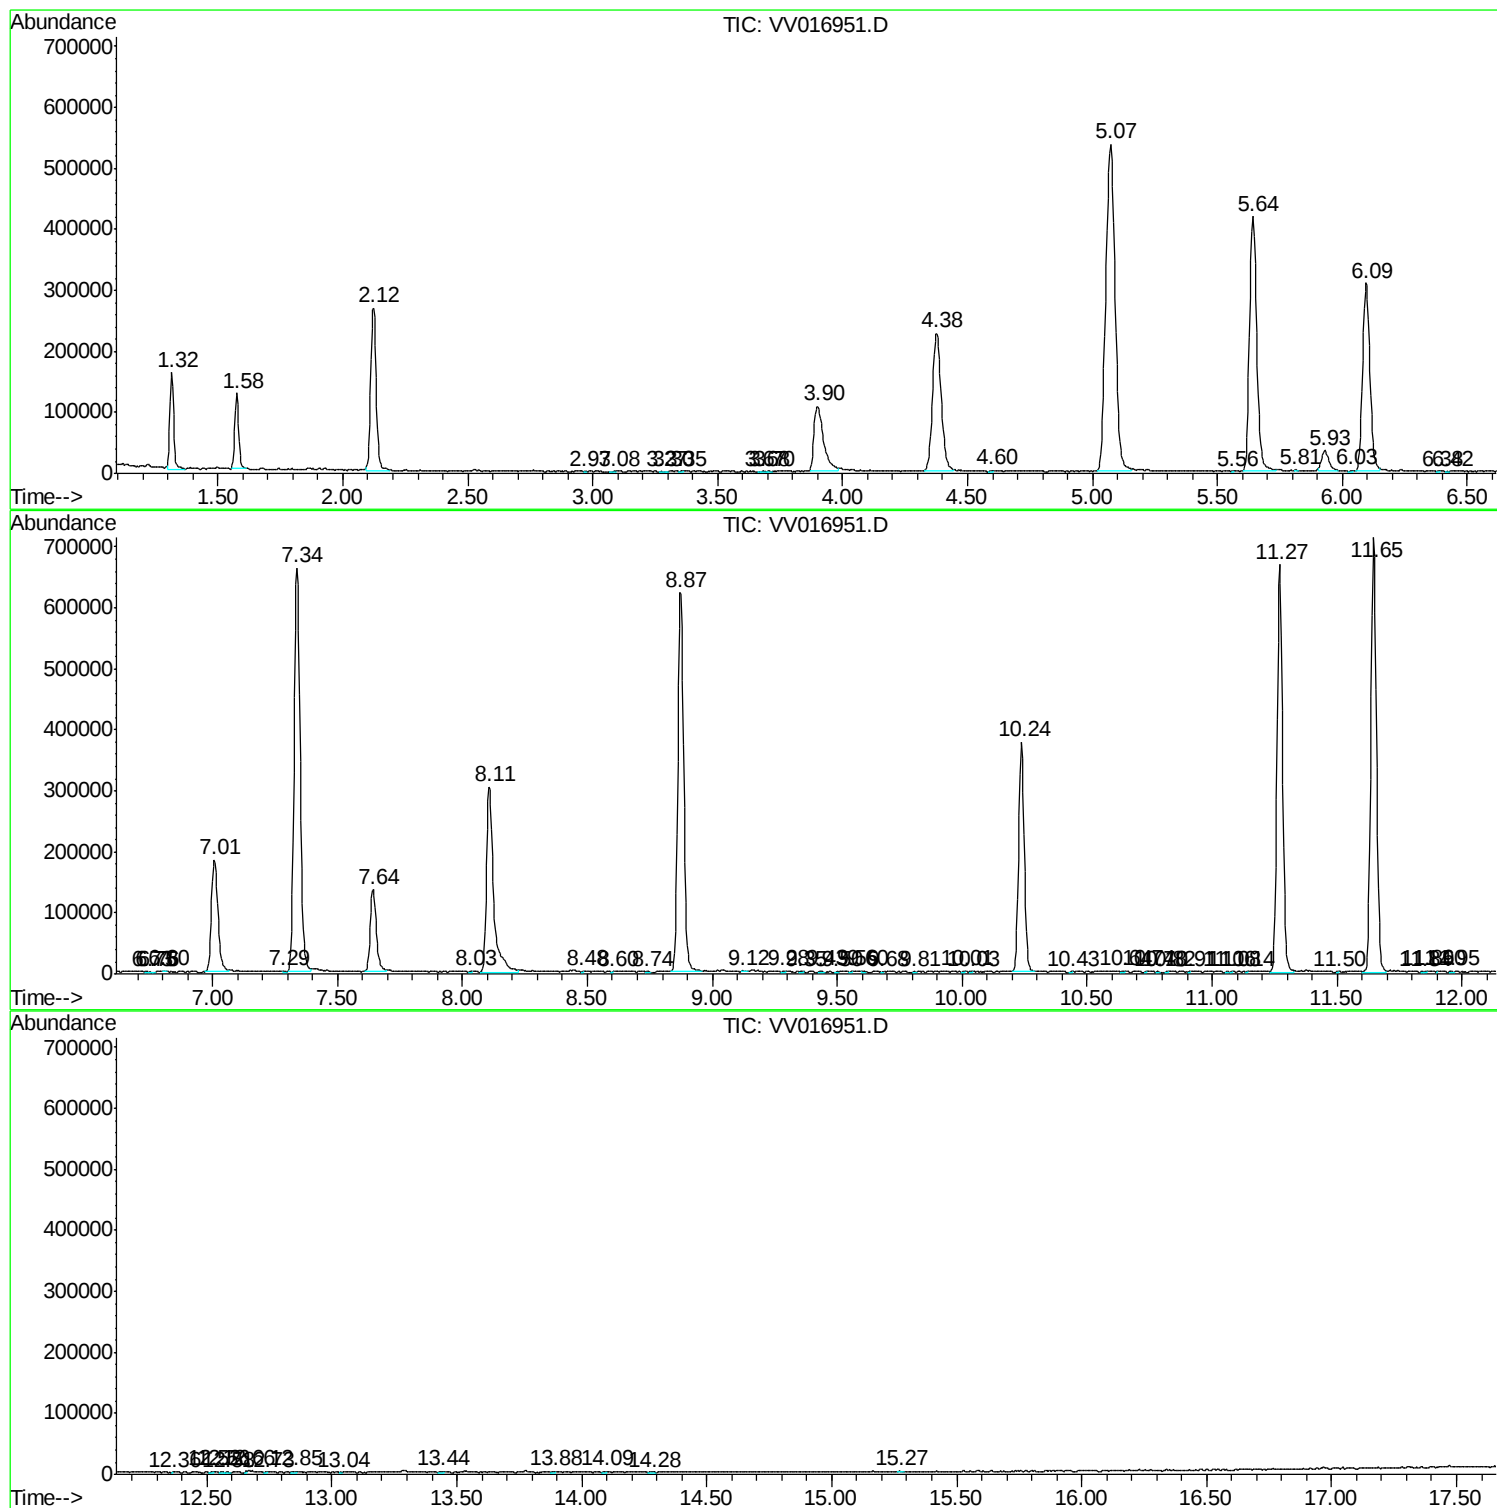

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
Data File : VV016951.D
Acq On : 16 Jun 2020 11:02
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
Data File : VV016951.D
Acq On : 16 Jun 2020 11:02
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc