


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061620\
 Data File : VV016947.D
 Acq On : 16 Jun 2020 09:05
 Operator : SY/MD
 Sample : BFB90
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB90

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 17 02:00:28 2020

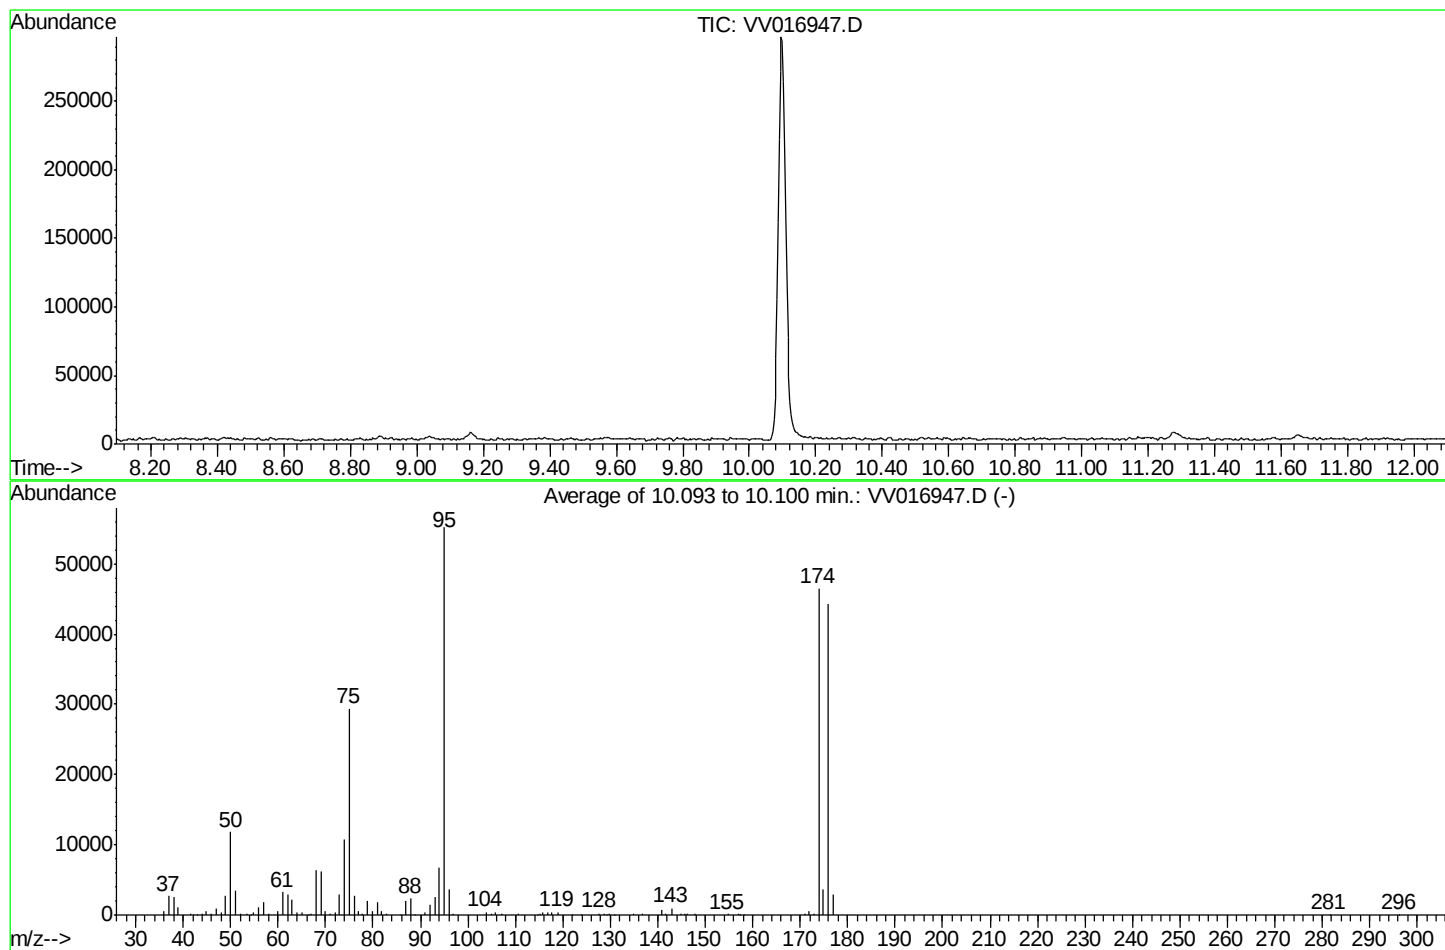

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	11790	PASS
75	95	30	80	53.3	29424	PASS
95	95	100	100	100.0	55194	PASS
96	95	5	9	6.5	3577	PASS
173	174	0.00	2	0.5	252	PASS
174	95	50	120	84.1	46394	PASS
175	174	5	9	7.8	3614	PASS
176	174	95	101	95.4	44258	PASS
177	176	5	9	6.5	2864	PASS

m/z	Abundance
35.50	160.0
36.20	117.0
36.80	145.0
38.10	118.0
38.90	195.0
39.90	382.0
41.00	114.0
42.00	119.0
42.80	125.0
44.00	392.0
50.30	105.0
51.00	102.0
52.20	105.0
66.50	104.0
69.60	137.0
77.40	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
35.90	512.0
37.00	2837.0
38.00	2600.0
39.00	1135.0
40.00	293.0
41.40	121.0
42.20	128.0
43.00	237.0
44.00	671.0
45.00	599.0
45.80	139.0
47.00	754.0
47.90	414.0
48.90	2828.0
50.00	11416.0
51.00	3432.0
52.10	306.0
53.40	147.0
54.30	111.0
54.90	329.0
56.00	963.0
57.00	1644.0
58.00	265.0
59.90	501.0
60.90	3111.0
62.00	2931.0
63.00	2119.0
64.00	232.0
64.90	395.0
66.30	143.0
67.00	183.0
68.00	5788.0
69.00	6105.0
70.00	542.0
70.90	139.0
72.00	391.0
73.00	2626.0
74.00	10494.0
75.00	27784.0
76.00	2703.0
76.90	412.0
77.90	216.0
78.90	1766.0
79.90	603.0
80.90	1802.0
81.90	474.0
82.80	140.0
87.00	1928.0
87.90	2189.0
88.80	126.0
91.00	295.0
91.90	1396.0
93.00	2477.0
94.00	6562.0
95.00	52496.0
96.00	3388.0
96.90	204.0
103.80	416.0
104.90	128.0
105.90	323.0
107.00	136.0
110.60	108.0
114.70	135.0
115.80	297.0
116.90	366.0
117.70	288.0
118.80	313.0
123.90	110.0
127.60	203.0
128.70	129.0
129.20	129.0
129.80	241.0
130.80	140.0
134.80	197.0
136.80	108.0
140.90	618.0
141.70	165.0
142.90	935.0
144.90	133.0
145.70	100.0
146.20	117.0
147.80	164.0
154.90	164.0
157.10	158.0
170.90	115.0
171.90	540.0
173.00	758.0
173.90	42800.0
174.90	3333.0
175.90	40792.0
176.90	2896.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

296.20

113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
35.90	619.0
37.00	2895.0
38.00	2667.0
39.00	1256.0
40.10	321.0
41.50	155.0
42.20	133.0
43.00	212.0
44.00	631.0
45.00	627.0
45.90	117.0
47.00	1003.0
48.00	426.0
49.00	2880.0
50.00	12327.0
51.00	3633.0
52.10	363.0
53.40	133.0
54.90	300.0
56.00	1065.0
57.00	1882.0
58.00	275.0
59.90	630.0
61.00	3393.0
62.00	3097.0
63.00	2202.0
64.00	293.0
64.90	376.0
66.30	151.0
67.00	184.0
68.00	6618.0
69.00	6480.0
70.00	550.0
70.90	152.0
72.00	360.0
73.00	3079.0
74.00	11215.0
75.00	30424.0
76.00	2899.0
76.90	511.0
77.90	253.0
78.90	2033.0
79.90	650.0
80.90	1973.0
81.90	525.0
82.80	143.0
86.90	2066.0
87.90	2378.0
88.80	147.0
91.00	352.0
92.00	1563.0
93.00	2625.0
94.00	6942.0
95.00	56888.0
96.00	3617.0
96.90	257.0
103.80	462.0
104.90	129.0
105.80	344.0
107.00	153.0
110.70	149.0
114.70	107.0
115.10	130.0
115.90	358.0
116.80	453.0
117.80	286.0
118.90	481.0
122.00	122.0
127.70	245.0
128.80	120.0
129.20	120.0
129.80	209.0
130.80	121.0
134.80	162.0
136.70	168.0
140.90	723.0
141.70	186.0
142.90	1012.0
144.90	148.0
145.70	111.0
146.20	123.0
147.80	171.0
154.90	154.0
157.10	143.0
170.90	133.0
171.80	522.0
173.90	47880.0
174.90	3780.0
175.90	45736.0
176.90	2955.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.00	729.0
37.00	2810.0
38.00	2545.0
39.00	1247.0
39.90	339.0
41.50	168.0
42.20	161.0
43.00	188.0
44.00	580.0
44.90	565.0
45.90	134.0
47.00	1021.0
48.10	458.0
49.00	2589.0
50.00	11627.0
51.00	3591.0
52.10	375.0
53.20	127.0
54.90	235.0
56.00	1012.0
57.00	1899.0
58.00	203.0
59.90	640.0
61.00	3118.0
62.00	2910.0
62.90	2069.0
63.90	338.0
65.00	373.0
66.30	129.0
66.90	171.0
68.00	6559.0
69.00	6223.0
70.00	548.0
71.00	141.0
71.90	310.0
73.00	3192.0
74.00	10642.0
75.00	30064.0
76.00	2694.0
76.90	503.0
77.80	293.0
78.90	2133.0
79.90	623.0
80.90	1977.0
81.90	511.0
82.90	103.0
85.70	103.0
86.90	2235.0
87.90	2306.0
90.90	343.0
92.00	1605.0
93.00	2531.0
94.00	6753.0
95.00	56200.0
96.00	3726.0
96.90	245.0
103.80	404.0
104.90	135.0
105.70	364.0
107.00	126.0
110.70	148.0
115.10	170.0
115.90	363.0
116.80	518.0
117.80	266.0
118.90	551.0
121.90	126.0
127.70	249.0
128.80	125.0
129.80	207.0
134.70	118.0
136.70	196.0
140.90	790.0
141.70	188.0
142.90	857.0
145.00	123.0
145.60	108.0
146.20	121.0
147.70	168.0
154.70	189.0
157.30	129.0
158.10	105.0
170.90	137.0
171.80	621.0
173.90	48504.0
174.90	3731.0
175.90	46248.0
176.90	2741.0
281.60	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90