

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021547.D
 Acq On : 16 Jun 2021 13:56
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 17 02:04:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 17 02:01:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	489101	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	455348	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	248007	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	150700	46.799	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	93.600%	
7) Chloroethane-d5	1.568	69	122299	51.055	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.120%	
11) 1,1-Dichloroethene-d2	2.105	63	201164	36.559	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	73.120%	
21) 2-Butanone-d5	3.896	46	246006	106.537	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	106.540%	
24) Chloroform-d	4.349	84	298867	46.623	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.240%	
26) 1,2-Dichloroethane-d4	5.034	65	181362	49.120	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.240%	
32) Benzene-d6	5.050	84	622357	48.857	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.720%	
36) 1,2-Dichloropropane-d6	6.072	67	194356	49.406	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	98.820%	
41) Toluene-d8	7.317	98	587708	48.426	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.860%	
43) trans-1,3-Dichloroprop...	7.622	79	96755	45.959	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.920%	
47) 2-Hexanone-d5	8.088	63	182431	100.994	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	100.990%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	273119	50.016	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.040%	
66) 1,2-Dichlorobenzene-d4	11.625	152	255535	49.566	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.140%	
Target Compounds						
44) trans-1,3-Dichloropropene	7.625	75	3741	0.708	ug/L	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021547.D
Acq On : 16 Jun 2021 13:56
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 17 02:04:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 17 02:01:55 2021
Response via : Initial Calibration

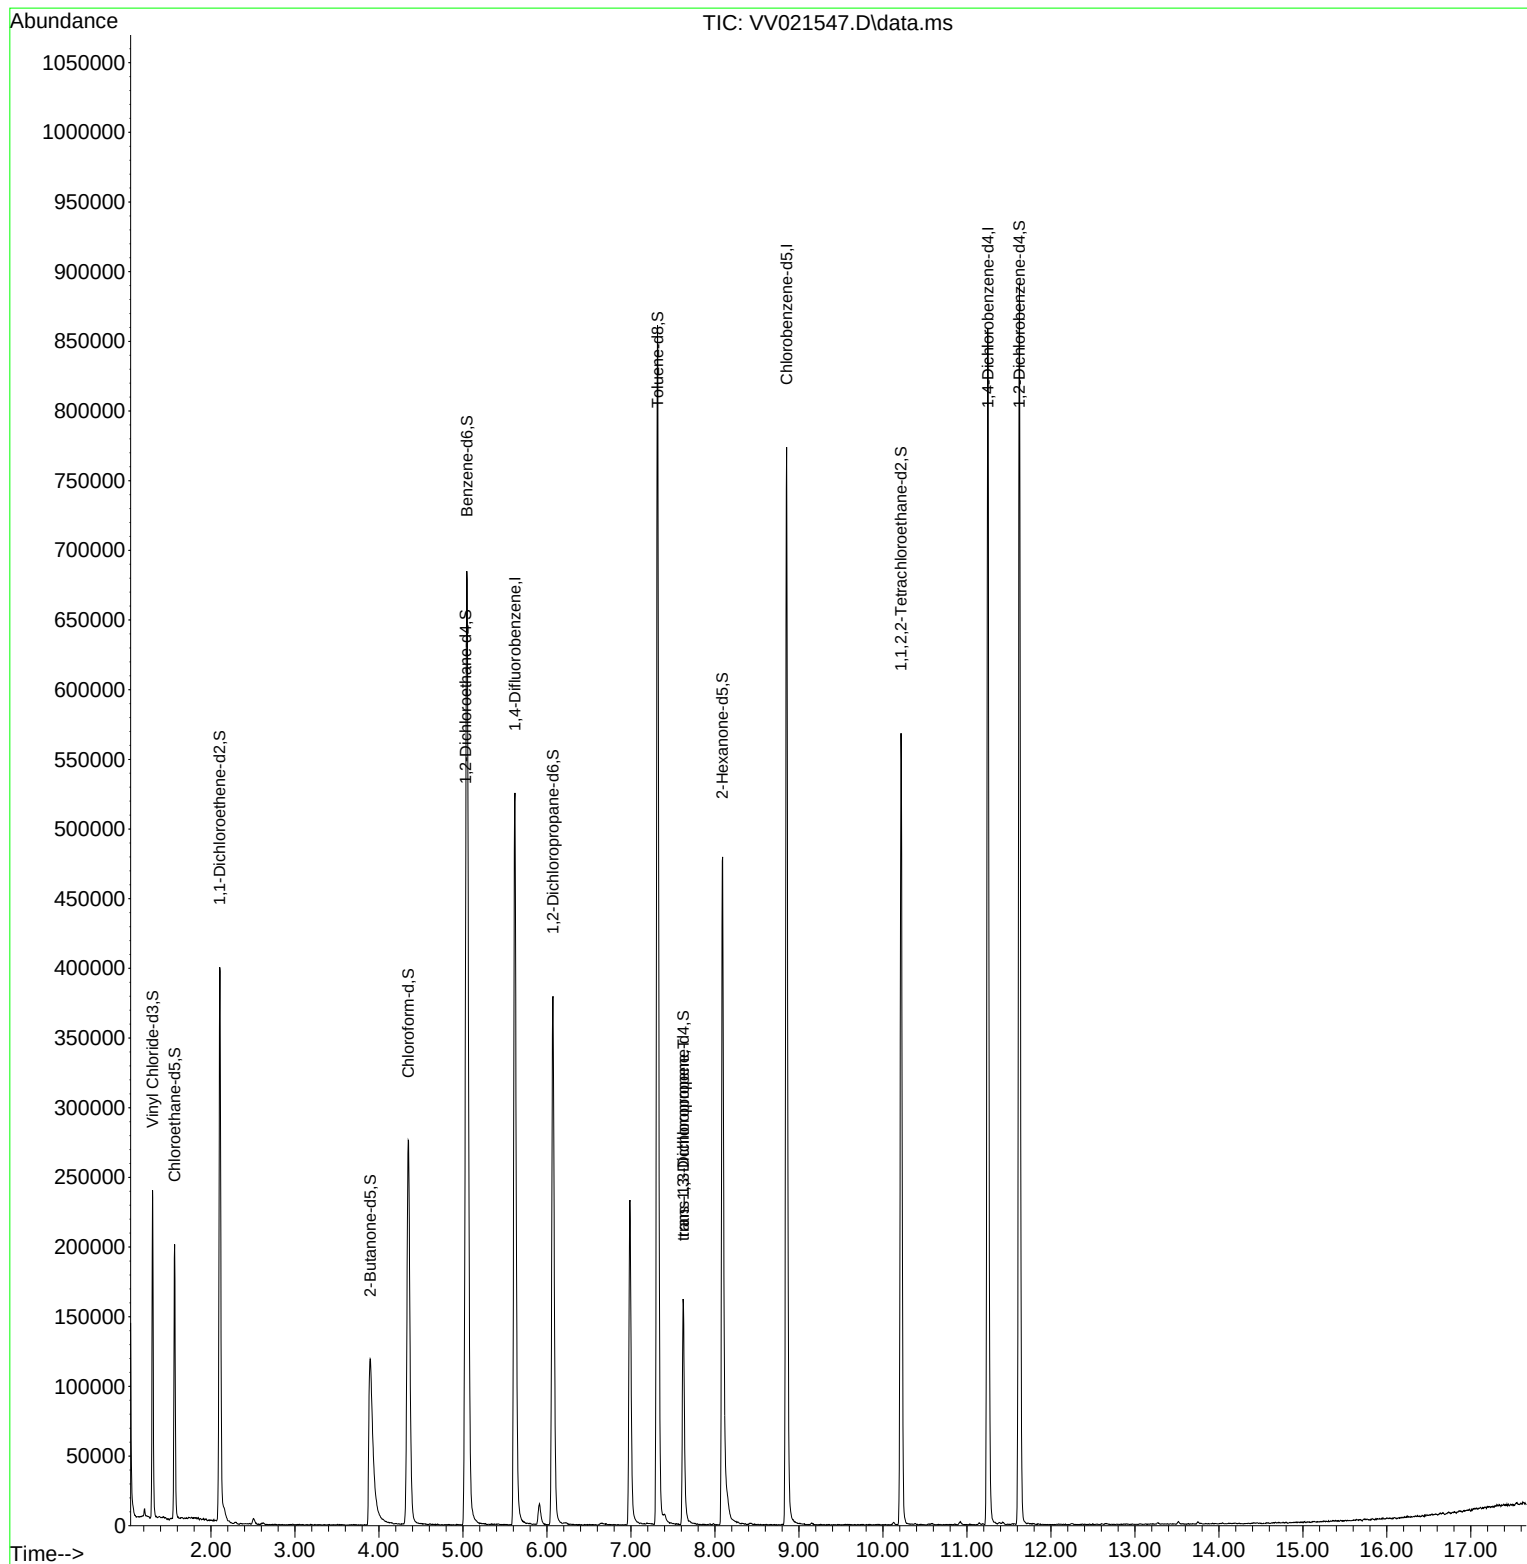

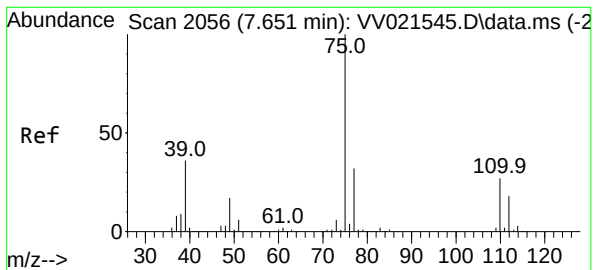

#44
 trans-1,3-Dichloropropene
 Concen: 0.708 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.026 min
 Lab File: VV021547.D
 Acq: 16 Jun 2021 13:56

Instrument :
 MSVOA_V
 ClientSampleId :

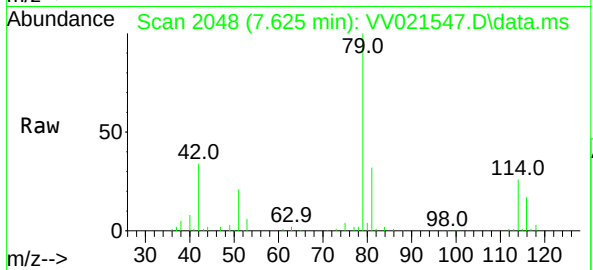

Tgt Ion: 75 Resp: 3741
 Ion Ratio Lower Upper
 75 100
 77 53.2 22.9 42.5#

