

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021546.D
 Acq On : 16 Jun 2021 13:32
 Operator : SY/MD
 Sample : VV0616MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	243554	244651	13.98%	1.779%
2	1.568	156	164	178	rBV	198023	225682	12.89%	1.641%
3	2.105	322	331	367	rVB	401321	621316	35.49%	4.517%
4	2.831	555	557	560	rBV2	292	152	0.01%	0.001%
5	2.857	561	565	570	rVB2	546	457	0.03%	0.003%
6	2.973	598	601	605	rBV2	275	234	0.01%	0.002%
7	3.008	609	612	613	rVV	217	112	0.01%	0.001%
8	3.040	617	622	631	rVB3	591	974	0.06%	0.007%
9	3.079	631	634	635	rBV3	277	124	0.01%	0.001%
10	3.159	657	659	662	rBV	352	185	0.01%	0.001%
11	3.201	668	672	673	rBV	337	200	0.01%	0.001%
12	3.327	705	711	713	rBV2	375	411	0.02%	0.003%
13	3.394	729	732	734	rBV	181	113	0.01%	0.001%
14	3.413	734	738	741	rVB4	346	284	0.02%	0.002%
15	3.442	741	747	749	rBV2	362	326	0.02%	0.002%
16	3.497	760	764	768	rVV2	293	230	0.01%	0.002%
17	3.622	800	803	804	rBV2	292	128	0.01%	0.001%
18	3.671	814	818	823	rVB3	301	238	0.01%	0.002%
19	3.761	843	846	852	rBV	159	152	0.01%	0.001%
20	3.793	852	856	858	rVV2	353	223	0.01%	0.002%
21	3.802	858	859	865	rVV2	362	238	0.01%	0.002%
22	3.892	876	887	929	rBV	112839	398169	22.75%	2.895%
23	4.346	1012	1028	1058	rBV	278963	694023	39.65%	5.046%
24	4.651	1120	1123	1126	rVB2	717	440	0.03%	0.003%
25	4.716	1141	1143	1147	rBV2	293	210	0.01%	0.002%
26	4.751	1152	1154	1156	rBV2	256	148	0.01%	0.001%
27	4.896	1197	1199	1201	rBV2	337	189	0.01%	0.001%
28	4.925	1205	1208	1211	rBV3	307	209	0.01%	0.002%
29	4.982	1221	1226	1227	rBV	310	208	0.01%	0.002%
30	5.047	1228	1246	1284	rVV2	686455	1750540	100.00%	12.728%
31	5.516	1390	1392	1393	rBV	379	170	0.01%	0.001%
32	5.616	1410	1423	1456	rBV	529744	1072761	61.28%	7.800%
33	5.908	1502	1514	1531	rBV2	15505	33673	1.92%	0.245%
34	6.069	1550	1564	1594	rBV	380215	772559	44.13%	5.617%
35	6.288	1630	1632	1635	rVB2	321	126	0.01%	0.001%
36	6.375	1655	1659	1660	rBV2	204	119	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021546.D
 Acq On : 16 Jun 2021 13:32
 Operator : SY/MD
 Sample : VV0616MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.384	1660	1662	1667	rVB3	343	223	0.01%	0.002%
38	6.413	1667	1671	1673	rBV2	245	153	0.01%	0.001%
39	6.497	1693	1697	1698	rBV2	442	305	0.02%	0.002%
40	6.535	1706	1709	1711	rVB2	577	325	0.02%	0.002%
41	6.574	1717	1721	1723	rBV2	151	109	0.01%	0.001%
42	6.587	1723	1725	1728	rVB2	231	137	0.01%	0.001%
43	6.606	1729	1731	1734	rVB2	537	235	0.01%	0.002%
44	6.635	1734	1740	1741	rBV2	1320	969	0.06%	0.007%
45	6.789	1786	1788	1792	rVB2	600	407	0.02%	0.003%
46	6.812	1792	1795	1797	rBV3	277	160	0.01%	0.001%
47	6.867	1807	1812	1814	rBV2	222	210	0.01%	0.002%
48	6.918	1824	1828	1832	rBV2	208	249	0.01%	0.002%
49	6.986	1837	1849	1883	rBV	235672	437677	25.00%	3.182%
50	7.259	1932	1934	1938	rVB3	693	381	0.02%	0.003%
51	7.317	1938	1952	1973	rBV	847673	1480389	84.57%	10.764%
52	7.622	2037	2047	2067	rBV	160791	280633	16.03%	2.040%
53	7.838	2112	2114	2117	rVB	655	301	0.02%	0.002%
54	7.921	2137	2140	2141	rBV	384	167	0.01%	0.001%
55	7.979	2155	2158	2160	rBV3	941	728	0.04%	0.005%
56	8.037	2173	2176	2181	rBV2	148	174	0.01%	0.001%
57	8.088	2181	2192	2241	rBV	440543	837862	47.86%	6.092%
58	8.500	2316	2320	2321	rBV	294	187	0.01%	0.001%
59	8.513	2321	2324	2328	rVV3	379	328	0.02%	0.002%
60	8.542	2331	2333	2334	rBV3	288	139	0.01%	0.001%
61	8.635	2360	2362	2365	rVB2	337	113	0.01%	0.001%
62	8.680	2374	2376	2380	rBV	307	215	0.01%	0.002%
63	8.715	2384	2387	2393	rBV	486	278	0.02%	0.002%
64	8.770	2401	2404	2407	rBV2	318	190	0.01%	0.001%
65	8.854	2417	2430	2451	rBV	761877	1256244	71.76%	9.134%
66	9.156	2513	2524	2531	rBV7	1620	2882	0.16%	0.021%
67	9.185	2531	2533	2535	rVV2	423	207	0.01%	0.002%
68	9.207	2539	2540	2546	rVB2	311	173	0.01%	0.001%
69	9.236	2547	2549	2552	rBV	409	200	0.01%	0.001%
70	9.281	2561	2563	2566	rVB2	311	152	0.01%	0.001%
71	9.301	2566	2569	2570	rBV	523	244	0.01%	0.002%
72	9.349	2581	2584	2590	rVB3	384	281	0.02%	0.002%
73	9.465	2617	2620	2624	rVB2	264	201	0.01%	0.001%
74	9.551	2643	2647	2648	rBV2	529	364	0.02%	0.003%
75	9.706	2693	2695	2698	rBV2	224	122	0.01%	0.001%
76	9.786	2718	2720	2723	rBV2	205	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021546.D
 Acq On : 16 Jun 2021 13:32
 Operator : SY/MD
 Sample : VV0616MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK191

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.841	2734	2737	2739	rBV2	338	204	0.01%	0.001%
78	9.889	2749	2752	2753	rBV	237	113	0.01%	0.001%
79	10.030	2794	2796	2800	rVV2	283	164	0.01%	0.001%
80	10.092	2811	2815	2817	rBV2	535	392	0.02%	0.003%
81	10.175	2837	2841	2842	rBV	396	221	0.01%	0.002%
82	10.217	2842	2854	2876	rVV	544668	863561	49.33%	6.279%
83	10.458	2927	2929	2932	rBV2	352	197	0.01%	0.001%
84	10.542	2951	2955	2956	rBV2	890	615	0.04%	0.004%
85	10.850	3046	3051	3052	rBV	672	409	0.02%	0.003%
86	10.889	3061	3063	3064	rBV	346	145	0.01%	0.001%
87	11.027	3104	3106	3109	rBV2	417	263	0.02%	0.002%
88	11.146	3137	3143	3150	rBV5	974	1521	0.09%	0.011%
89	11.188	3153	3156	3163	rBV5	1246	1295	0.07%	0.009%
90	11.249	3164	3175	3199	rBV	867259	1338016	76.43%	9.728%
91	11.577	3274	3277	3280	rBV2	511	378	0.02%	0.003%
92	11.625	3280	3292	3312	rVV	857603	1386588	79.21%	10.082%
93	12.043	3420	3422	3424	rBV	294	141	0.01%	0.001%
94	12.108	3440	3442	3447	rVB2	569	419	0.02%	0.003%
95	12.207	3471	3473	3474	rBV	361	130	0.01%	0.001%
96	12.307	3499	3504	3505	rBV	316	254	0.01%	0.002%
97	12.654	3603	3612	3619	rBV4	3415	5649	0.32%	0.041%
98	13.268	3796	3803	3818	rBV4	5141	7903	0.45%	0.057%
99	13.513	3872	3879	3889	rVB3	6894	11021	0.63%	0.080%
100	13.747	3946	3952	3964	rVB3	6282	9562	0.55%	0.070%




Sum of corrected areas: 13753571

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021546.D
Acq On : 16 Jun 2021 13:32
Operator : SY/MD
Sample : VV0616MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

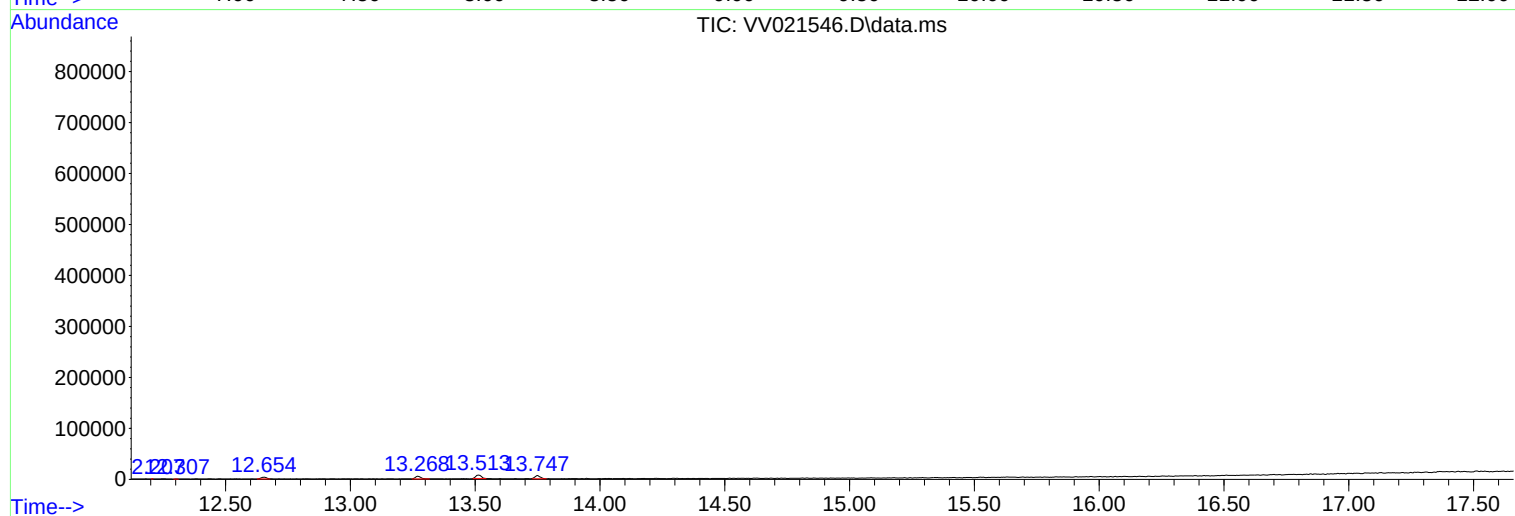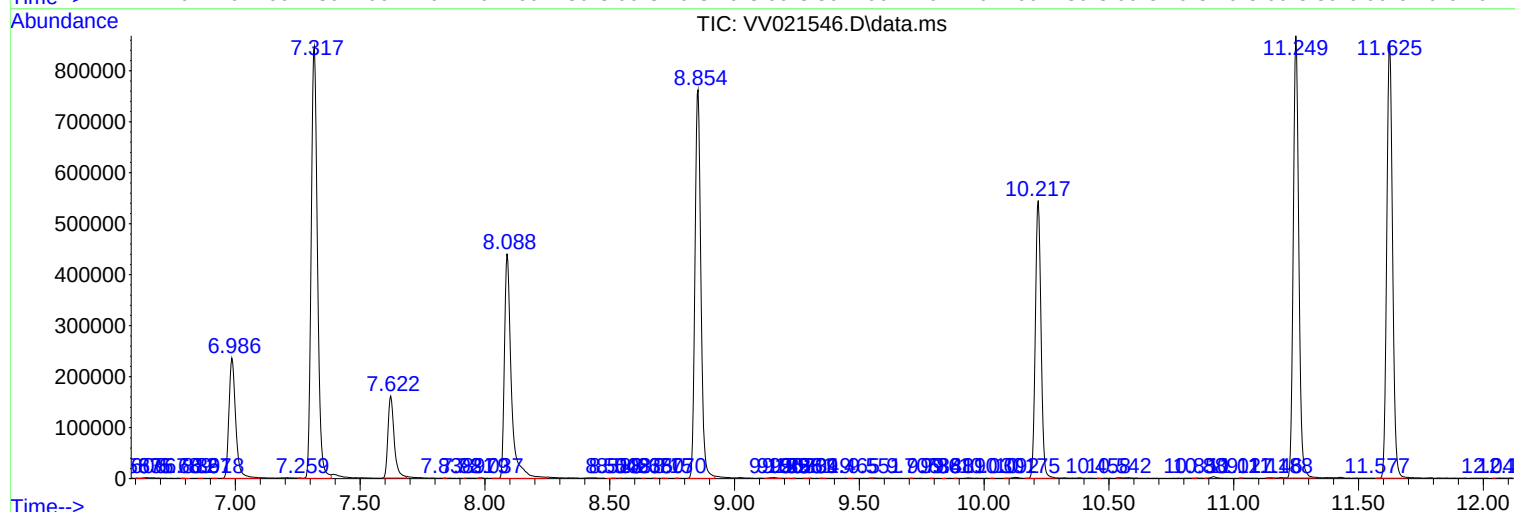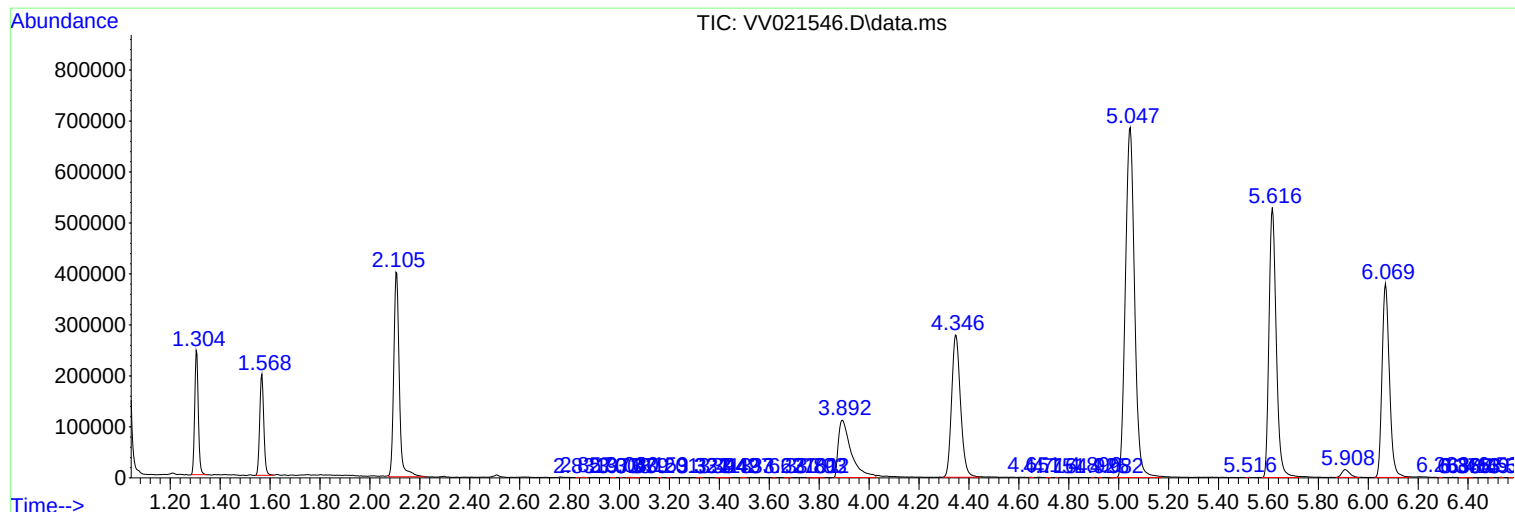

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021546.D
Acq On : 16 Jun 2021 13:32
Operator : SY/MD
Sample : VV0616MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021546.D
Acq On : 16 Jun 2021 13:32
Operator : SY/MD
Sample : VV0616MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc