

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021547.D
 Acq On : 16 Jun 2021 13:56
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK192

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	234462	237469	13.59%	1.720%
2	1.568	156	164	178	rBV	196654	221780	12.69%	1.606%
3	2.105	322	331	362	rVB	397388	602016	34.45%	4.359%
4	2.349	403	407	409	rBV3	792	618	0.04%	0.004%
5	2.664	501	505	507	rBV	431	351	0.02%	0.003%
6	2.732	524	526	530	rVB2	346	140	0.01%	0.001%
7	2.757	530	534	537	rVV3	389	355	0.02%	0.003%
8	2.783	540	542	545	rVB2	303	120	0.01%	0.001%
9	2.812	546	551	555	rBV2	347	314	0.02%	0.002%
10	3.031	616	619	621	rBV2	340	201	0.01%	0.001%
11	3.050	623	625	628	rVV2	448	269	0.02%	0.002%
12	3.185	663	667	669	rBV2	509	319	0.02%	0.002%
13	3.236	680	683	686	rBV2	385	238	0.01%	0.002%
14	3.281	694	697	698	rBV	237	118	0.01%	0.001%
15	3.336	711	714	716	rBV	172	138	0.01%	0.001%
16	3.349	716	718	721	rVV	314	170	0.01%	0.001%
17	3.371	721	725	727	rVB2	222	137	0.01%	0.001%
18	3.397	732	733	735	rVV2	283	124	0.01%	0.001%
19	3.413	735	738	742	rVB2	442	272	0.02%	0.002%
20	3.455	750	751	754	rBV	299	137	0.01%	0.001%
21	3.510	765	768	770	rVB3	488	243	0.01%	0.002%
22	3.651	809	812	814	rBV2	252	166	0.01%	0.001%
23	3.699	824	827	830	rVB2	351	203	0.01%	0.001%
24	3.825	864	866	869	rBV	286	157	0.01%	0.001%
25	3.896	877	888	933	rBV	119164	430284	24.62%	3.116%
26	4.349	1013	1029	1062	rBV	275238	684564	39.17%	4.957%
27	4.593	1102	1105	1106	rBV	425	229	0.01%	0.002%
28	4.751	1150	1154	1158	rVB3	309	264	0.02%	0.002%
29	4.780	1160	1163	1164	rBV	231	123	0.01%	0.001%
30	4.924	1205	1208	1211	rBV3	550	441	0.03%	0.003%
31	5.047	1229	1246	1290	rBV2	684562	1747599	100.00%	12.655%
32	5.333	1333	1335	1338	rBV2	371	227	0.01%	0.002%
33	5.487	1381	1383	1386	rBV2	350	216	0.01%	0.002%
34	5.548	1399	1402	1404	rBV	286	178	0.01%	0.001%
35	5.619	1411	1424	1452	rBV	525371	1057225	60.50%	7.655%
36	5.912	1504	1515	1533	rVB3	14699	32408	1.85%	0.235%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021547.D
 Acq On : 16 Jun 2021 13:56
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK192

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1593	rBV	379141	772190	44.19%	5.591%
38	6.349	1649	1651	1655	rVB3	464	287	0.02%	0.002%
39	6.387	1659	1663	1665	rBV2	436	270	0.02%	0.002%
40	6.413	1667	1671	1674	rBV2	252	144	0.01%	0.001%
41	6.449	1679	1682	1685	rBV2	339	168	0.01%	0.001%
42	6.471	1685	1689	1692	rBV2	208	167	0.01%	0.001%
43	6.513	1700	1702	1705	rVB2	374	190	0.01%	0.001%
44	6.529	1705	1707	1710	rBV	213	118	0.01%	0.001%
45	6.542	1710	1711	1714	rBV2	254	154	0.01%	0.001%
46	6.577	1720	1722	1726	rVB3	277	172	0.01%	0.001%
47	6.645	1731	1743	1745	rBV5	1424	2076	0.12%	0.015%
48	6.760	1777	1779	1781	rBV	208	122	0.01%	0.001%
49	6.799	1787	1791	1794	rBV3	226	165	0.01%	0.001%
50	6.989	1837	1850	1878	rBV	233290	428973	24.55%	3.106%
51	7.317	1939	1952	1975	rBV	860898	1490546	85.29%	10.793%
52	7.622	2037	2047	2067	rBV	161817	280762	16.07%	2.033%
53	7.793	2097	2100	2104	rVB4	496	306	0.02%	0.002%
54	7.854	2117	2119	2120	rBV	348	142	0.01%	0.001%
55	7.982	2155	2159	2164	rBV4	766	716	0.04%	0.005%
56	8.092	2181	2193	2240	rBV	479403	898698	51.42%	6.508%
57	8.397	2284	2288	2290	rBV4	519	352	0.02%	0.003%
58	8.416	2290	2294	2296	rBV3	914	753	0.04%	0.005%
59	8.545	2331	2334	2338	rVB3	360	230	0.01%	0.002%
60	8.664	2368	2371	2373	rBV2	343	205	0.01%	0.001%
61	8.696	2379	2381	2384	rBV2	185	139	0.01%	0.001%
62	8.731	2390	2392	2396	rVB2	240	131	0.01%	0.001%
63	8.760	2397	2401	2407	rBV2	354	308	0.02%	0.002%
64	8.854	2418	2430	2453	rBV	773153	1255064	71.82%	9.088%
65	9.153	2516	2523	2530	rBV4	1168	1788	0.10%	0.013%
66	9.246	2550	2552	2554	rBV	275	146	0.01%	0.001%
67	9.262	2554	2557	2560	rVV2	392	197	0.01%	0.001%
68	9.297	2565	2568	2573	rVB2	431	365	0.02%	0.003%
69	9.329	2573	2578	2580	rBV2	253	155	0.01%	0.001%
70	9.349	2580	2584	2586	rBV2	367	291	0.02%	0.002%
71	9.477	2621	2624	2630	rVB	251	230	0.01%	0.002%
72	9.583	2655	2657	2659	rVB	368	127	0.01%	0.001%
73	9.699	2690	2693	2697	rBV3	337	294	0.02%	0.002%
74	9.741	2703	2706	2710	rBV2	322	265	0.02%	0.002%
75	9.805	2724	2726	2730	rVV2	315	227	0.01%	0.002%
76	9.857	2739	2742	2745	rVB2	331	204	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021547.D
 Acq On : 16 Jun 2021 13:56
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK192

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.960	2772	2774	2779	rVB	338	203	0.01%	0.001%
78	10.034	2792	2797	2799	rBV4	271	248	0.01%	0.002%
79	10.063	2804	2806	2811	rBV2	221	161	0.01%	0.001%
80	10.101	2815	2818	2819	rBV2	354	161	0.01%	0.001%
81	10.127	2820	2826	2832	rBV3	1548	2085	0.12%	0.015%
82	10.217	2842	2854	2874	rBV	568068	892638	51.08%	6.464%
83	10.413	2913	2915	2919	rVB	374	162	0.01%	0.001%
84	10.532	2949	2952	2954	rBV	488	332	0.02%	0.002%
85	10.577	2962	2966	2968	rBV4	685	565	0.03%	0.004%
86	10.664	2992	2993	2998	rVV3	331	210	0.01%	0.002%
87	10.722	3008	3011	3015	rBV	281	208	0.01%	0.002%
88	10.854	3050	3052	3055	rVV2	492	301	0.02%	0.002%
89	10.921	3062	3073	3080	rBV7	2365	4171	0.24%	0.030%
90	11.120	3132	3135	3137	rBV	298	205	0.01%	0.001%
91	11.146	3137	3143	3149	rBV4	1374	1610	0.09%	0.012%
92	11.249	3163	3175	3199	rBV	858100	1344728	76.95%	9.737%
93	11.625	3279	3292	3320	rBV	890540	1401647	80.20%	10.149%
94	12.146	3451	3454	3457	rBV2	369	267	0.02%	0.002%
95	12.172	3460	3462	3465	rVB2	449	226	0.01%	0.002%
96	12.374	3521	3525	3530	rBV3	443	438	0.03%	0.003%
97	12.461	3549	3552	3556	rBV2	379	256	0.01%	0.002%
98	12.500	3561	3564	3567	rVB2	625	362	0.02%	0.003%
99	12.599	3592	3595	3600	rBV3	682	717	0.04%	0.005%
100	12.644	3606	3609	3612	rBV4	673	529	0.03%	0.004%




Sum of corrected areas: 13810080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021547.D
Acq On : 16 Jun 2021 13:56
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK192

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

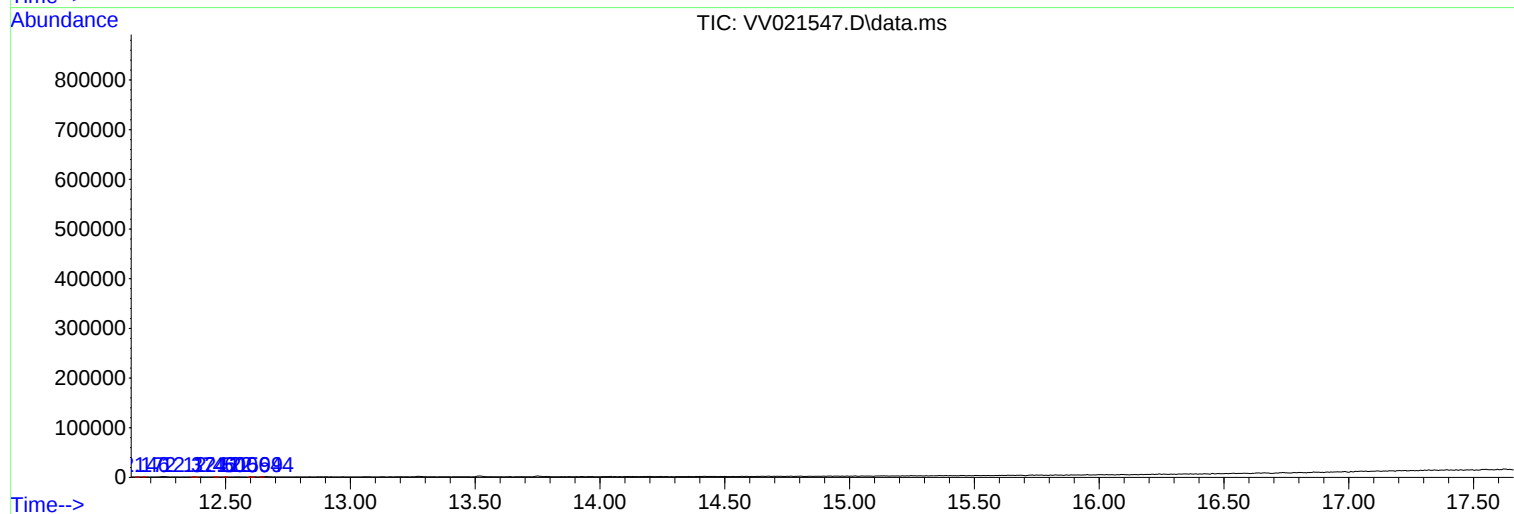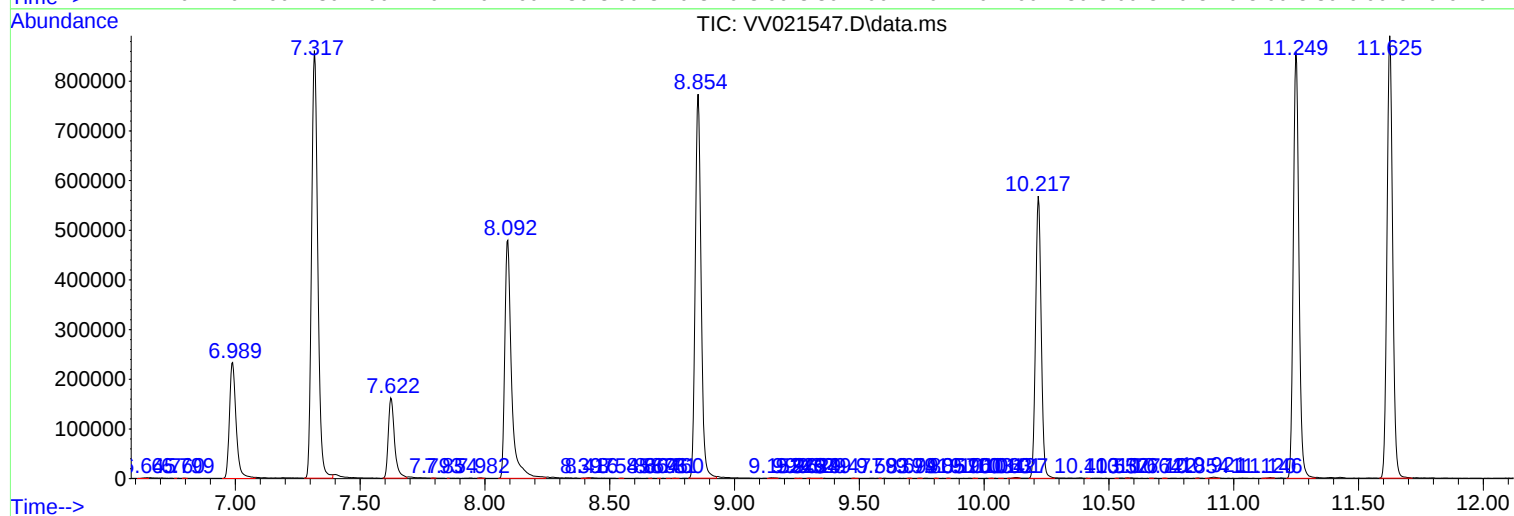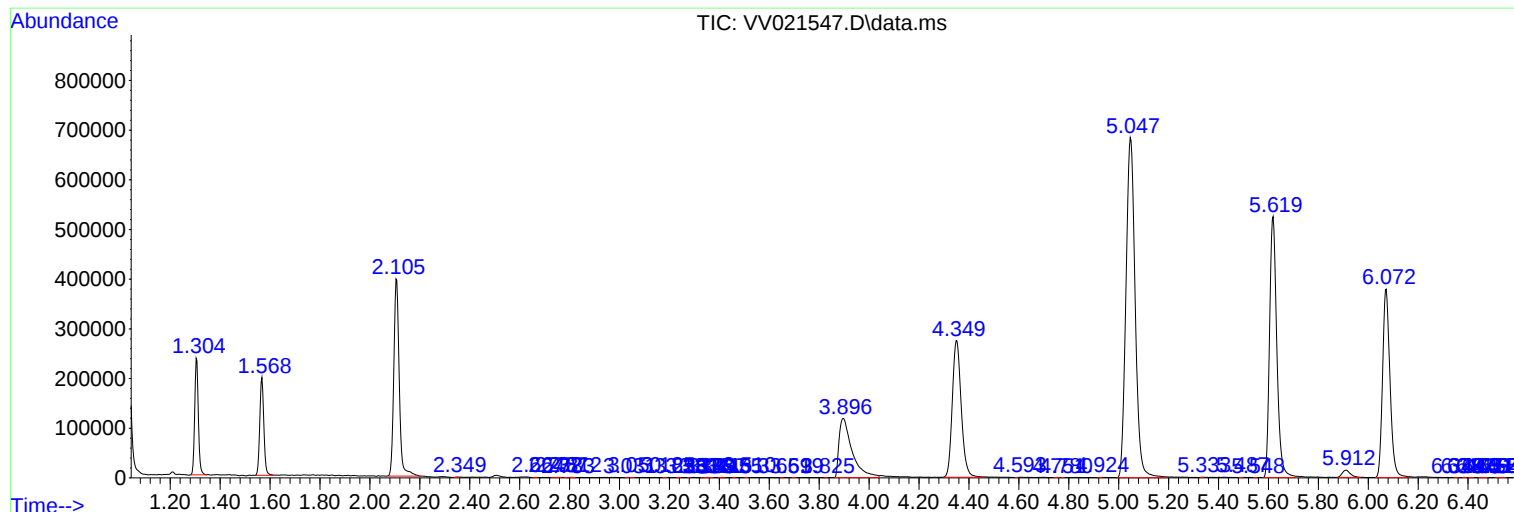

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021547.D
Acq On : 16 Jun 2021 13:56
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK192

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
Data File : VV021547.D
Acq On : 16 Jun 2021 13:56
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK192

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
