
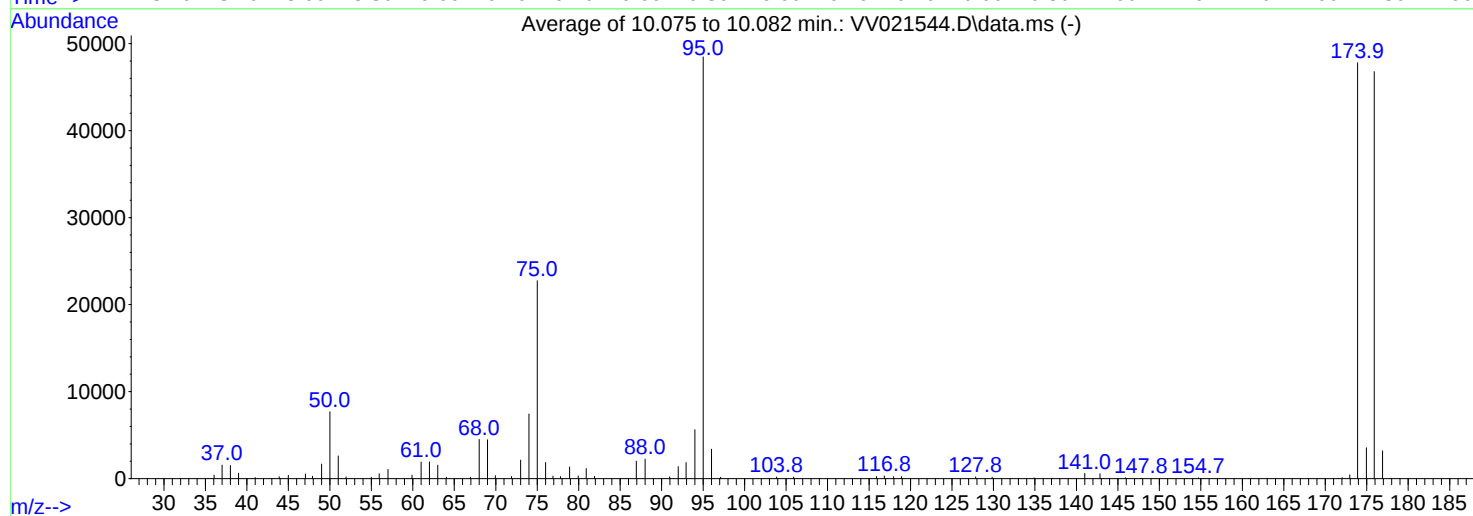


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061621\
 Data File : VV021544.D
 Acq On : 16 Jun 2021 12:36
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB170

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 17 02:01:55 2021

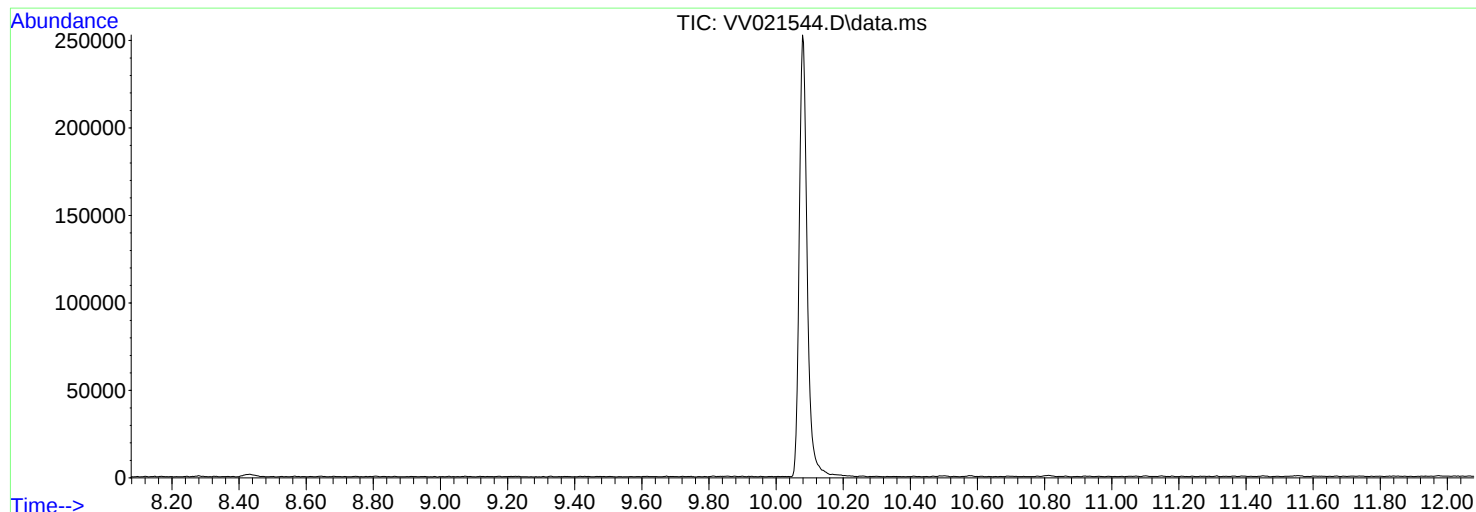

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	7690	PASS
75	95	30	80	46.9	22744	PASS
95	95	100	100	100.0	48477	PASS
96	95	5	9	7.0	3393	PASS
173	174	0.00	2	0.9	444	PASS
174	95	50	120	98.6	47795	PASS
175	174	5	9	7.4	3557	PASS
176	174	95	105	97.9	46779	PASS
177	176	5	10	6.9	3209	PASS

Scan 2800 (10.043 min): VV021544.D\data.ms
BFB70

m/z	Abundance
39.90	212.0
43.90	493.0

Instrument :
MSVOA_V
ClientSampleId :
BFB170

m/z	Abundance
36.10	373.0
37.00	1627.0
38.00	1491.0
39.00	698.0
39.90	208.0
41.00	112.0
44.00	705.0
45.00	346.0
47.10	547.0
47.90	247.0
49.00	1620.0
50.00	7516.0
51.00	2505.0
52.00	189.0
55.00	144.0
56.00	602.0
57.00	1089.0
59.90	398.0
61.00	1889.0
62.00	1964.0
63.00	1650.0
64.10	130.0
66.80	128.0
68.00	4355.0
69.00	4426.0
70.00	351.0
71.90	219.0
73.00	2223.0
74.00	7488.0
75.00	22688.0
76.00	1824.0
76.90	255.0
77.80	233.0
78.90	1377.0
79.90	361.0
80.90	1181.0
81.80	300.0
85.70	134.0
87.00	1961.0
88.00	2254.0
90.90	189.0
92.00	1336.0
92.90	1930.0
94.00	5892.0
95.00	48632.0
96.00	3436.0
97.10	141.0
103.80	184.0
105.90	197.0
115.90	235.0
116.90	301.0
118.00	194.0
118.90	262.0
127.80	215.0
129.80	169.0
134.90	138.0
141.00	657.0
142.90	538.0
145.90	123.0
147.80	117.0
154.70	119.0
172.00	175.0
173.00	444.0
173.90	49864.0
174.90	3542.0
175.90	48704.0
176.90	3229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB170

m/z	Abundance
36.10	431.0
37.00	1581.0
38.00	1541.0
39.00	646.0
40.00	213.0
41.00	140.0
44.00	716.0
45.00	390.0
47.00	541.0
47.90	289.0
49.00	1725.0
50.00	7942.0
51.00	2758.0
52.00	221.0
55.00	178.0
56.00	603.0
57.00	1112.0
59.90	417.0
61.00	1993.0
62.00	2027.0
63.00	1571.0
64.00	165.0
67.00	169.0
68.00	4680.0
69.00	4636.0
70.00	362.0
71.90	246.0
73.00	2203.0
74.00	7710.0
75.00	23520.0
76.00	1909.0
76.90	322.0
77.80	252.0
78.90	1411.0
79.90	319.0
80.90	1186.0
81.90	258.0
86.90	2079.0
88.00	2320.0
90.90	210.0
92.00	1423.0
93.00	1902.0
94.00	5751.0
95.00	50288.0
96.00	3495.0
97.10	175.0
103.80	201.0
105.90	186.0
115.90	239.0
116.90	318.0
117.90	247.0
118.90	239.0
127.80	205.0
129.80	178.0
134.90	127.0
137.10	111.0
141.00	631.0
142.80	587.0
145.90	128.0
154.70	132.0
172.10	151.0
173.00	447.0
173.90	49496.0
174.90	3663.0
175.90	48480.0
176.90	3334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB170

m/z	Abundance
36.00	396.0
37.00	1500.0
38.00	1499.0
39.00	536.0
39.90	224.0
41.00	114.0
43.90	741.0
45.00	404.0
47.00	489.0
47.90	277.0
49.00	1688.0
50.00	7613.0
51.00	2568.0
51.90	196.0
55.00	193.0
55.90	522.0
57.00	1005.0
59.90	409.0
61.00	1877.0
62.00	1800.0
63.00	1402.0
64.00	215.0
67.00	195.0
68.00	4477.0
69.00	4359.0
69.90	347.0
71.90	262.0
73.00	1961.0
74.00	7076.0
75.00	22024.0
76.00	1861.0
76.90	330.0
77.80	236.0
78.90	1253.0
80.00	290.0
80.90	1108.0
82.00	237.0
86.90	1952.0
88.00	2135.0
91.00	224.0
92.00	1382.0
93.00	1738.0
94.00	5223.0
95.00	46512.0
96.00	3247.0
97.10	164.0
103.90	185.0
105.90	164.0
115.90	221.0
116.80	306.0
117.90	243.0
118.90	216.0
127.90	194.0
129.90	176.0
141.00	525.0
142.80	575.0
145.90	105.0
155.00	121.0
157.00	117.0
160.80	118.0
171.60	119.0
172.90	441.0
173.90	44024.0
175.00	3467.0
175.90	43152.0
176.90	3065.0
177.90	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB170