

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031564.D
 Acq On : 16 Jun 2023 10:28
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK358

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	85488	90533	10.19%	1.323%
2	1.539	148	155	171	rVB	85620	103634	11.67%	1.514%
3	2.066	309	319	337	rVB	178933	259945	29.27%	3.799%
4	2.323	396	399	400	rBV2	231	128	0.01%	0.002%
5	2.455	436	440	446	rBV3	782	780	0.09%	0.011%
6	2.603	482	486	488	rBV2	373	246	0.03%	0.004%
7	2.703	513	517	520	rVB2	429	338	0.04%	0.005%
8	2.773	537	539	542	rBV2	133	57	0.01%	0.001%
9	2.799	543	547	548	rBV2	209	140	0.02%	0.002%
10	2.944	590	592	594	rBV	160	67	0.01%	0.001%
11	2.973	594	601	604	rBV2	302	342	0.04%	0.005%
12	3.063	626	629	632	rBV	321	247	0.03%	0.004%
13	3.172	659	663	670	rBV	322	410	0.05%	0.006%
14	3.365	720	723	725	rBV	161	121	0.01%	0.002%
15	3.519	766	771	776	rBV2	182	263	0.03%	0.004%
16	3.551	778	781	782	rBV2	328	211	0.02%	0.003%
17	3.616	796	801	803	rBV2	195	161	0.02%	0.002%
18	3.693	821	825	832	rVB2	228	340	0.04%	0.005%
19	3.725	833	835	838	rVB	196	91	0.01%	0.001%
20	3.744	838	841	844	rBV	311	212	0.02%	0.003%
21	3.802	849	859	886	rBV	57404	161926	18.23%	2.366%
22	4.259	984	1001	1033	rBV	147356	389917	43.91%	5.698%
23	4.629	1113	1116	1121	rBV	349	349	0.04%	0.005%
24	4.834	1179	1180	1184	rVB	178	70	0.01%	0.001%
25	4.963	1203	1220	1248	rBV2	331564	888055	100.00%	12.977%
26	5.291	1319	1322	1324	rBV2	167	88	0.01%	0.001%
27	5.481	1377	1381	1384	rBV2	208	199	0.02%	0.003%
28	5.497	1384	1386	1388	rBV	357	207	0.02%	0.003%
29	5.542	1388	1400	1427	rBV	280792	573567	64.59%	8.382%
30	5.821	1484	1487	1488	rBV2	1117	673	0.08%	0.010%
31	5.995	1528	1541	1561	rBV	206602	426697	48.05%	6.235%
32	6.227	1610	1613	1616	rBV2	346	228	0.03%	0.003%
33	6.320	1639	1642	1646	rVB2	415	329	0.04%	0.005%
34	6.346	1646	1650	1651	rBV	349	257	0.03%	0.004%
35	6.384	1660	1662	1666	rBV2	286	153	0.02%	0.002%
36	6.436	1675	1678	1680	rBV	248	204	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031564.D
 Acq On : 16 Jun 2023 10:28
 Operator : SY/MD
 Sample : VV0616WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK358

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.622	1733	1736	1739	rBV2	274	212	0.02%	0.003%
38	6.825	1796	1799	1802	rBV	199	171	0.02%	0.002%
39	6.918	1818	1828	1847	rBV	102489	189369	21.32%	2.767%
40	7.249	1919	1931	1955	rBV	362569	639311	71.99%	9.342%
41	7.558	2016	2027	2052	rBV2	77140	139533	15.71%	2.039%
42	7.792	2099	2100	2102	rBV	214	67	0.01%	0.001%
43	7.918	2137	2139	2142	rBV3	330	257	0.03%	0.004%
44	8.030	2165	2174	2204	rBV	215271	393922	44.36%	5.756%
45	8.506	2320	2322	2323	rBV	200	72	0.01%	0.001%
46	8.612	2352	2355	2360	rVB	411	258	0.03%	0.004%
47	8.651	2364	2367	2370	rVB2	294	153	0.02%	0.002%
48	8.789	2398	2410	2434	rBV	427485	709779	79.93%	10.372%
49	9.001	2474	2476	2481	rBV	269	198	0.02%	0.003%
50	9.046	2487	2490	2494	rBV2	183	181	0.02%	0.003%
51	9.149	2519	2522	2526	rVB2	359	225	0.03%	0.003%
52	9.169	2526	2528	2529	rBV	152	39	0.00%	0.001%
53	9.333	2577	2579	2584	rVB2	362	215	0.02%	0.003%
54	9.413	2601	2604	2607	rBV	285	186	0.02%	0.003%
55	9.464	2618	2620	2623	rBV	288	225	0.03%	0.003%
56	9.606	2662	2664	2668	rVB2	216	120	0.01%	0.002%
57	9.767	2711	2714	2715	rBV	223	109	0.01%	0.002%
58	9.870	2743	2746	2748	rBV2	354	229	0.03%	0.003%
59	10.075	2808	2810	2813	rBV	214	97	0.01%	0.001%
60	10.107	2817	2820	2822	rBV	234	163	0.02%	0.002%
61	10.159	2824	2836	2857	rBV	314015	490535	55.24%	7.168%
62	10.323	2882	2887	2892	rBV3	492	545	0.06%	0.008%
63	10.435	2917	2922	2924	rBV	328	275	0.03%	0.004%
64	10.484	2933	2937	2943	rVB3	414	467	0.05%	0.007%
65	10.558	2959	2960	2964	rVB	272	73	0.01%	0.001%
66	10.844	3046	3049	3050	rBV2	198	135	0.02%	0.002%
67	11.191	3145	3157	3178	rBV	450786	679123	76.47%	9.924%
68	11.567	3262	3274	3296	rBV	442222	683421	76.96%	9.987%
69	12.072	3427	3431	3435	rBV3	385	354	0.04%	0.005%
70	12.107	3440	3442	3444	rBV	240	139	0.02%	0.002%
71	12.715	3630	3631	3634	rBV	218	142	0.02%	0.002%
72	13.207	3781	3784	3795	rVB5	1838	2369	0.27%	0.035%
73	13.252	3795	3798	3803	rBV2	301	340	0.04%	0.005%
74	13.451	3852	3860	3866	rBV5	3781	5447	0.61%	0.080%
75	13.509	3876	3878	3881	rBV	327	199	0.02%	0.003%
76	13.686	3928	3933	3945	rVB6	2061	2760	0.31%	0.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031564.D
Acq On : 16 Jun 2023 10:28
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis

77	14.130	4068	4071	4073	rBV2	477	304	0.03%	0.004%
78	14.207	4092	4095	4098	rBV3	489	293	0.03%	0.004%




Sum of corrected areas: 6843197

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031564.D
Acq On : 16 Jun 2023 10:28
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

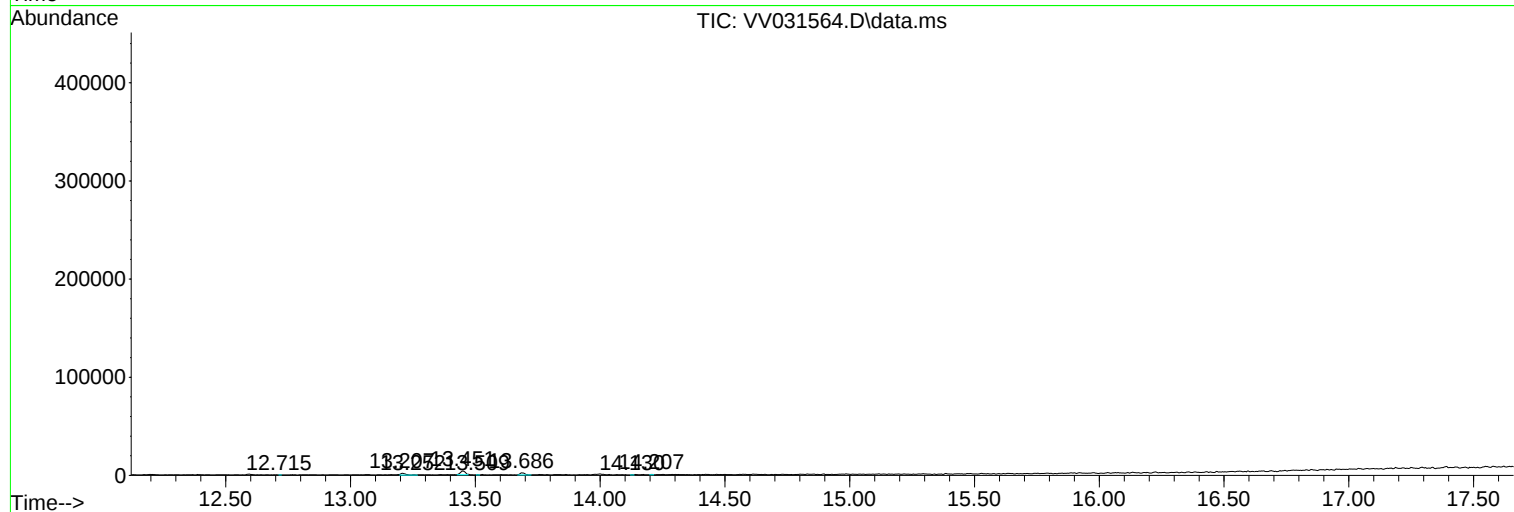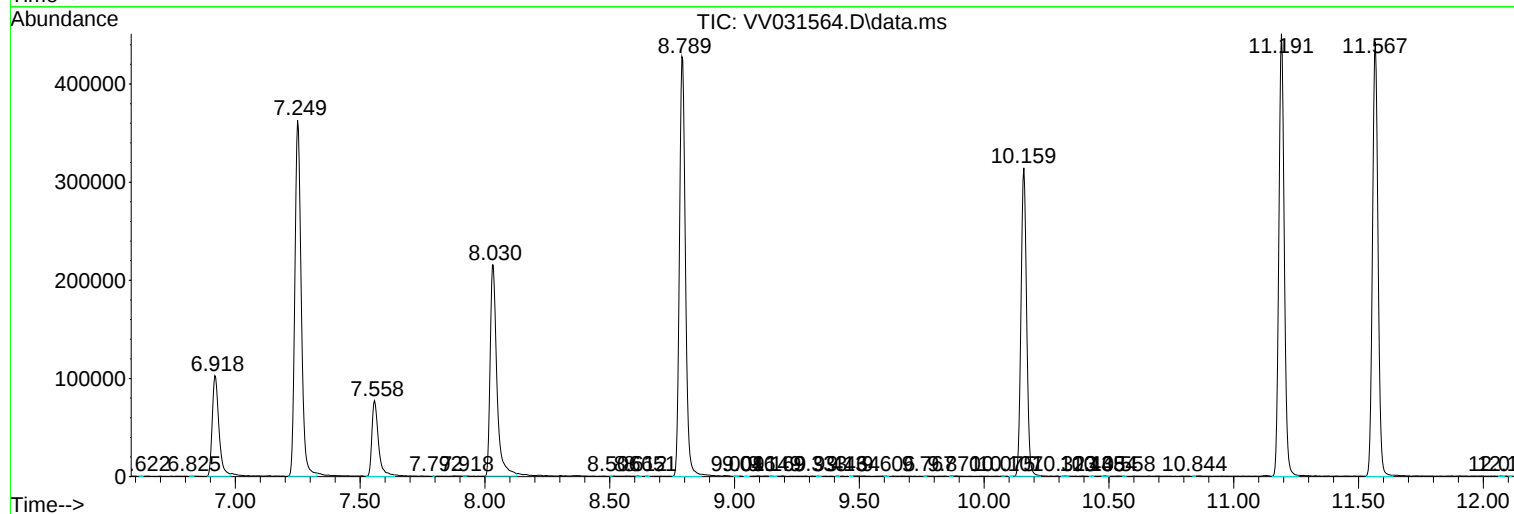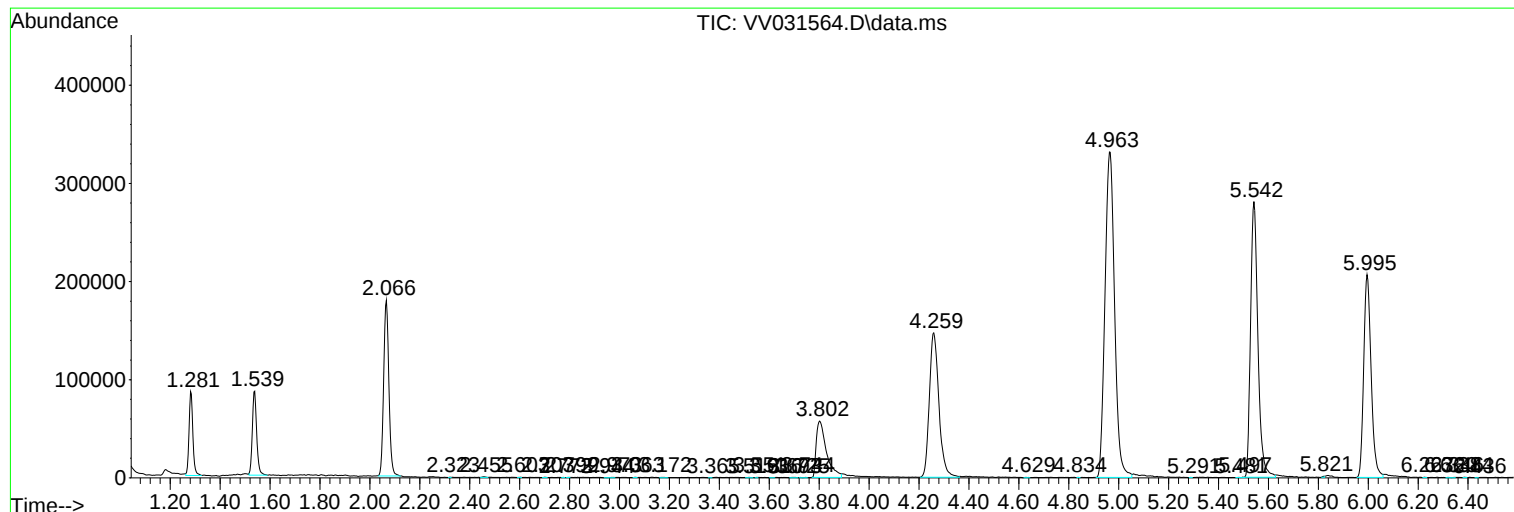

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031564.D
Acq On : 16 Jun 2023 10:28
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031564.D
Acq On : 16 Jun 2023 10:28
Operator : SY/MD
Sample : VV0616WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------