

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031565.D
 Acq On : 16 Jun 2023 10:55
 Operator : SY/MD
 Sample : 03254-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYY9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	86274	91249	10.25%	1.187%
2	1.536	148	154	170	rVB	84437	100771	11.32%	1.310%
3	2.066	309	319	337	rBV3	213453	348347	39.14%	4.530%
4	2.217	364	366	369	rBV3	444	261	0.03%	0.003%
5	2.397	421	422	426	rVB2	301	133	0.01%	0.002%
6	2.455	433	440	448	rVB3	1336	1968	0.22%	0.026%
7	2.622	491	492	493	rBV3	148	31	0.00%	0.000%
8	2.706	511	518	530	rVB4	2246	4110	0.46%	0.053%
9	2.761	530	535	537	rBV2	306	319	0.04%	0.004%
10	2.790	542	544	548	rVV2	235	142	0.02%	0.002%
11	2.844	556	561	564	rBV2	205	236	0.03%	0.003%
12	2.912	580	582	583	rBV	226	83	0.01%	0.001%
13	2.931	586	588	591	rBV	169	74	0.01%	0.001%
14	2.950	591	594	598	rBV2	331	289	0.03%	0.004%
15	2.999	607	609	613	rBV2	203	209	0.02%	0.003%
16	3.018	613	615	617	rVV2	190	82	0.01%	0.001%
17	3.050	622	625	627	rBV2	352	238	0.03%	0.003%
18	3.121	632	647	664	rVV	48022	99634	11.19%	1.296%
19	3.236	678	683	685	rBV	522	392	0.04%	0.005%
20	3.352	716	719	721	rBV	244	196	0.02%	0.003%
21	3.407	733	736	738	rVB	229	111	0.01%	0.001%
22	3.417	738	739	740	rBV	155	46	0.01%	0.001%
23	3.471	752	756	758	rBV	237	185	0.02%	0.002%
24	3.555	780	782	783	rBV	207	72	0.01%	0.001%
25	3.648	807	811	814	rVB2	280	204	0.02%	0.003%
26	3.687	814	823	824	rBV2	332	313	0.04%	0.004%
27	3.802	848	859	895	rBV2	69150	236976	26.62%	3.082%
28	4.259	983	1001	1033	rBV	147911	395467	44.43%	5.143%
29	4.519	1065	1082	1107	rBV2	150470	383275	43.06%	4.984%
30	4.764	1155	1158	1163	rBV3	348	288	0.03%	0.004%
31	4.963	1202	1220	1253	rBV2	333092	890108	100.00%	11.575%
32	5.275	1315	1317	1322	rBV3	257	175	0.02%	0.002%
33	5.349	1339	1340	1341	rBV3	226	80	0.01%	0.001%
34	5.410	1356	1359	1363	rBV4	292	215	0.02%	0.003%
35	5.542	1387	1400	1429	rBV	280765	581490	65.33%	7.562%
36	5.802	1479	1481	1483	rBV2	463	279	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031565.D
 Acq On : 16 Jun 2023 10:55
 Operator : SY/MD
 Sample : 03254-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYY9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.844	1483	1494	1512	rVV4	26435	55354	6.22%	0.720%
38	5.995	1528	1541	1565	rBV	208889	429067	48.20%	5.580%
39	6.211	1607	1608	1613	rBB	212	86	0.01%	0.001%
40	6.246	1616	1619	1623	rVB3	422	278	0.03%	0.004%
41	6.452	1680	1683	1685	rBV	275	211	0.02%	0.003%
42	6.609	1728	1732	1736	rBV	297	246	0.03%	0.003%
43	6.918	1817	1828	1850	rBV2	101921	189188	21.25%	2.460%
44	7.166	1903	1905	1908	rBV2	161	62	0.01%	0.001%
45	7.249	1918	1931	1952	rBV	364021	639546	71.85%	8.317%
46	7.558	2017	2027	2055	rBV2	77628	137882	15.49%	1.793%
47	7.725	2077	2079	2082	rBV2	367	253	0.03%	0.003%
48	7.786	2092	2098	2101	rBV6	1173	1399	0.16%	0.018%
49	7.912	2126	2137	2154	rBV2	57595	97513	10.96%	1.268%
50	8.030	2164	2174	2206	rBV	218863	400222	44.96%	5.205%
51	8.465	2304	2309	2315	rBV3	269	326	0.04%	0.004%
52	8.619	2356	2357	2358	rBV3	289	86	0.01%	0.001%
53	8.648	2362	2366	2370	rVB2	309	223	0.03%	0.003%
54	8.693	2379	2380	2383	rBV2	203	107	0.01%	0.001%
55	8.747	2393	2397	2398	rBV	245	195	0.02%	0.003%
56	8.789	2398	2410	2435	rBV	439821	715944	80.43%	9.310%
57	8.992	2472	2473	2474	rBV	153	49	0.01%	0.001%
58	9.153	2518	2523	2524	rBV	334	252	0.03%	0.003%
59	9.310	2569	2572	2574	rBV	341	189	0.02%	0.002%
60	9.400	2597	2600	2603	rBV	272	150	0.02%	0.002%
61	9.574	2650	2654	2656	rBV2	169	127	0.01%	0.002%
62	9.651	2674	2678	2679	rBV2	246	168	0.02%	0.002%
63	9.693	2688	2691	2695	rBV2	381	311	0.03%	0.004%
64	9.934	2763	2766	2767	rBV2	237	129	0.01%	0.002%
65	10.027	2793	2795	2798	rBV	250	172	0.02%	0.002%
66	10.159	2824	2836	2857	rBV	310086	489683	55.01%	6.368%
67	10.371	2900	2902	2903	rBV	277	109	0.01%	0.001%
68	10.423	2915	2918	2923	rVB2	340	229	0.03%	0.003%
69	10.458	2926	2929	2932	rVB	305	180	0.02%	0.002%
70	10.805	3033	3037	3040	rBV	318	205	0.02%	0.003%
71	10.821	3040	3042	3043	rBV	143	78	0.01%	0.001%
72	10.908	3067	3069	3070	rBV	82	41	0.00%	0.001%
73	10.915	3070	3071	3074	rVB2	221	113	0.01%	0.001%
74	10.934	3074	3077	3078	rBV2	112	63	0.01%	0.001%
75	10.950	3080	3082	3085	rBV2	198	133	0.01%	0.002%
76	10.963	3085	3086	3090	rBV	171	139	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031565.D
 Acq On : 16 Jun 2023 10:55
 Operator : SY/MD
 Sample : 03254-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYY9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.021	3101	3104	3109	rVB3	369	302	0.03%	0.004%
78	11.191	3145	3157	3182	rBV	449842	692069	77.75%	9.000%
79	11.567	3262	3274	3296	rBV	448495	688271	77.32%	8.951%
80	11.731	3322	3325	3328	rBV2	348	268	0.03%	0.003%
81	11.792	3341	3344	3351	rBV	359	391	0.04%	0.005%
82	12.017	3411	3414	3416	rBV2	325	227	0.03%	0.003%
83	12.046	3420	3423	3426	rVV2	357	190	0.02%	0.002%
84	12.085	3430	3435	3438	rBV2	330	380	0.04%	0.005%
85	12.345	3512	3516	3517	rBV	245	167	0.02%	0.002%
86	12.426	3538	3541	3547	rBV3	411	426	0.05%	0.006%
87	12.551	3577	3580	3581	rBV	309	187	0.02%	0.002%
88	12.587	3588	3591	3593	rBV2	794	545	0.06%	0.007%
89	12.648	3608	3610	3612	rBV2	300	191	0.02%	0.002%
90	12.699	3623	3626	3628	rBV2	322	236	0.03%	0.003%
91	13.085	3739	3746	3752	rBV2	370	662	0.07%	0.009%
92	13.114	3752	3755	3761	rBV	317	332	0.04%	0.004%
93	13.152	3765	3767	3770	rBV	429	261	0.03%	0.003%
94	13.451	3852	3860	3873	rVB2	2195	3289	0.37%	0.043%
95	13.693	3929	3935	3940	rBV5	1462	1677	0.19%	0.022%
96	13.786	3961	3964	3967	rVB	601	443	0.05%	0.006%
97	13.805	3967	3970	3972	rBV	292	209	0.02%	0.003%
98	13.959	4016	4018	4020	rBV2	365	144	0.02%	0.002%
99	14.191	4088	4090	4091	rBV2	298	93	0.01%	0.001%




Sum of corrected areas: 7689716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031565.D
Acq On : 16 Jun 2023 10:55
Operator : SY/MD
Sample : 03254-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYY9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

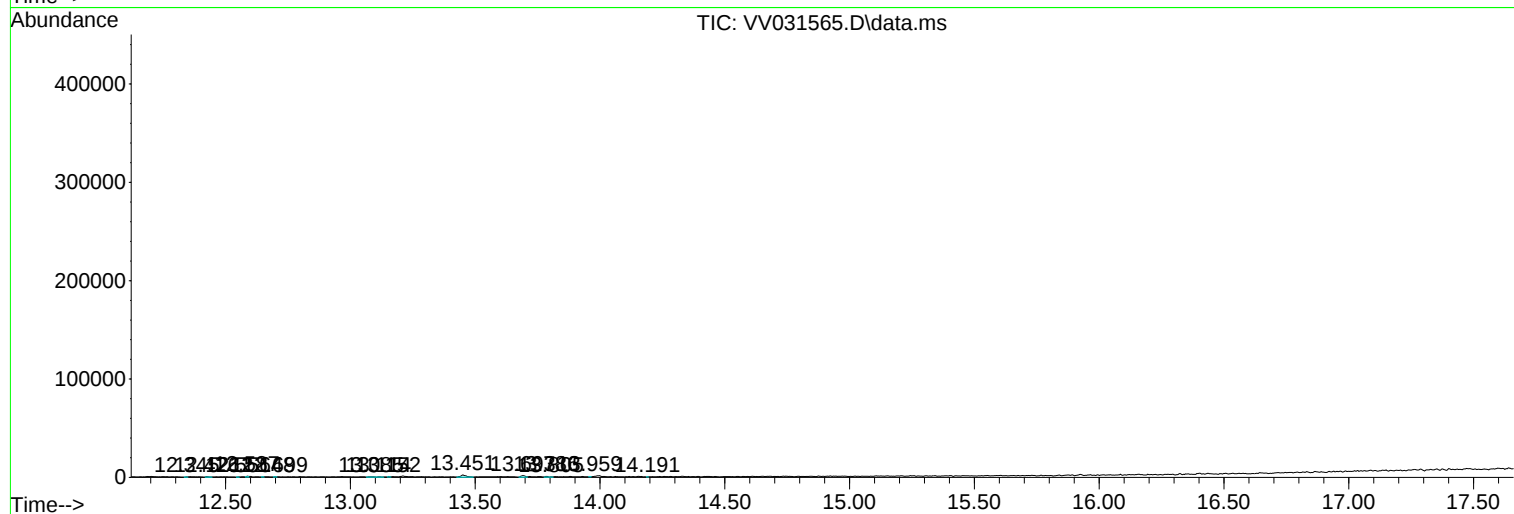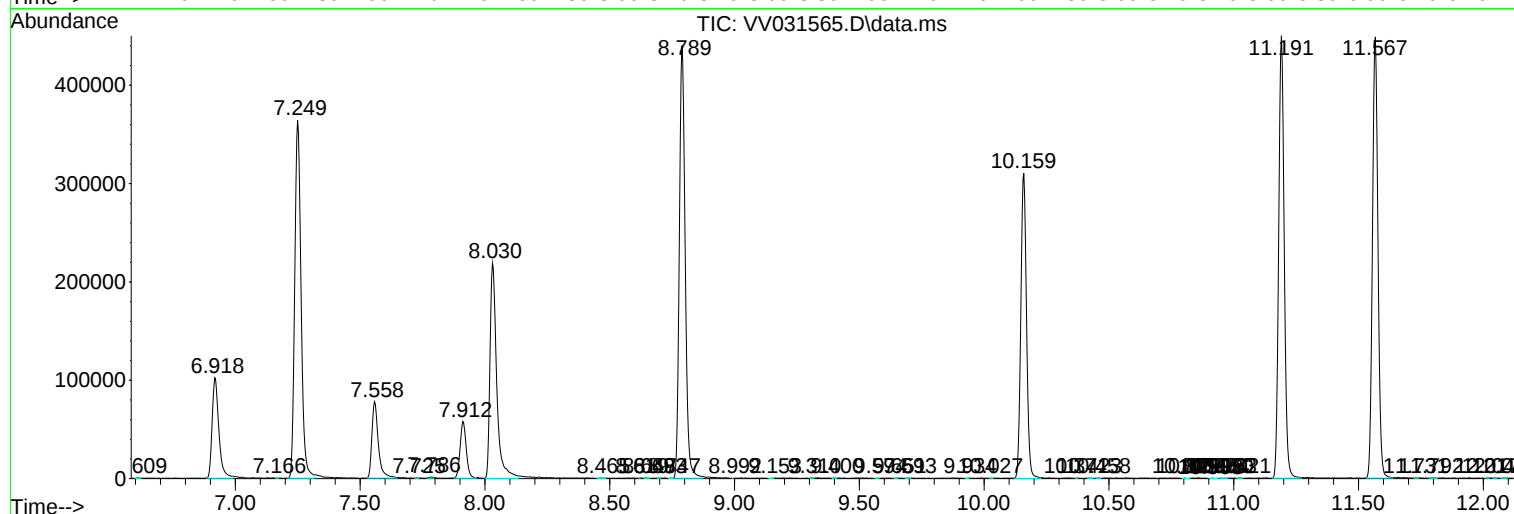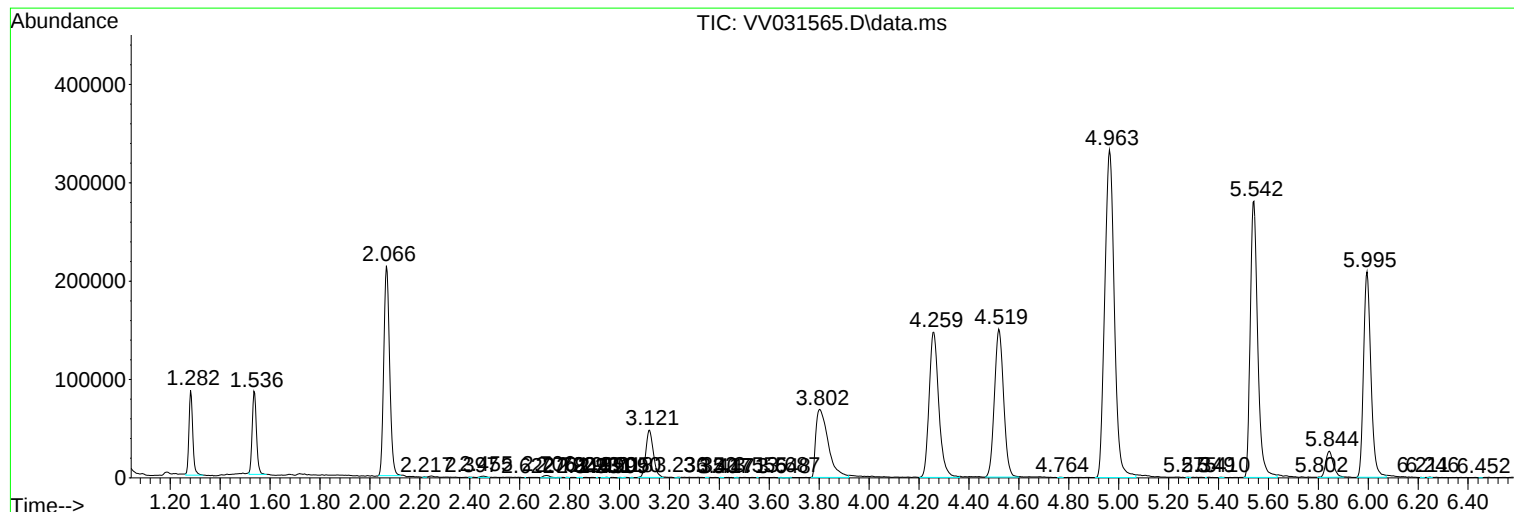

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031565.D
Acq On : 16 Jun 2023 10:55
Operator : SY/MD
Sample : 03254-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYY9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031565.D
Acq On : 16 Jun 2023 10:55
Operator : SY/MD
Sample : 03254-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYY9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------