

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031566.D
 Acq On : 16 Jun 2023 11:18
 Operator : SY/MD
 Sample : 03254-03DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VW031566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	93	rVB	89329	98913	11.47%	1.221%
2	1.536	148	154	171	rVB	82323	107743	12.49%	1.330%
3	2.066	309	319	337	rBV	176585	259787	30.11%	3.207%
4	2.240	370	373	376	rBV2	684	486	0.06%	0.006%
5	2.352	405	408	411	rBV2	361	216	0.03%	0.003%
6	2.384	416	418	422	rBV3	252	212	0.02%	0.003%
7	2.458	434	441	446	rBV4	1341	1920	0.22%	0.024%
8	2.529	460	463	466	rBV	336	256	0.03%	0.003%
9	2.561	470	473	482	rVB3	732	986	0.11%	0.012%
10	2.642	496	498	501	rBV2	182	90	0.01%	0.001%
11	2.709	511	519	528	rVB5	2405	4162	0.48%	0.051%
12	2.793	540	545	546	rBV	169	137	0.02%	0.002%
13	2.838	556	559	563	rVB3	357	291	0.03%	0.004%
14	2.864	563	567	570	rBV	189	177	0.02%	0.002%
15	2.938	587	590	591	rBV	223	97	0.01%	0.001%
16	3.047	621	624	626	rBV	288	149	0.02%	0.002%
17	3.121	631	647	672	rVV	90745	188928	21.90%	2.332%
18	3.449	745	749	755	rBV3	246	255	0.03%	0.003%
19	3.651	809	812	815	rBV	184	126	0.01%	0.002%
20	3.735	834	838	841	rVB2	222	163	0.02%	0.002%
21	3.761	841	846	848	rBV2	343	317	0.04%	0.004%
22	3.822	848	865	895	rBV2	307022	862722	100.00%	10.651%
23	4.259	986	1001	1034	rBV	141633	372814	43.21%	4.603%
24	4.523	1067	1083	1104	rVB2	146787	370560	42.95%	4.575%
25	4.719	1142	1144	1148	rBV2	168	100	0.01%	0.001%
26	4.738	1148	1150	1155	rBV2	354	235	0.03%	0.003%
27	4.966	1203	1221	1246	rBV2	327752	860265	99.72%	10.621%
28	5.265	1309	1314	1317	rBV4	352	319	0.04%	0.004%
29	5.542	1387	1400	1431	rBV	275411	569999	66.07%	7.037%
30	5.851	1485	1496	1514	rVB8	4592	10035	1.16%	0.124%
31	5.931	1515	1521	1526	rBV4	316	445	0.05%	0.005%
32	5.995	1527	1541	1568	rBV	201555	418991	48.57%	5.173%
33	6.188	1600	1601	1603	rVB	350	91	0.01%	0.001%
34	6.249	1618	1620	1623	rBV	202	101	0.01%	0.001%
35	6.278	1627	1629	1634	rVB2	360	256	0.03%	0.003%
36	6.452	1680	1683	1685	rBV2	203	138	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031566.D
 Acq On : 16 Jun 2023 11:18
 Operator : SY/MD
 Sample : 03254-03DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.532	1706	1708	1710	rVB	367	119	0.01%	0.001%
38	6.654	1742	1746	1749	rBV2	167	152	0.02%	0.002%
39	6.719	1764	1766	1768	rVB	278	117	0.01%	0.001%
40	6.741	1768	1773	1777	rBV2	293	349	0.04%	0.004%
41	6.918	1817	1828	1845	rBV	99222	181460	21.03%	2.240%
42	7.249	1919	1931	1951	rBV	347434	613040	71.06%	7.568%
43	7.558	2017	2027	2053	rBV2	74327	133857	15.52%	1.653%
44	7.712	2073	2075	2078	rVB2	314	147	0.02%	0.002%
45	7.850	2114	2118	2122	rBV2	328	361	0.04%	0.004%
46	7.915	2130	2138	2148	rVB4	5351	8842	1.02%	0.109%
47	8.031	2164	2174	2203	rBV	216670	393202	45.58%	4.854%
48	8.410	2288	2292	2293	rBV2	331	219	0.03%	0.003%
49	8.452	2303	2305	2311	rVB3	376	334	0.04%	0.004%
50	8.580	2343	2345	2348	rBV2	218	122	0.01%	0.002%
51	8.632	2359	2361	2365	rVB	300	168	0.02%	0.002%
52	8.703	2381	2383	2386	rVB2	207	108	0.01%	0.001%
53	8.789	2399	2410	2437	rBV	427565	702574	81.44%	8.674%
54	9.053	2491	2492	2494	rBV	258	107	0.01%	0.001%
55	9.085	2494	2502	2516	rVB3	7030	11610	1.35%	0.143%
56	9.182	2530	2532	2535	rBV2	183	109	0.01%	0.001%
57	9.313	2570	2573	2576	rBV2	239	147	0.02%	0.002%
58	9.333	2577	2579	2583	rVB2	283	188	0.02%	0.002%
59	9.381	2592	2594	2598	rBV	285	164	0.02%	0.002%
60	9.410	2602	2603	2607	rVV	217	111	0.01%	0.001%
61	9.487	2619	2627	2643	rVB3	7651	12744	1.48%	0.157%
62	9.670	2680	2684	2686	rBV2	229	167	0.02%	0.002%
63	9.706	2692	2695	2698	rBV2	370	313	0.04%	0.004%
64	9.821	2726	2731	2737	rBV2	189	276	0.03%	0.003%
65	9.921	2759	2762	2763	rBV2	197	115	0.01%	0.001%
66	9.963	2772	2775	2776	rBV	272	146	0.02%	0.002%
67	9.976	2776	2779	2780	rBV	193	104	0.01%	0.001%
68	10.050	2800	2802	2805	rVB	255	116	0.01%	0.001%
69	10.069	2805	2808	2815	rBV	297	371	0.04%	0.005%
70	10.159	2824	2836	2862	rBV	304168	479237	55.55%	5.916%
71	10.394	2903	2909	2913	rBV5	3844	5231	0.61%	0.065%
72	10.484	2929	2937	2947	rBV2	5567	7305	0.85%	0.090%
73	10.522	2947	2949	2952	rVB2	331	160	0.02%	0.002%
74	10.683	2988	2999	3010	rBV2	5734	8604	1.00%	0.106%
75	10.860	3046	3054	3066	rVB2	12238	17784	2.06%	0.220%
76	11.024	3103	3105	3107	rBV2	450	213	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031566.D
 Acq On : 16 Jun 2023 11:18
 Operator : SY/MD
 Sample : 03254-03DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.191	3146	3157	3176	rBV	449047	688002	79.75%	8.494%
78	11.278	3179	3184	3197	rVB	9060	13197	1.53%	0.163%
79	11.400	3220	3222	3224	rVB	265	109	0.01%	0.001%
80	11.416	3224	3227	3228	rBV2	327	202	0.02%	0.002%
81	11.474	3240	3245	3250	rBV4	2132	2435	0.28%	0.030%
82	11.567	3263	3274	3293	rBV	427579	663872	76.95%	8.196%
83	11.825	3352	3354	3359	rBV3	388	194	0.02%	0.002%
84	11.870	3359	3368	3382	rVB5	6391	10703	1.24%	0.132%
85	12.018	3411	3414	3416	rBV2	316	252	0.03%	0.003%
86	12.146	3452	3454	3458	rBV2	208	167	0.02%	0.002%
87	12.300	3500	3502	3503	rBV2	261	93	0.01%	0.001%
88	12.542	3573	3577	3584	rBV3	444	536	0.06%	0.007%
89	12.857	3672	3675	3676	rBV	254	135	0.02%	0.002%
90	12.982	3710	3714	3717	rBV	301	283	0.03%	0.003%
91	13.172	3770	3773	3776	rVB2	340	216	0.03%	0.003%
92	13.255	3793	3799	3805	rBV3	379	545	0.06%	0.007%
93	13.284	3805	3808	3810	rBV2	289	211	0.02%	0.003%
94	13.455	3852	3861	3869	rVB5	2285	3581	0.42%	0.044%
95	13.493	3869	3873	3875	rBV2	404	324	0.04%	0.004%
96	13.596	3903	3905	3909	rVB	429	268	0.03%	0.003%
97	13.693	3930	3935	3940	rBV4	993	871	0.10%	0.011%
98	13.744	3948	3951	3954	rBV2	356	247	0.03%	0.003%
99	14.059	4047	4049	4051	rBV2	421	269	0.03%	0.003%
100	14.821	4284	4286	4287	rBV2	754	336	0.04%	0.004%




Sum of corrected areas: 8100023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031566.D
Acq On : 16 Jun 2023 11:18
Operator : SY/MD
Sample : 03254-03DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

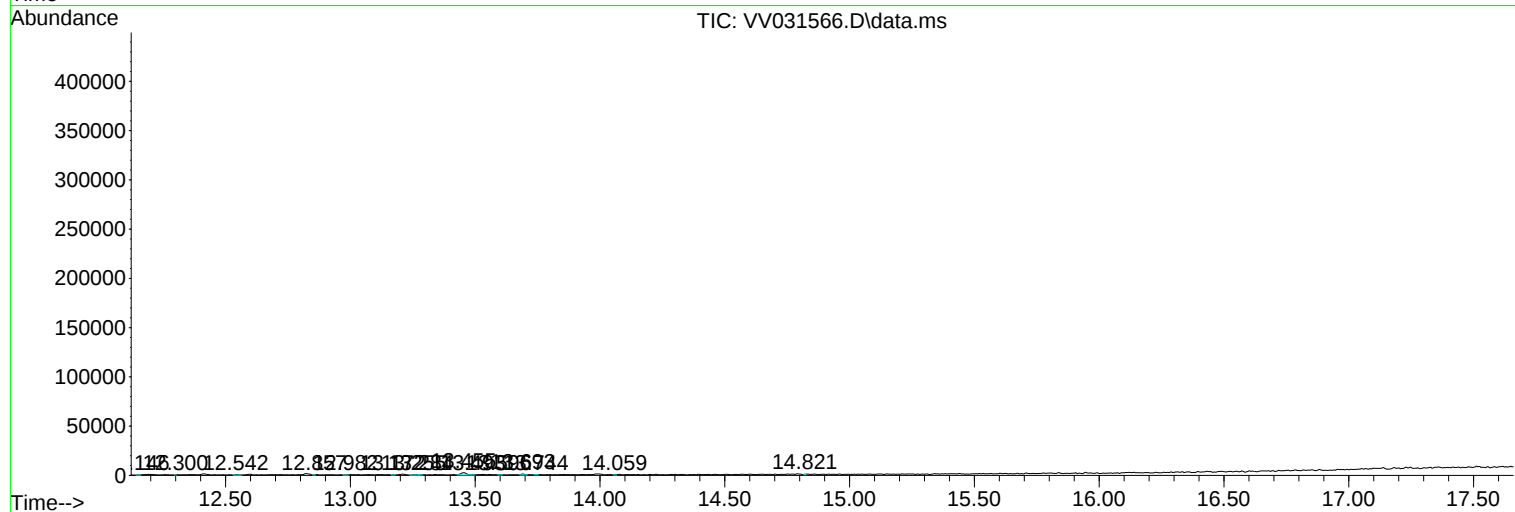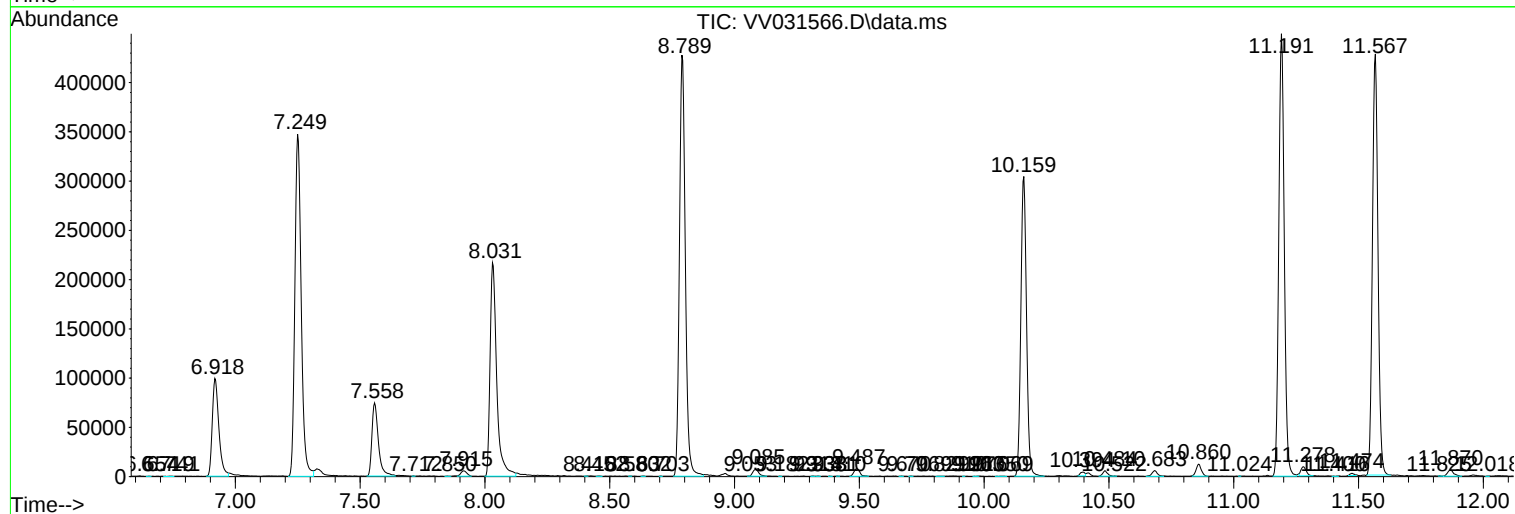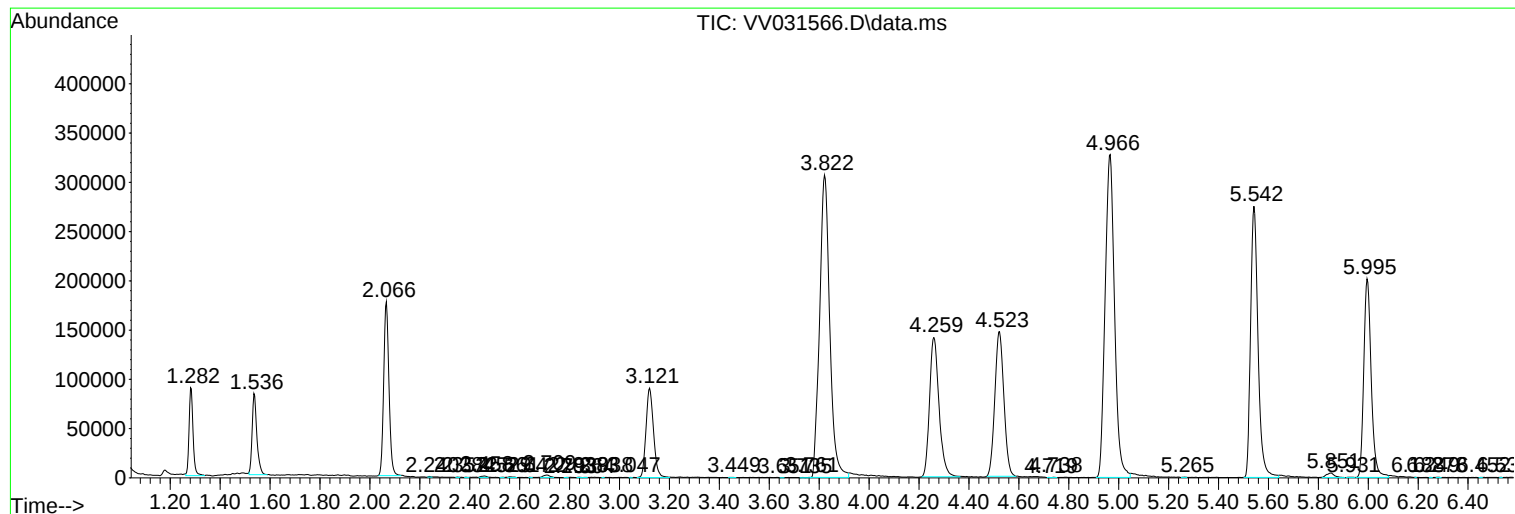

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031566.D
Acq On : 16 Jun 2023 11:18
Operator : SY/MD
Sample : 03254-03DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031566.D
Acq On : 16 Jun 2023 11:18
Operator : SY/MD
Sample : 03254-03DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------