

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031567.D
 Acq On : 16 Jun 2023 11:41
 Operator : SY/MD
 Sample : 03254-12DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	95	rVB	80818	89891	10.63%	1.305%
2	1.555	148	160	176	rVB2	159737	276510	32.70%	4.015%
3	2.066	309	319	334	rBV	169131	246086	29.10%	3.573%
4	2.320	395	398	401	rBV	433	247	0.03%	0.004%
5	2.458	434	441	451	rVB5	2149	4084	0.48%	0.059%
6	2.561	466	473	478	rBV2	766	887	0.10%	0.013%
7	2.655	498	502	503	rBV	306	156	0.02%	0.002%
8	2.706	511	518	531	rVB4	1849	2969	0.35%	0.043%
9	2.851	559	563	567	rBV2	309	286	0.03%	0.004%
10	2.870	567	569	573	rVB2	340	228	0.03%	0.003%
11	2.899	573	578	580	rBV	221	210	0.02%	0.003%
12	2.912	580	582	585	rBV2	207	168	0.02%	0.002%
13	2.986	600	605	609	rBV2	357	433	0.05%	0.006%
14	3.066	629	630	632	rBV2	133	57	0.01%	0.001%
15	3.121	634	647	663	rBV	14576	30091	3.56%	0.437%
16	3.381	722	728	733	rBV2	266	283	0.03%	0.004%
17	3.407	733	736	740	rBV	220	224	0.03%	0.003%
18	3.494	761	763	766	rVB	285	108	0.01%	0.002%
19	3.597	793	795	799	rVB	339	193	0.02%	0.003%
20	3.616	799	801	803	rBV	183	111	0.01%	0.002%
21	3.699	824	827	829	rBV2	142	66	0.01%	0.001%
22	3.716	829	832	833	rBV2	173	125	0.01%	0.002%
23	3.802	848	859	886	rBV	61330	175737	20.78%	2.552%
24	4.259	984	1001	1032	rBV2	142104	375110	44.36%	5.446%
25	4.597	1104	1106	1109	rBB2	332	141	0.02%	0.002%
26	4.645	1118	1121	1122	rBV	167	75	0.01%	0.001%
27	4.728	1142	1147	1150	rBV	184	209	0.02%	0.003%
28	4.770	1156	1160	1165	rBV3	348	336	0.04%	0.005%
29	4.876	1189	1193	1196	rBV2	184	178	0.02%	0.003%
30	4.899	1197	1200	1203	rBV	306	184	0.02%	0.003%
31	4.963	1203	1220	1246	rBV2	315672	845656	100.00%	12.278%
32	5.413	1358	1360	1361	rBV2	202	67	0.01%	0.001%
33	5.442	1366	1369	1371	rBV2	161	90	0.01%	0.001%
34	5.455	1371	1373	1375	rBV2	210	97	0.01%	0.001%
35	5.490	1381	1384	1386	rBV	290	183	0.02%	0.003%
36	5.542	1387	1400	1429	rBV	281656	573773	67.85%	8.331%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031567.D
 Acq On : 16 Jun 2023 11:41
 Operator : SY/MD
 Sample : 03254-12DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.825	1484	1488	1489	rBV3	988	626	0.07%	0.009%
38	5.886	1505	1507	1512	rVB	179	130	0.02%	0.002%
39	5.921	1512	1518	1520	rBV2	247	279	0.03%	0.004%
40	5.995	1528	1541	1568	rBV	197584	409191	48.39%	5.941%
41	6.297	1632	1635	1639	rBV3	299	218	0.03%	0.003%
42	6.384	1660	1662	1665	rBV2	151	106	0.01%	0.002%
43	6.426	1673	1675	1676	rBV	67	34	0.00%	0.000%
44	6.439	1676	1679	1682	rVV	265	155	0.02%	0.002%
45	6.558	1715	1716	1717	rBV	208	63	0.01%	0.001%
46	6.571	1717	1720	1722	rVV2	234	182	0.02%	0.003%
47	6.661	1745	1748	1750	rBV2	194	132	0.02%	0.002%
48	6.918	1816	1828	1847	rBV	95407	180591	21.36%	2.622%
49	7.182	1905	1910	1918	rBV4	465	735	0.09%	0.011%
50	7.249	1918	1931	1955	rBV	346609	612076	72.38%	8.887%
51	7.558	2017	2027	2057	rBV	74296	133058	15.73%	1.932%
52	7.744	2081	2085	2088	rBV3	367	253	0.03%	0.004%
53	8.031	2165	2174	2209	rBV	204892	380263	44.97%	5.521%
54	8.407	2288	2291	2295	rVB3	229	191	0.02%	0.003%
55	8.429	2295	2298	2299	rBV	254	180	0.02%	0.003%
56	8.577	2343	2344	2345	rVB	115	22	0.00%	0.000%
57	8.719	2386	2388	2392	rBV	138	132	0.02%	0.002%
58	8.789	2399	2410	2442	rBV	427049	706298	83.52%	10.255%
59	8.957	2456	2462	2470	rBV5	3760	5159	0.61%	0.075%
60	9.024	2477	2483	2485	rBV3	396	427	0.05%	0.006%
61	9.130	2514	2516	2519	rBV2	294	136	0.02%	0.002%
62	9.178	2528	2531	2534	rBV	254	123	0.01%	0.002%
63	9.458	2615	2618	2621	rBV	176	94	0.01%	0.001%
64	9.493	2623	2629	2635	rVB3	650	859	0.10%	0.012%
65	9.522	2636	2638	2640	rVB2	283	113	0.01%	0.002%
66	9.686	2686	2689	2693	rBV2	156	145	0.02%	0.002%
67	9.969	2775	2777	2778	rBV	150	69	0.01%	0.001%
68	10.069	2806	2808	2809	rBV	165	48	0.01%	0.001%
69	10.159	2824	2836	2858	rBV	302128	473842	56.03%	6.880%
70	10.397	2902	2910	2921	rBV4	1841	2723	0.32%	0.040%
71	10.448	2924	2926	2928	rBV	202	126	0.01%	0.002%
72	10.526	2947	2950	2952	rBV	202	86	0.01%	0.001%
73	10.600	2972	2973	2975	rBV	217	125	0.01%	0.002%
74	10.680	2991	2998	3012	rBV4	3740	5489	0.65%	0.080%
75	10.860	3048	3054	3062	rBV2	3244	4227	0.50%	0.061%
76	10.969	3083	3088	3093	rBV	413	440	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031567.D
 Acq On : 16 Jun 2023 11:41
 Operator : SY/MD
 Sample : 03254-12DL 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYX3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.030	3105	3107	3112	rBV2	184	161	0.02%	0.002%
78	11.191	3146	3157	3179	rBV	444367	676435	79.99%	9.821%
79	11.355	3206	3208	3210	rBV2	260	122	0.01%	0.002%
80	11.477	3239	3246	3253	rVB6	1986	2750	0.33%	0.040%
81	11.567	3262	3274	3299	rBV	421792	657602	77.76%	9.548%
82	11.825	3351	3354	3355	rBV	311	150	0.02%	0.002%
83	11.873	3363	3369	3374	rVB5	1218	1635	0.19%	0.024%
84	11.927	3382	3386	3392	rVB2	530	578	0.07%	0.008%
85	11.956	3392	3395	3397	rBV3	375	284	0.03%	0.004%
86	12.037	3418	3420	3423	rBV2	260	200	0.02%	0.003%
87	12.133	3448	3450	3452	rBV	222	107	0.01%	0.002%
88	12.358	3518	3520	3525	rBV3	368	286	0.03%	0.004%
89	12.702	3622	3627	3631	rBV2	394	549	0.06%	0.008%
90	12.950	3701	3704	3707	rBV	244	143	0.02%	0.002%
91	13.053	3734	3736	3737	rBV	238	85	0.01%	0.001%
92	13.278	3804	3806	3807	rBV	220	84	0.01%	0.001%
93	13.513	3876	3879	3881	rBV	316	196	0.02%	0.003%
94	13.770	3956	3959	3960	rBV	313	195	0.02%	0.003%
95	13.841	3977	3981	3986	rBV2	439	509	0.06%	0.007%
96	13.882	3992	3994	3998	rBV2	318	164	0.02%	0.002%
97	14.278	4114	4117	4123	rBV3	437	517	0.06%	0.008%
98	14.548	4199	4201	4205	rVB	607	354	0.04%	0.005%




Sum of corrected areas: 6887501

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031567.D
Acq On : 16 Jun 2023 11:41
Operator : SY/MD
Sample : 03254-12DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

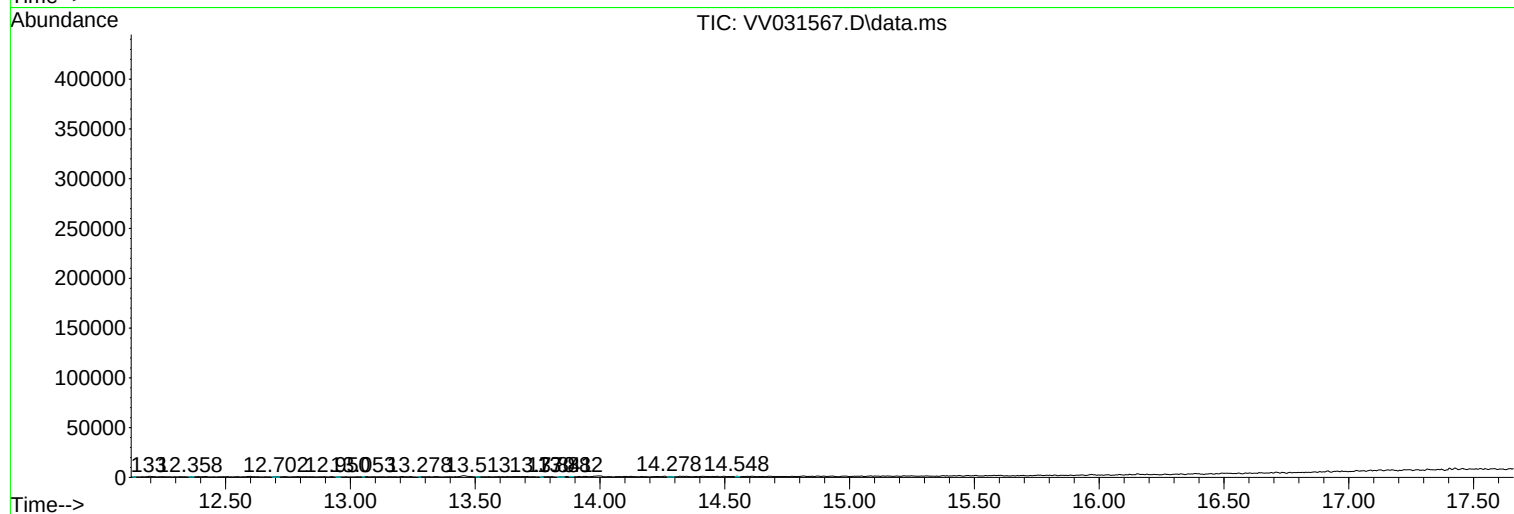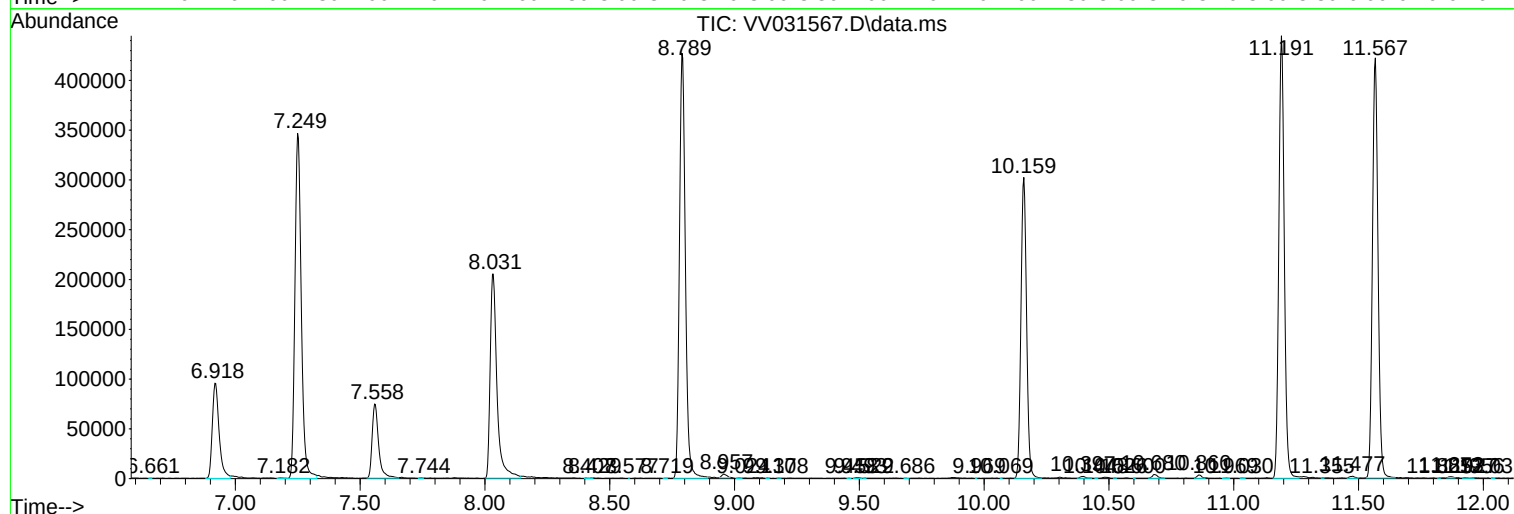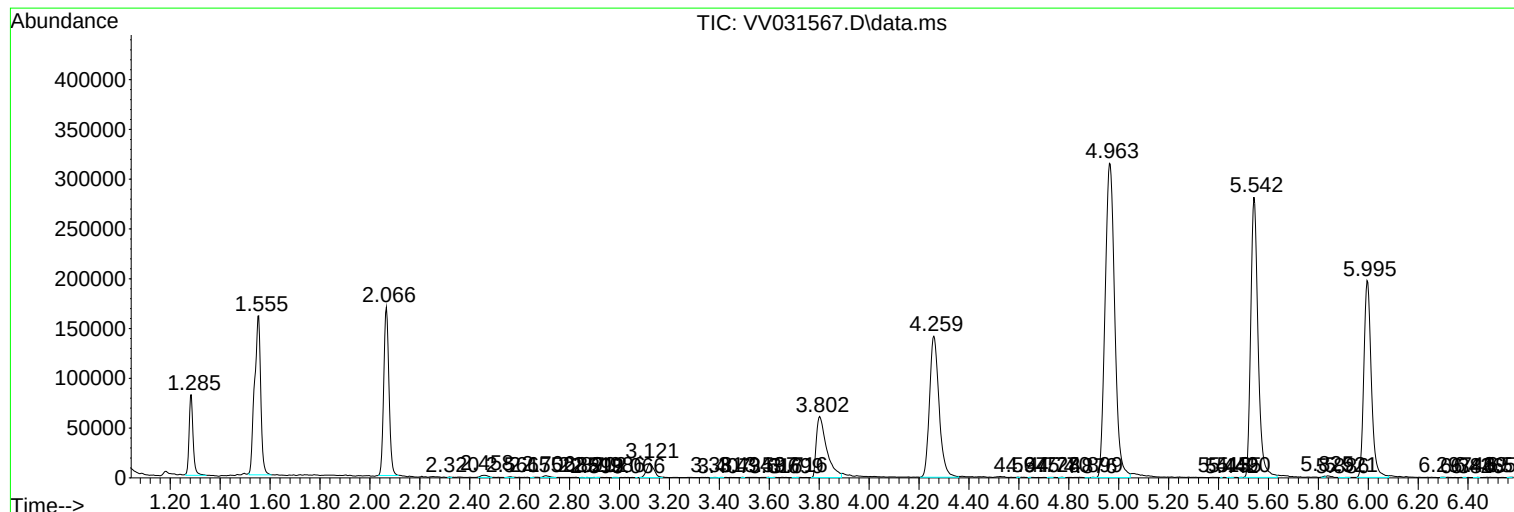

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031567.D
Acq On : 16 Jun 2023 11:41
Operator : SY/MD
Sample : 03254-12DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031567.D
Acq On : 16 Jun 2023 11:41
Operator : SY/MD
Sample : 03254-12DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------