

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031568.D
 Acq On : 16 Jun 2023 12:04
 Operator : SY/MD
 Sample : 03254-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	93	rVB	77558	84542	10.35%	1.286%
2	1.539	148	155	173	rVB	79713	97599	11.95%	1.484%
3	2.066	309	319	334	rBV	162819	234986	28.77%	3.574%
4	2.355	407	409	412	rBV	271	195	0.02%	0.003%
5	2.535	463	465	467	rBV2	163	46	0.01%	0.001%
6	2.567	473	475	477	rVB	253	80	0.01%	0.001%
7	2.635	493	496	498	rBV	305	228	0.03%	0.003%
8	2.879	570	572	576	rBV2	176	106	0.01%	0.002%
9	2.899	576	578	579	rBV2	176	77	0.01%	0.001%
10	2.944	590	592	593	rBV	231	80	0.01%	0.001%
11	2.973	599	601	603	rBV	186	119	0.01%	0.002%
12	3.047	622	624	628	rBV2	185	158	0.02%	0.002%
13	3.127	637	649	662	rVB2	3825	7569	0.93%	0.115%
14	3.172	662	663	664	rBV2	111	28	0.00%	0.000%
15	3.301	700	703	705	rBV2	164	140	0.02%	0.002%
16	3.339	712	715	721	rBV2	243	325	0.04%	0.005%
17	3.371	721	725	726	rBV	168	117	0.01%	0.002%
18	3.391	729	731	740	rBV2	285	275	0.03%	0.004%
19	3.429	740	743	747	rBV2	242	209	0.03%	0.003%
20	3.519	768	771	777	rVB2	234	182	0.02%	0.003%
21	3.551	777	781	782	rBV2	191	143	0.02%	0.002%
22	3.596	792	795	796	rBV	203	135	0.02%	0.002%
23	3.731	829	837	839	rBV2	318	383	0.05%	0.006%
24	3.802	849	859	892	rBV	59443	182654	22.37%	2.778%
25	4.259	986	1001	1031	rBV	135488	357297	43.75%	5.434%
26	4.571	1096	1098	1101	rBV3	347	188	0.02%	0.003%
27	4.603	1105	1108	1110	rBV	167	78	0.01%	0.001%
28	4.628	1115	1116	1117	rBV	156	46	0.01%	0.001%
29	4.693	1135	1136	1140	rVB2	243	111	0.01%	0.002%
30	4.783	1159	1164	1165	rBV2	349	220	0.03%	0.003%
31	4.966	1203	1221	1255	rBV2	303171	816658	100.00%	12.421%
32	5.481	1378	1381	1386	rBV2	268	230	0.03%	0.003%
33	5.542	1387	1400	1425	rBV	278194	575127	70.42%	8.748%
34	5.825	1484	1488	1489	rBV2	981	695	0.09%	0.011%
35	5.995	1528	1541	1568	rBV	190927	398061	48.74%	6.054%
36	6.233	1614	1615	1617	rBV	197	68	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031568.D
 Acq On : 16 Jun 2023 12:04
 Operator : SY/MD
 Sample : 03254-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.355	1649	1653	1654	rBV	306	165	0.02%	0.003%
38	6.455	1682	1684	1686	rVB	244	86	0.01%	0.001%
39	6.471	1686	1689	1691	rBV	97	69	0.01%	0.001%
40	6.625	1734	1737	1738	rBV	123	56	0.01%	0.001%
41	6.683	1753	1755	1759	rBV2	224	123	0.02%	0.002%
42	6.853	1805	1808	1809	rBV2	169	91	0.01%	0.001%
43	6.918	1817	1828	1856	rBV	93429	178673	21.88%	2.718%
44	7.114	1886	1889	1890	rBV2	221	127	0.02%	0.002%
45	7.249	1920	1931	1952	rBV	327915	576665	70.61%	8.771%
46	7.554	2014	2026	2058	rBV2	91054	182910	22.40%	2.782%
47	7.882	2120	2128	2136	rBV2	3869	5955	0.73%	0.091%
48	7.992	2158	2162	2164	rVB2	305	235	0.03%	0.004%
49	8.030	2164	2174	2202	rBV	199771	367615	45.01%	5.591%
50	8.686	2375	2378	2381	rBV2	300	213	0.03%	0.003%
51	8.792	2394	2411	2437	rBV	430122	714930	87.54%	10.874%
52	8.959	2459	2463	2468	rVB4	671	647	0.08%	0.010%
53	9.066	2493	2496	2498	rBV2	228	146	0.02%	0.002%
54	9.175	2527	2530	2533	rBV2	282	208	0.03%	0.003%
55	9.329	2576	2578	2580	rBV2	180	120	0.01%	0.002%
56	9.603	2662	2663	2665	rVB	235	60	0.01%	0.001%
57	9.760	2709	2712	2715	rBV2	362	248	0.03%	0.004%
58	9.828	2730	2733	2740	rVB2	337	244	0.03%	0.004%
59	10.159	2825	2836	2853	rBV	292612	457898	56.07%	6.965%
60	10.332	2881	2890	2899	rBV2	5111	6742	0.83%	0.103%
61	10.397	2908	2910	2912	rBV	228	101	0.01%	0.002%
62	10.410	2912	2914	2920	rVB2	321	225	0.03%	0.003%
63	10.512	2942	2946	2948	rBV2	202	146	0.02%	0.002%
64	10.615	2974	2978	2983	rBV	366	291	0.04%	0.004%
65	10.834	3042	3046	3049	rBV3	304	307	0.04%	0.005%
66	10.853	3049	3052	3054	rBV2	329	258	0.03%	0.004%
67	10.921	3071	3073	3074	rBV	156	50	0.01%	0.001%
68	10.985	3089	3093	3097	rBV	310	206	0.03%	0.003%
69	11.127	3134	3137	3146	rVB3	513	479	0.06%	0.007%
70	11.191	3146	3157	3180	rBV	449468	688136	84.26%	10.466%
71	11.352	3205	3207	3209	rBV2	276	154	0.02%	0.002%
72	11.384	3215	3217	3220	rVB2	379	181	0.02%	0.003%
73	11.426	3226	3230	3231	rBV	238	174	0.02%	0.003%
74	11.500	3251	3253	3256	rBV2	319	135	0.02%	0.002%
75	11.567	3262	3274	3292	rBV	401068	626144	76.67%	9.524%
76	11.795	3341	3345	3347	rBV3	324	329	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031568.D
 Acq On : 16 Jun 2023 12:04
 Operator : SY/MD
 Sample : 03254-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

77	11.856	3362	3364	3365	rBV3	232	102	0.01%	0.002%
78	12.088	3429	3436	3438	rBV	285	344	0.04%	0.005%
79	12.384	3526	3528	3531	rVB2	376	175	0.02%	0.003%
80	12.615	3596	3600	3605	rBV3	394	393	0.05%	0.006%
81	12.834	3666	3668	3671	rBV	299	141	0.02%	0.002%
82	13.422	3846	3851	3853	rBV	372	300	0.04%	0.005%
83	13.458	3855	3862	3871	rVB4	1272	1958	0.24%	0.030%
84	13.975	4017	4023	4024	rBV2	564	541	0.07%	0.008%
85	14.152	4076	4078	4079	rBV	225	70	0.01%	0.001%




Sum of corrected areas: 6574721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031568.D
Acq On : 16 Jun 2023 12:04
Operator : SY/MD
Sample : 03254-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

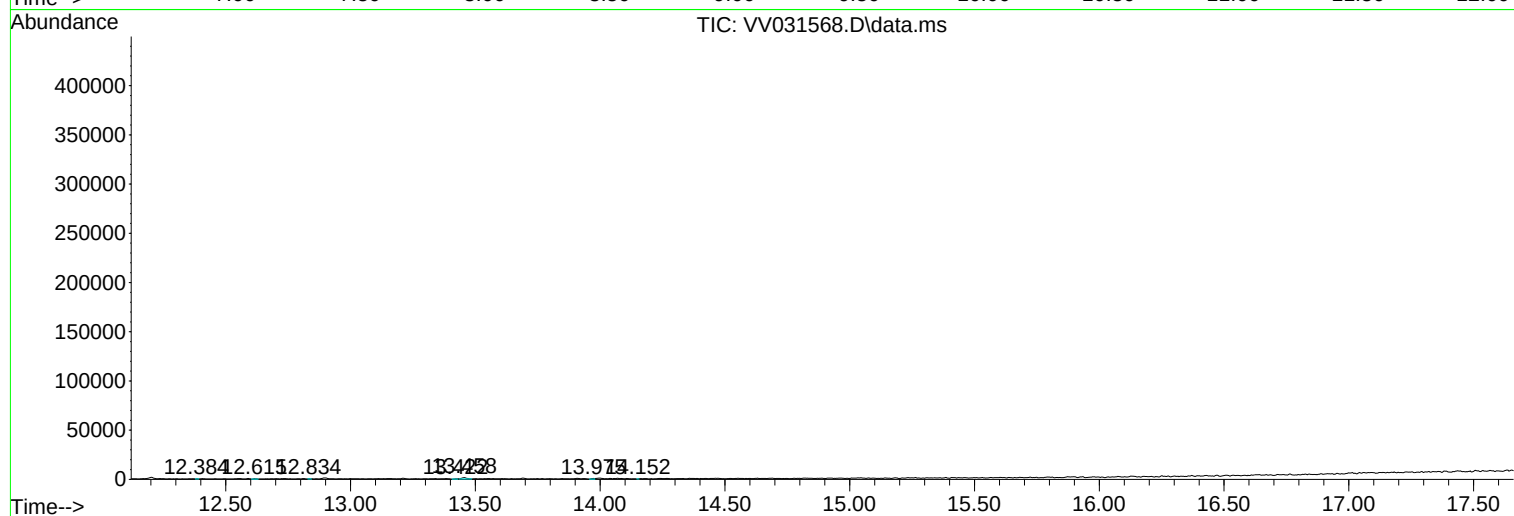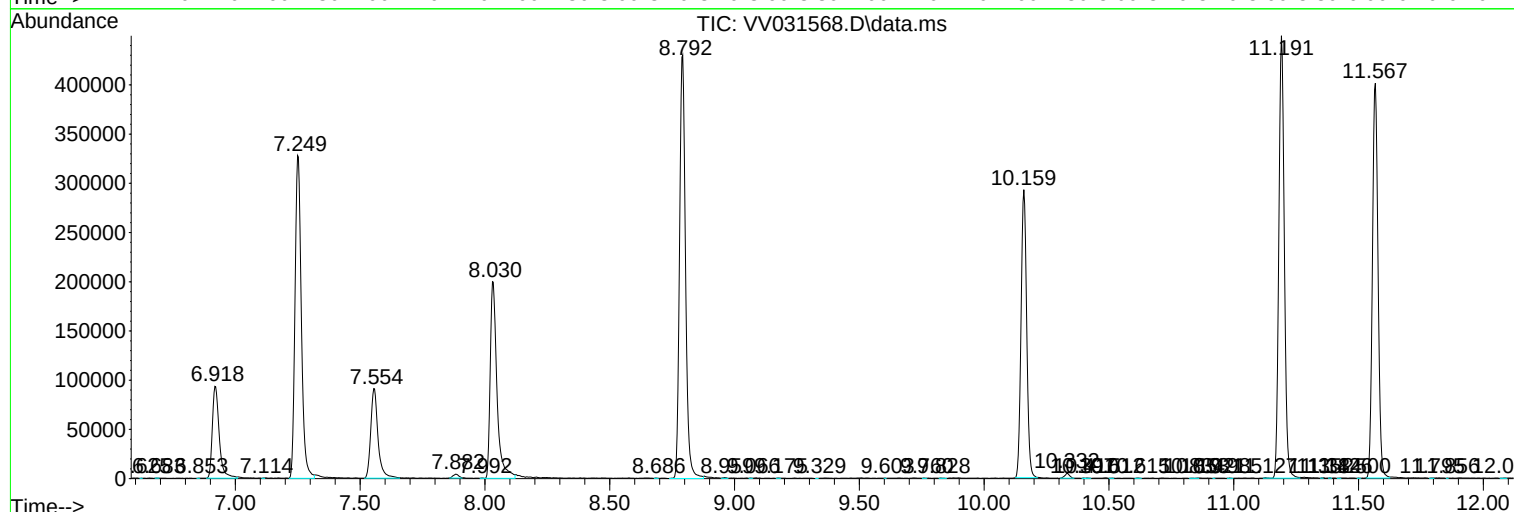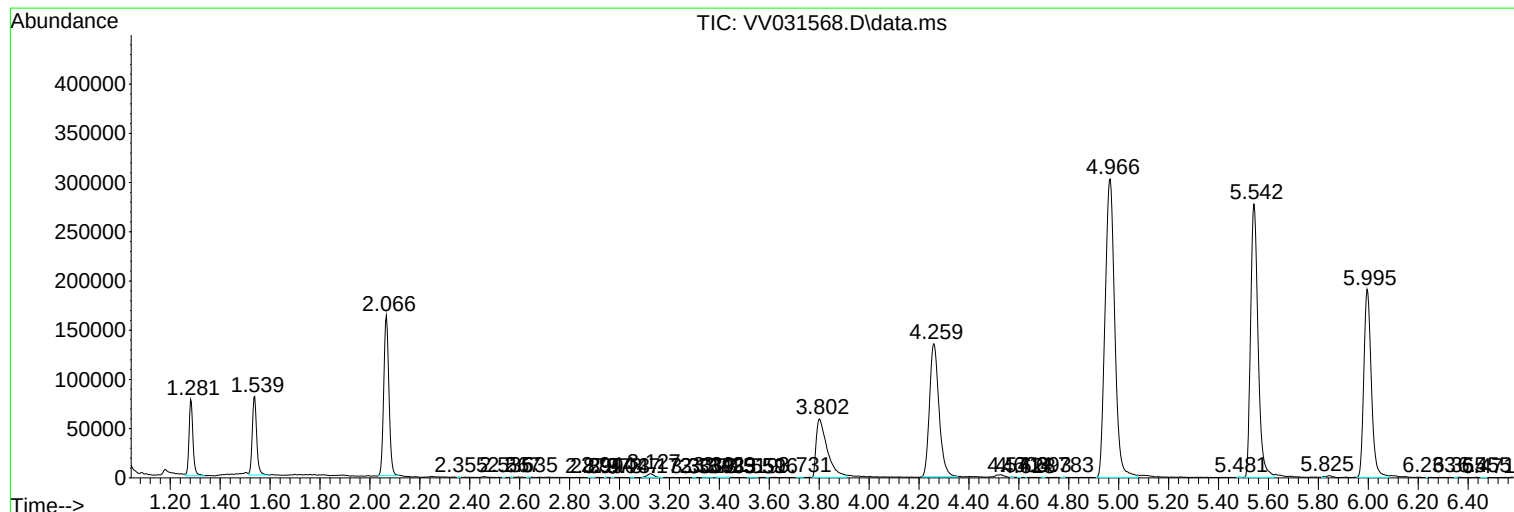

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031568.D
Acq On : 16 Jun 2023 12:04
Operator : SY/MD
Sample : 03254-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031568.D
Acq On : 16 Jun 2023 12:04
Operator : SY/MD
Sample : 03254-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------