

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031569.D
 Acq On : 16 Jun 2023 12:28
 Operator : SY/MD
 Sample : 03254-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	96	rVB	83584	93287	11.62%	1.355%
2	1.539	148	155	167	rVB	76233	92117	11.48%	1.338%
3	2.066	309	319	336	rBV	159357	233222	29.06%	3.387%
4	2.355	407	409	412	rBV	333	232	0.03%	0.003%
5	2.535	463	465	468	rBV	192	88	0.01%	0.001%
6	2.658	499	503	505	rBV2	354	208	0.03%	0.003%
7	2.706	509	518	530	rVV2	4028	7577	0.94%	0.110%
8	2.786	541	543	549	rVB3	306	151	0.02%	0.002%
9	2.857	563	565	566	rBV3	173	77	0.01%	0.001%
10	2.895	573	577	579	rBV2	283	270	0.03%	0.004%
11	2.986	603	605	608	rBV2	219	127	0.02%	0.002%
12	3.121	633	647	669	rBV	67583	142380	17.74%	2.068%
13	3.256	688	689	691	rBV2	204	93	0.01%	0.001%
14	3.294	696	701	703	rBV2	596	474	0.06%	0.007%
15	3.397	729	733	736	rBV	238	240	0.03%	0.003%
16	3.510	758	768	771	rBV	351	513	0.06%	0.007%
17	3.542	775	778	783	rBV2	318	256	0.03%	0.004%
18	3.577	786	789	792	rBV	311	248	0.03%	0.004%
19	3.616	798	801	802	rBV	208	147	0.02%	0.002%
20	3.712	828	831	835	rVB	248	169	0.02%	0.002%
21	3.738	835	839	842	rBV2	248	259	0.03%	0.004%
22	3.822	848	865	893	rBV4	110666	360618	44.93%	5.237%
23	4.259	986	1001	1026	rBV	134212	350497	43.67%	5.090%
24	4.526	1071	1084	1102	rVB3	27398	68987	8.60%	1.002%
25	4.616	1109	1112	1115	rVB	320	159	0.02%	0.002%
26	4.635	1115	1118	1121	rBV	300	153	0.02%	0.002%
27	4.773	1159	1161	1162	rVB	201	57	0.01%	0.001%
28	4.966	1204	1221	1246	rBV2	299997	802610	100.00%	11.655%
29	5.336	1333	1336	1341	rBV3	356	322	0.04%	0.005%
30	5.410	1357	1359	1363	rBV	279	202	0.03%	0.003%
31	5.542	1384	1400	1428	rBV	283183	582753	72.61%	8.462%
32	5.844	1483	1494	1509	rBV5	8472	18813	2.34%	0.273%
33	5.924	1517	1519	1522	rVB	250	75	0.01%	0.001%
34	5.995	1528	1541	1565	rBV	188402	388548	48.41%	5.642%
35	6.246	1616	1619	1622	rBV3	326	207	0.03%	0.003%
36	6.355	1652	1653	1656	rBV	296	158	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031569.D
 Acq On : 16 Jun 2023 12:28
 Operator : SY/MD
 Sample : 03254-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.394	1663	1665	1668	rVB2	223	104	0.01%	0.002%
38	6.860	1808	1810	1811	rBV	126	49	0.01%	0.001%
39	6.918	1818	1828	1850	rBV	91353	170416	21.23%	2.475%
40	7.127	1891	1893	1894	rBV	285	112	0.01%	0.002%
41	7.249	1920	1931	1957	rBV	318691	565579	70.47%	8.213%
42	7.558	2018	2027	2052	rBV	68504	122646	15.28%	1.781%
43	7.882	2119	2128	2130	rBV2	4912	5894	0.73%	0.086%
44	8.034	2165	2175	2207	rBV	200734	370388	46.15%	5.379%
45	8.551	2333	2336	2339	rBV	326	262	0.03%	0.004%
46	8.590	2344	2348	2354	rVB2	354	428	0.05%	0.006%
47	8.625	2354	2359	2362	rBV2	413	305	0.04%	0.004%
48	8.664	2369	2371	2374	rVB2	365	160	0.02%	0.002%
49	8.789	2399	2410	2433	rBV	441891	720547	89.78%	10.463%
50	8.960	2461	2463	2464	rBV	424	194	0.02%	0.003%
51	9.001	2471	2476	2480	rBV2	344	367	0.05%	0.005%
52	9.037	2485	2487	2490	rBV	223	112	0.01%	0.002%
53	9.464	2614	2620	2626	rBV3	433	604	0.08%	0.009%
54	9.535	2638	2642	2645	rBV	252	211	0.03%	0.003%
55	9.615	2665	2667	2668	rBV	269	113	0.01%	0.002%
56	9.763	2710	2713	2718	rBV	221	176	0.02%	0.003%
57	9.879	2744	2749	2752	rBV2	434	425	0.05%	0.006%
58	9.982	2778	2781	2783	rBV	254	178	0.02%	0.003%
59	10.062	2803	2806	2808	rBV2	305	212	0.03%	0.003%
60	10.159	2824	2836	2855	rBV	291228	456129	56.83%	6.624%
61	10.265	2867	2869	2872	rBV	211	116	0.01%	0.002%
62	10.332	2879	2890	2903	rBV2	5185	8708	1.08%	0.126%
63	10.587	2966	2969	2974	rBV2	311	219	0.03%	0.003%
64	10.644	2981	2987	2991	rBV3	416	500	0.06%	0.007%
65	10.963	3082	3086	3088	rBV	364	358	0.04%	0.005%
66	11.091	3123	3126	3128	rBV2	384	251	0.03%	0.004%
67	11.191	3146	3157	3183	rBV	450907	692935	86.34%	10.062%
68	11.567	3261	3274	3295	rBV	398654	616817	76.85%	8.957%
69	11.905	3374	3379	3380	rBV2	331	320	0.04%	0.005%
70	12.201	3466	3471	3481	rVB5	2186	3261	0.41%	0.047%
71	12.265	3488	3491	3495	rBV2	360	293	0.04%	0.004%
72	13.406	3844	3846	3847	rBV	340	128	0.02%	0.002%
73	13.821	3970	3975	3978	rBV3	518	573	0.07%	0.008%




Sum of corrected areas: 6886384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031569.D
Acq On : 16 Jun 2023 12:28
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

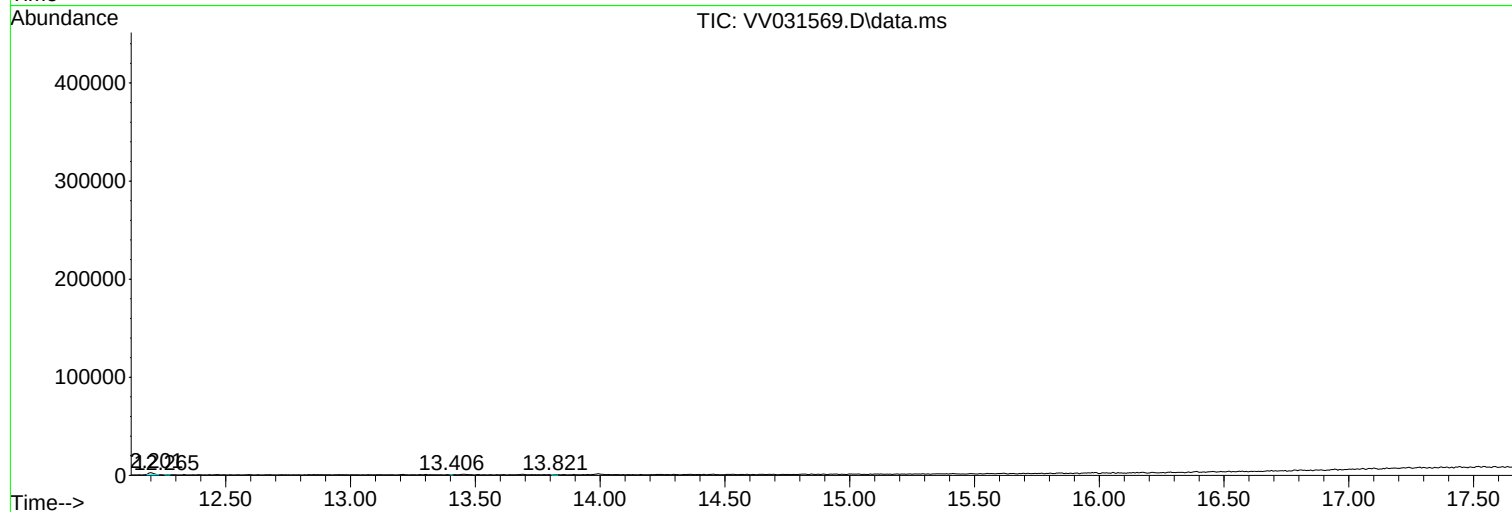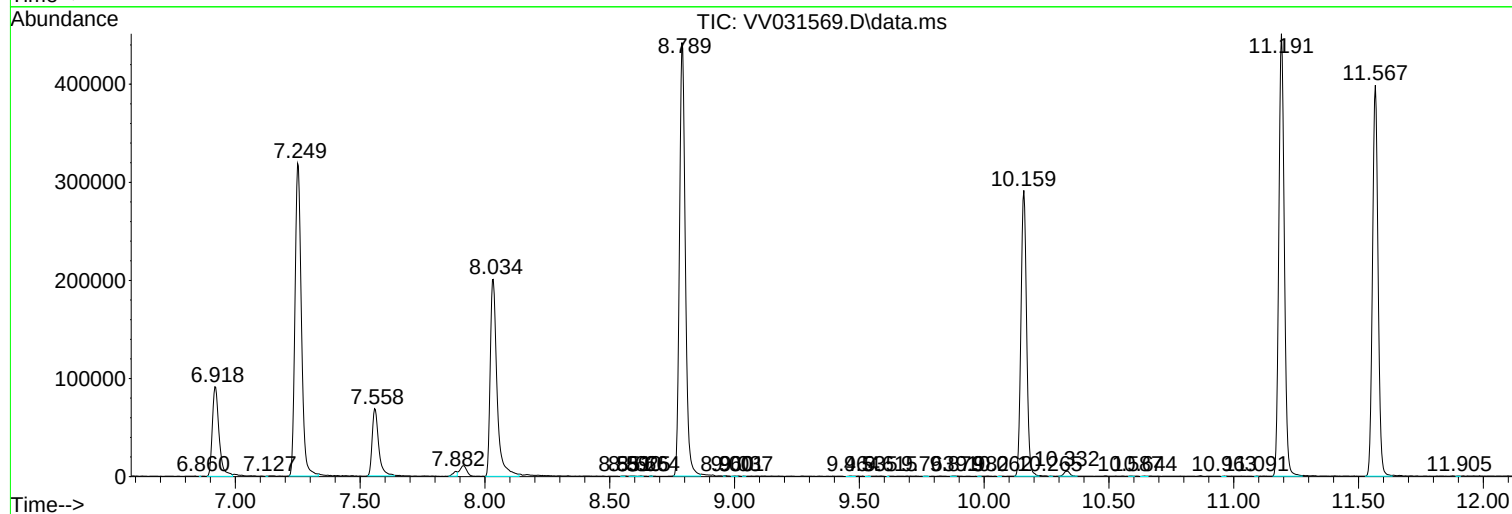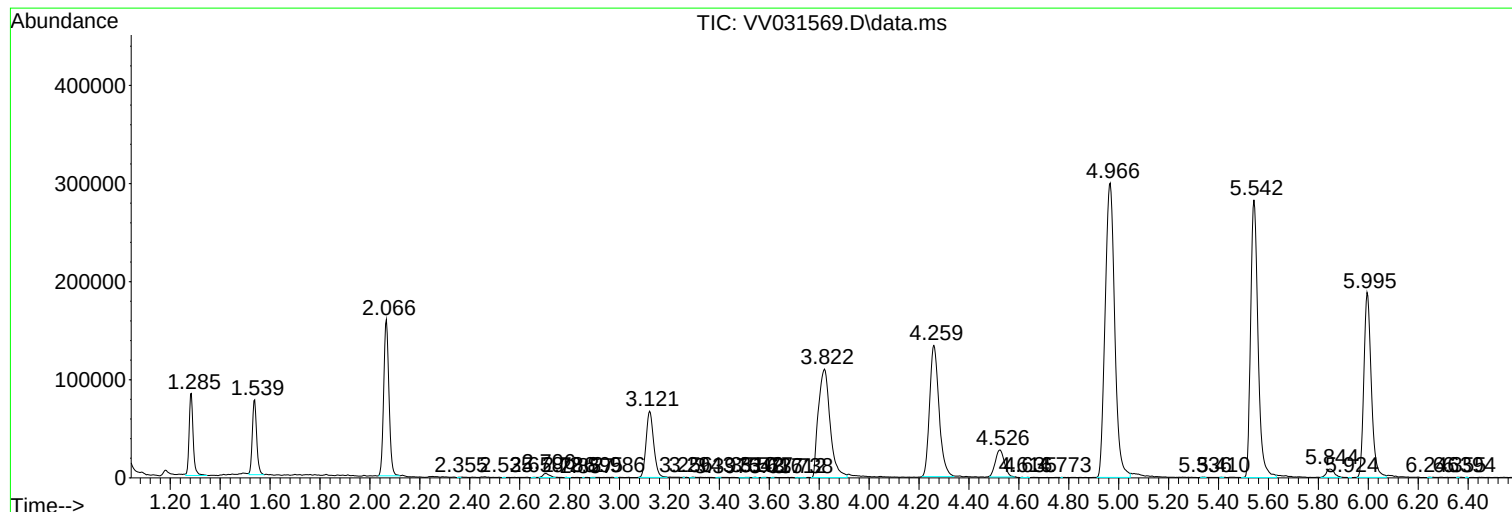

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031569.D
Acq On : 16 Jun 2023 12:28
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031569.D
Acq On : 16 Jun 2023 12:28
Operator : SY/MD
Sample : 03254-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------