

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031570.D
 Acq On : 16 Jun 2023 12:51
 Operator : SY/MD
 Sample : 03254-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	52	rBV	5786	8212	0.99%	0.104%
2	1.285	69	76	96	rVB2	105204	117909	14.24%	1.489%
3	1.539	147	155	171	rVB	78787	96242	11.62%	1.215%
4	2.066	308	319	332	rBV	164964	242286	29.26%	3.060%
5	2.240	370	373	375	rBV2	364	233	0.03%	0.003%
6	2.272	381	383	390	rBV3	476	466	0.06%	0.006%
7	2.452	434	439	440	rBV3	641	455	0.05%	0.006%
8	2.529	461	463	467	rVB2	385	226	0.03%	0.003%
9	2.706	507	518	533	rBV3	10705	19292	2.33%	0.244%
10	2.809	547	550	553	rVB2	327	236	0.03%	0.003%
11	2.899	575	578	583	rVB2	279	246	0.03%	0.003%
12	3.121	632	647	668	rBV	168200	353472	42.69%	4.464%
13	3.490	758	762	763	rBV	375	262	0.03%	0.003%
14	3.616	797	801	804	rBV3	316	278	0.03%	0.004%
15	3.822	849	865	897	rBV3	238904	689392	83.26%	8.706%
16	4.105	950	953	957	rVB2	786	577	0.07%	0.007%
17	4.127	957	960	963	rBV	426	334	0.04%	0.004%
18	4.259	984	1001	1031	rBV	138880	366624	44.28%	4.630%
19	4.523	1065	1083	1107	rBV3	81935	215079	25.97%	2.716%
20	4.883	1190	1195	1199	rBV2	365	285	0.03%	0.004%
21	4.966	1204	1221	1245	rBV2	308459	828044	100.00%	10.456%
22	5.249	1304	1309	1310	rBV2	462	320	0.04%	0.004%
23	5.342	1336	1338	1342	rVB3	341	242	0.03%	0.003%
24	5.394	1350	1354	1355	rBV2	347	221	0.03%	0.003%
25	5.542	1388	1400	1429	rBV	285722	589750	71.22%	7.447%
26	5.844	1482	1494	1516	rBV5	33192	72226	8.72%	0.912%
27	5.995	1528	1541	1569	rBV	192168	401107	48.44%	5.065%
28	6.162	1592	1593	1598	rVB2	573	315	0.04%	0.004%
29	6.285	1625	1631	1636	rVB3	406	458	0.06%	0.006%
30	6.362	1652	1655	1660	rBV3	428	439	0.05%	0.006%
31	6.400	1663	1667	1670	rBV2	283	240	0.03%	0.003%
32	6.449	1679	1682	1686	rBV	298	275	0.03%	0.003%
33	6.580	1718	1723	1724	rBV2	391	281	0.03%	0.004%
34	6.918	1815	1828	1860	rBV	94412	180954	21.85%	2.285%
35	7.249	1920	1931	1956	rBV	329615	581206	70.19%	7.339%
36	7.558	2018	2027	2053	rBV2	71335	128944	15.57%	1.628%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031570.D
 Acq On : 16 Jun 2023 12:51
 Operator : SY/MD
 Sample : 03254-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.674	2060	2063	2066	rVB3	378	245	0.03%	0.003%
38	7.747	2080	2086	2087	rBV3	387	295	0.04%	0.004%
39	7.789	2093	2099	2103	rBV5	1047	1338	0.16%	0.017%
40	7.809	2103	2105	2110	rVB2	341	219	0.03%	0.003%
41	7.915	2118	2138	2153	rBV7	40361	77545	9.36%	0.979%
42	8.030	2165	2174	2209	rBV	209369	385961	46.61%	4.874%
43	8.262	2244	2246	2252	rBV4	345	300	0.04%	0.004%
44	8.349	2271	2273	2278	rVB2	400	322	0.04%	0.004%
45	8.384	2282	2284	2287	rVV2	388	231	0.03%	0.003%
46	8.590	2344	2348	2353	rBV	265	247	0.03%	0.003%
47	8.789	2399	2410	2438	rBV	442021	726340	87.72%	9.172%
48	9.040	2483	2488	2491	rBV3	276	252	0.03%	0.003%
49	9.117	2510	2512	2518	rVB2	255	219	0.03%	0.003%
50	9.239	2545	2550	2555	rBV	190	258	0.03%	0.003%
51	9.291	2562	2566	2569	rBV2	324	310	0.04%	0.004%
52	9.805	2723	2726	2730	rVB2	310	234	0.03%	0.003%
53	9.876	2745	2748	2750	rBV2	469	353	0.04%	0.004%
54	10.008	2783	2789	2790	rBV	264	264	0.03%	0.003%
55	10.159	2824	2836	2857	rBV	298320	466042	56.28%	5.885%
56	10.333	2880	2890	2899	rVV3	6190	8979	1.08%	0.113%
57	10.564	2959	2962	2965	rBV2	258	216	0.03%	0.003%
58	10.870	3051	3057	3059	rBV2	421	549	0.07%	0.007%
59	10.921	3069	3073	3078	rBV3	264	269	0.03%	0.003%
60	10.944	3078	3080	3086	rBV	307	342	0.04%	0.004%
61	11.140	3136	3141	3144	rBV2	480	359	0.04%	0.005%
62	11.191	3146	3157	3181	rBV	454766	699978	84.53%	8.839%
63	11.474	3240	3245	3251	rVB3	324	477	0.06%	0.006%
64	11.567	3262	3274	3292	rBV	402675	630662	76.16%	7.964%
65	11.712	3316	3319	3324	rVB2	290	306	0.04%	0.004%
66	11.879	3367	3371	3373	rBV2	379	356	0.04%	0.004%
67	12.098	3435	3439	3442	rBV3	271	228	0.03%	0.003%
68	12.159	3455	3458	3461	rBV2	335	249	0.03%	0.003%
69	12.197	3461	3470	3481	rVV3	2505	4227	0.51%	0.053%
70	12.429	3539	3542	3546	rBV2	306	240	0.03%	0.003%
71	12.535	3571	3575	3578	rBV2	331	304	0.04%	0.004%
72	12.596	3592	3594	3599	rBV2	446	423	0.05%	0.005%
73	12.664	3608	3615	3618	rBV	301	337	0.04%	0.004%
74	12.808	3656	3660	3665	rBV2	330	325	0.04%	0.004%
75	13.214	3781	3786	3788	rBV2	580	562	0.07%	0.007%
76	13.300	3812	3813	3819	rVB2	348	221	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031570.D
 Acq On : 16 Jun 2023 12:51
 Operator : SY/MD
 Sample : 03254-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	13.365	3830	3833	3837	rVB3	316	248	0.03%	0.003%
78	13.451	3858	3860	3863	rBV2	303	229	0.03%	0.003%
79	13.554	3889	3892	3894	rBV	394	229	0.03%	0.003%
80	13.586	3899	3902	3909	rBV2	617	627	0.08%	0.008%
81	13.619	3909	3912	3917	rBV3	334	305	0.04%	0.004%
82	13.699	3930	3937	3940	rBV3	398	480	0.06%	0.006%
83	13.943	4008	4013	4018	rBV2	417	535	0.06%	0.007%
84	13.988	4018	4027	4038	rBV4	933	1971	0.24%	0.025%
85	14.066	4043	4051	4052	rBV2	509	535	0.06%	0.007%
86	14.252	4106	4109	4115	rBV	419	387	0.05%	0.005%
87	14.323	4129	4131	4135	rVB2	696	374	0.05%	0.005%
88	14.352	4135	4140	4143	rBV2	361	322	0.04%	0.004%
89	14.377	4143	4148	4151	rBV3	555	518	0.06%	0.007%
90	14.551	4197	4202	4203	rBV3	561	477	0.06%	0.006%
91	14.577	4207	4210	4214	rVV3	453	413	0.05%	0.005%
92	14.638	4226	4229	4231	rBV3	538	332	0.04%	0.004%
93	14.992	4335	4339	4343	rBV3	532	512	0.06%	0.006%
94	15.027	4348	4350	4353	rBV3	440	277	0.03%	0.003%
95	15.104	4368	4374	4377	rBV3	514	589	0.07%	0.007%
96	15.188	4396	4400	4403	rBV4	445	403	0.05%	0.005%
97	15.262	4420	4423	4428	rBV5	806	520	0.06%	0.007%
98	15.432	4474	4476	4481	rBV4	591	317	0.04%	0.004%
99	15.541	4507	4510	4512	rBV2	752	420	0.05%	0.005%
100	15.869	4610	4612	4613	rBV2	669	263	0.03%	0.003%




Sum of corrected areas: 7918995

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031570.D
Acq On : 16 Jun 2023 12:51
Operator : SY/MD
Sample : 03254-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

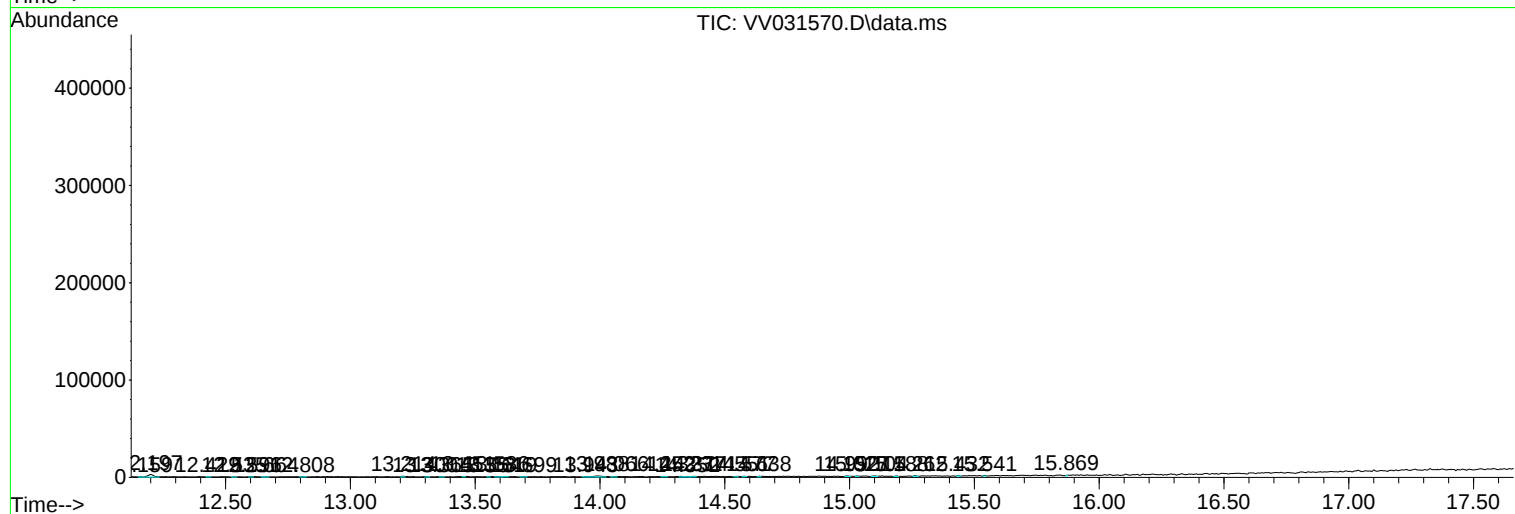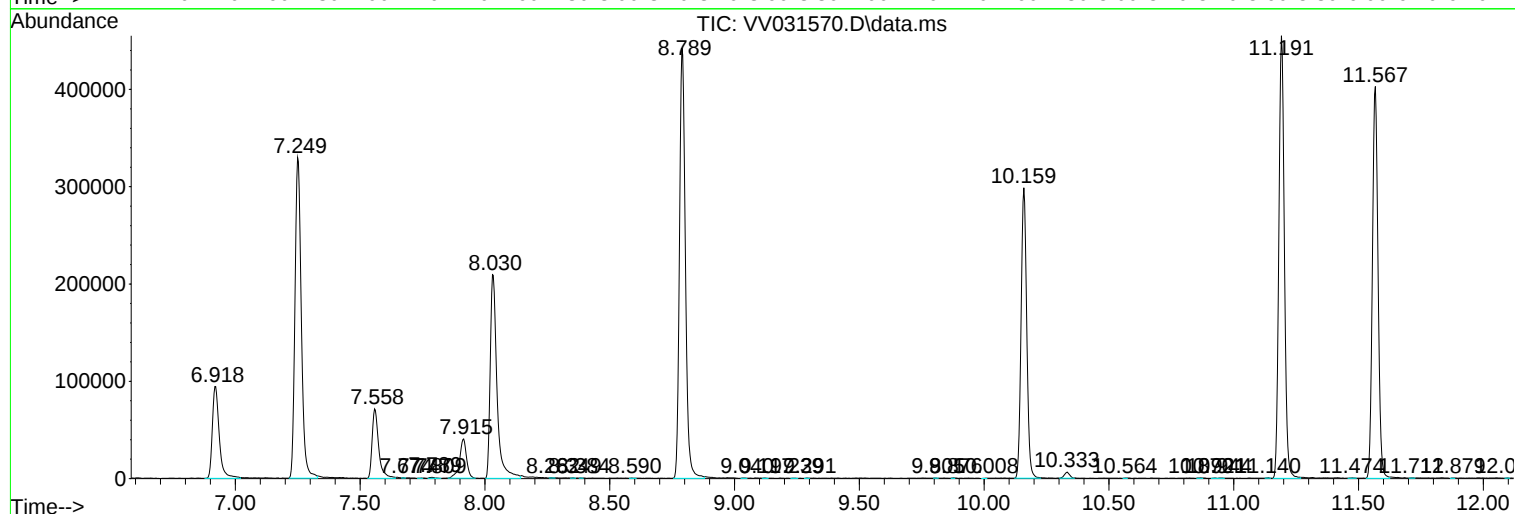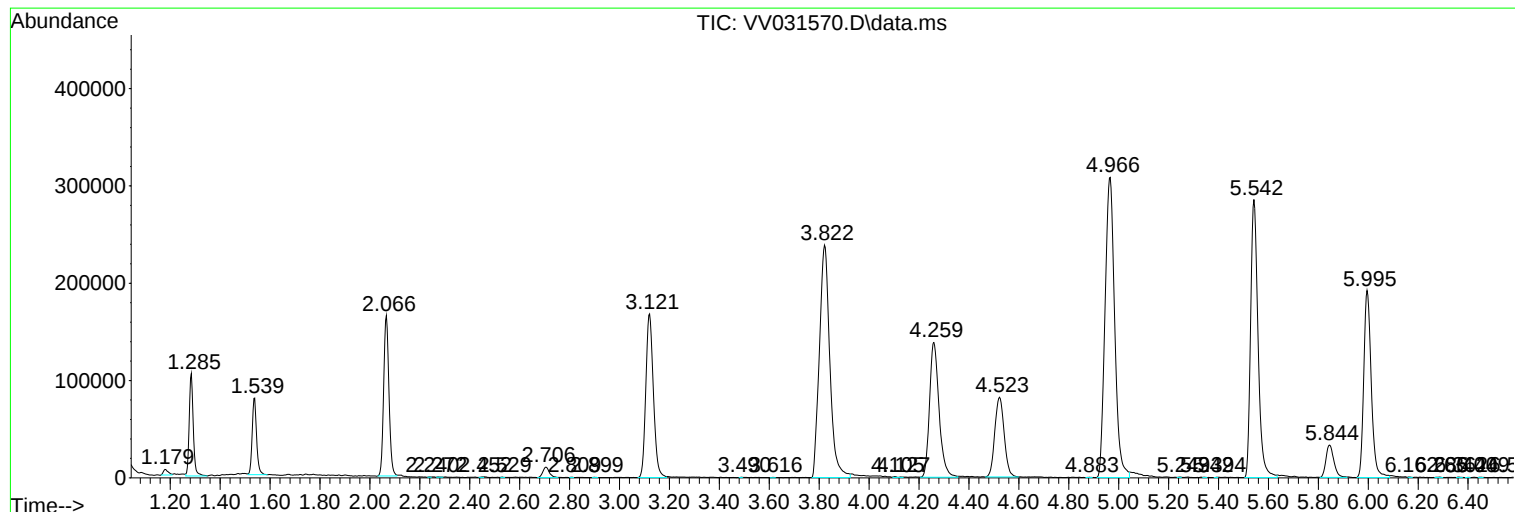

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031570.D
Acq On : 16 Jun 2023 12:51
Operator : SY/MD
Sample : 03254-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031570.D
Acq On : 16 Jun 2023 12:51
Operator : SY/MD
Sample : 03254-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------