

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031571.D
 Acq On : 16 Jun 2023 13:14
 Operator : SY/MD
 Sample : 03254-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	70892	73486	9.03%	1.185%
2	1.539	148	155	170	rVB	75990	93030	11.43%	1.500%
3	2.066	309	319	334	rBV	149165	217286	26.70%	3.504%
4	2.336	401	403	406	rBV2	259	179	0.02%	0.003%
5	2.455	434	440	448	rBV4	1138	1850	0.23%	0.030%
6	2.519	458	460	462	rBV	318	126	0.02%	0.002%
7	2.593	481	483	487	rVB	203	103	0.01%	0.002%
8	2.651	498	501	504	rBV	276	221	0.03%	0.004%
9	2.761	531	535	537	rBV	403	300	0.04%	0.005%
10	2.802	544	548	550	rBV2	127	115	0.01%	0.002%
11	2.870	566	569	573	rBV2	289	238	0.03%	0.004%
12	2.979	599	603	605	rBV	232	163	0.02%	0.003%
13	3.008	609	612	614	rBV	210	159	0.02%	0.003%
14	3.031	618	619	622	rBV2	237	152	0.02%	0.002%
15	3.056	626	627	629	rBV	106	56	0.01%	0.001%
16	3.072	630	632	636	rBV2	225	127	0.02%	0.002%
17	3.114	643	645	648	rVB2	367	218	0.03%	0.004%
18	3.137	650	652	654	rBV	165	102	0.01%	0.002%
19	3.204	671	673	676	rBV	174	85	0.01%	0.001%
20	3.378	724	727	729	rBV	251	169	0.02%	0.003%
21	3.484	756	760	762	rBV	118	91	0.01%	0.001%
22	3.507	762	767	770	rBV	261	317	0.04%	0.005%
23	3.568	782	786	787	rBV	142	95	0.01%	0.002%
24	3.619	798	802	804	rBV2	219	199	0.02%	0.003%
25	3.799	848	858	887	rBV2	63047	177256	21.78%	2.858%
26	4.259	985	1001	1031	rBV2	136683	361886	44.47%	5.835%
27	4.648	1119	1122	1124	rBV	180	90	0.01%	0.001%
28	4.674	1128	1130	1132	rVB	143	33	0.00%	0.001%
29	4.709	1139	1141	1142	rBV	144	68	0.01%	0.001%
30	4.838	1180	1181	1184	rBV	215	82	0.01%	0.001%
31	4.966	1204	1221	1249	rBV2	302811	813780	100.00%	13.122%
32	5.310	1323	1328	1333	rBV2	402	540	0.07%	0.009%
33	5.404	1355	1357	1360	rBV	256	80	0.01%	0.001%
34	5.542	1388	1400	1430	rBV	243093	509342	62.59%	8.213%
35	5.828	1485	1489	1490	rBV	972	702	0.09%	0.011%
36	5.995	1527	1541	1567	rBV2	192171	402921	49.51%	6.497%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031571.D
 Acq On : 16 Jun 2023 13:14
 Operator : SY/MD
 Sample : 03254-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.178	1596	1598	1600	rVB2	396	137	0.02%	0.002%
38	6.333	1644	1646	1652	rVB2	354	263	0.03%	0.004%
39	6.359	1652	1654	1655	rBV2	168	74	0.01%	0.001%
40	6.378	1658	1660	1662	rBV2	294	141	0.02%	0.002%
41	6.918	1818	1828	1858	rBV	93224	177570	21.82%	2.863%
42	7.143	1895	1898	1899	rBV	444	222	0.03%	0.004%
43	7.211	1916	1919	1920	rBV	237	134	0.02%	0.002%
44	7.249	1920	1931	1959	rVV	314317	559174	68.71%	9.016%
45	7.558	2018	2027	2047	rBV	72293	127709	15.69%	2.059%
46	7.937	2143	2145	2148	rBV2	322	203	0.02%	0.003%
47	8.030	2164	2174	2212	rBV	212552	396950	48.78%	6.401%
48	8.545	2331	2334	2342	rVB2	332	341	0.04%	0.005%
49	8.593	2347	2349	2353	rVB	375	191	0.02%	0.003%
50	8.616	2353	2356	2360	rBV3	317	255	0.03%	0.004%
51	8.641	2362	2364	2366	rVB2	370	158	0.02%	0.003%
52	8.693	2377	2380	2386	rBV	255	191	0.02%	0.003%
53	8.741	2391	2395	2397	rBV	193	180	0.02%	0.003%
54	8.789	2399	2410	2437	rBV	380767	625689	76.89%	10.089%
55	9.059	2493	2494	2495	rBV	112	30	0.00%	0.000%
56	9.149	2518	2522	2525	rBV2	294	304	0.04%	0.005%
57	9.326	2571	2577	2578	rBV	234	214	0.03%	0.003%
58	9.783	2717	2719	2721	rBV	231	127	0.02%	0.002%
59	9.866	2743	2745	2746	rBV	429	182	0.02%	0.003%
60	10.159	2824	2836	2854	rBV	308780	480118	59.00%	7.742%
61	10.487	2936	2938	2941	rBV	375	220	0.03%	0.004%
62	10.535	2949	2953	2955	rBV	183	173	0.02%	0.003%
63	10.651	2985	2989	2992	rBV2	322	269	0.03%	0.004%
64	10.731	3012	3014	3018	rBV	204	116	0.01%	0.002%
65	10.870	3053	3057	3062	rBV4	510	587	0.07%	0.009%
66	10.915	3068	3071	3072	rBV2	261	140	0.02%	0.002%
67	10.953	3079	3083	3088	rBV2	268	276	0.03%	0.004%
68	11.191	3145	3157	3185	rBV	380364	576818	70.88%	9.301%
69	11.567	3262	3274	3294	rBV	373262	596198	73.26%	9.613%
70	11.709	3316	3318	3320	rBV2	361	232	0.03%	0.004%
71	12.783	3649	3652	3653	rBV	327	161	0.02%	0.003%
72	12.963	3704	3708	3709	rBV	273	204	0.03%	0.003%
73	13.313	3815	3817	3820	rBV	297	153	0.02%	0.002%




Sum of corrected areas: 6201751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031571.D
Acq On : 16 Jun 2023 13:14
Operator : SY/MD
Sample : 03254-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

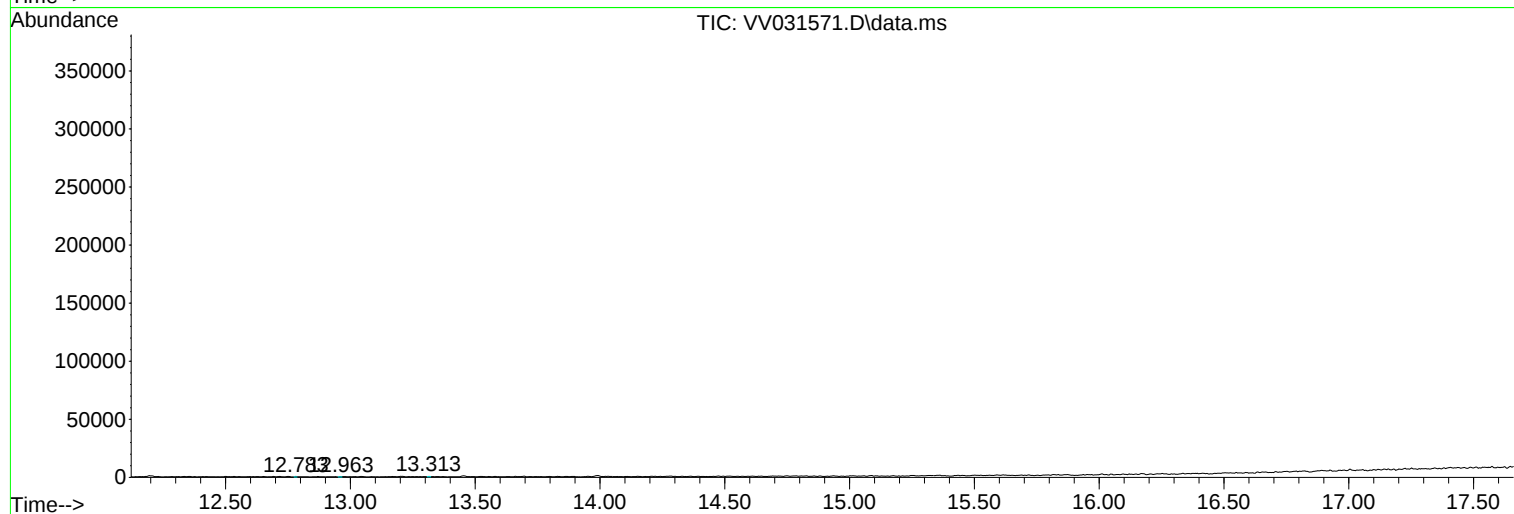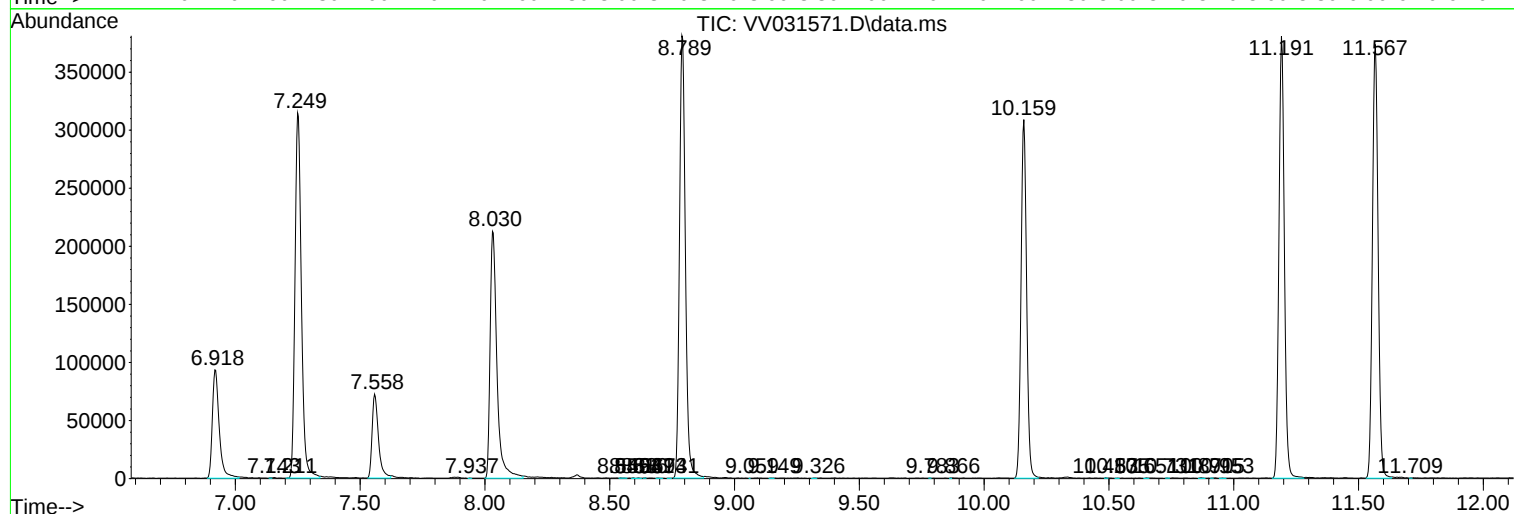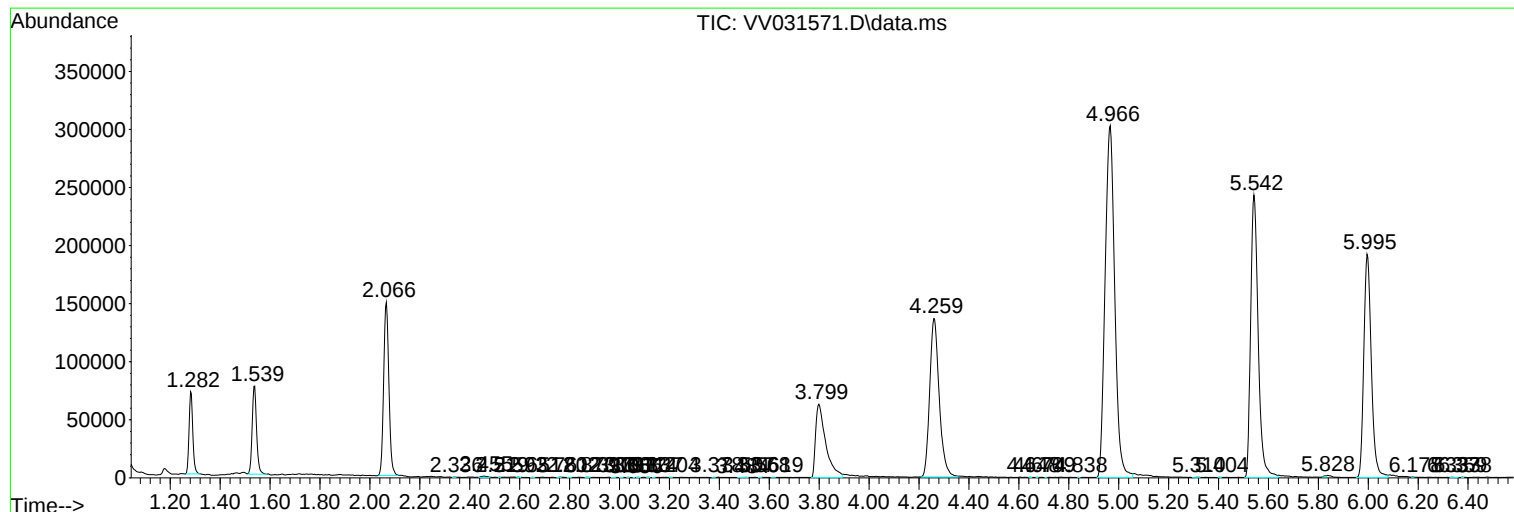

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031571.D
Acq On : 16 Jun 2023 13:14
Operator : SY/MD
Sample : 03254-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031571.D
Acq On : 16 Jun 2023 13:14
Operator : SY/MD
Sample : 03254-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------