

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031574.D
 Acq On : 16 Jun 2023 14:23
 Operator : SY/MD
 Sample : 03249-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	92	rVB2	100382	112332	13.99%	1.550%
2	1.539	148	155	156	rBV	80478	73188	9.12%	1.010%
3	2.066	309	319	338	rVB	156511	231898	28.88%	3.199%
4	2.458	430	441	453	rBV3	4708	8398	1.05%	0.116%
5	2.555	468	471	472	rBV2	392	256	0.03%	0.004%
6	2.709	509	519	529	rBV7	3163	5516	0.69%	0.076%
7	2.963	596	598	603	rVB2	381	245	0.03%	0.003%
8	3.008	609	612	615	rBV2	205	221	0.03%	0.003%
9	3.043	620	623	625	rBV	281	205	0.03%	0.003%
10	3.121	633	647	672	rBV	142381	298838	37.22%	4.123%
11	3.291	697	700	702	rVB2	352	157	0.02%	0.002%
12	3.400	729	734	737	rBV	189	208	0.03%	0.003%
13	3.465	748	754	758	rBV2	343	391	0.05%	0.005%
14	3.497	761	764	768	rBV2	193	188	0.02%	0.003%
15	3.642	806	809	813	rBV	250	197	0.02%	0.003%
16	3.732	832	837	840	rBV2	187	177	0.02%	0.002%
17	3.754	840	844	846	rBV	231	186	0.02%	0.003%
18	3.822	849	865	900	rBV3	131829	429829	53.54%	5.930%
19	4.262	985	1002	1028	rBV	130598	353341	44.01%	4.875%
20	4.523	1068	1083	1110	rVB2	59292	156137	19.45%	2.154%
21	4.654	1120	1124	1127	rBV3	405	350	0.04%	0.005%
22	4.712	1140	1142	1148	rBV2	204	124	0.02%	0.002%
23	4.879	1191	1194	1199	rVB2	217	196	0.02%	0.003%
24	4.966	1204	1221	1251	rBV2	302286	802892	100.00%	11.077%
25	5.307	1324	1327	1331	rBV3	395	311	0.04%	0.004%
26	5.336	1331	1336	1339	rVB2	432	338	0.04%	0.005%
27	5.371	1343	1347	1349	rBV	209	162	0.02%	0.002%
28	5.426	1361	1364	1369	rBB2	475	263	0.03%	0.004%
29	5.542	1388	1400	1423	rBV	273970	566147	70.51%	7.811%
30	5.850	1485	1496	1508	rBV7	3302	7174	0.89%	0.099%
31	5.947	1524	1526	1528	rBV	276	161	0.02%	0.002%
32	5.995	1528	1541	1561	rBV	188189	385470	48.01%	5.318%
33	6.240	1613	1617	1619	rBV2	259	159	0.02%	0.002%
34	6.455	1681	1684	1690	rVB2	420	425	0.05%	0.006%
35	6.484	1690	1693	1695	rBV2	206	133	0.02%	0.002%
36	6.587	1720	1725	1728	rBV2	194	208	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031574.D
 Acq On : 16 Jun 2023 14:23
 Operator : SY/MD
 Sample : 03249-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.632	1737	1739	1741	rVB	402	155	0.02%	0.002%
38	6.722	1765	1767	1772	rVB2	281	149	0.02%	0.002%
39	6.818	1793	1797	1801	rBV2	267	315	0.04%	0.004%
40	6.921	1816	1829	1847	rBV2	91914	170500	21.24%	2.352%
41	7.204	1915	1917	1920	rVB2	326	166	0.02%	0.002%
42	7.249	1920	1931	1949	rBV	317417	558291	69.54%	7.702%
43	7.558	2017	2027	2056	rBV	68132	123596	15.39%	1.705%
44	7.693	2066	2069	2073	rVB2	588	459	0.06%	0.006%
45	7.712	2073	2075	2077	rBV2	293	152	0.02%	0.002%
46	7.728	2077	2080	2084	rVB2	380	248	0.03%	0.003%
47	7.757	2084	2089	2092	rVB3	395	336	0.04%	0.005%
48	7.773	2092	2094	2096	rBV	352	177	0.02%	0.002%
49	7.883	2120	2128	2129	rVV2	1093	1093	0.14%	0.015%
50	7.915	2131	2138	2149	rVB3	8750	15094	1.88%	0.208%
51	8.034	2163	2175	2217	rBV	213226	398472	49.63%	5.497%
52	8.423	2292	2296	2297	rVB2	201	137	0.02%	0.002%
53	8.442	2297	2302	2305	rBV3	359	358	0.04%	0.005%
54	8.497	2317	2319	2322	rVB	323	158	0.02%	0.002%
55	8.532	2327	2330	2334	rBV	402	262	0.03%	0.004%
56	8.590	2346	2348	2354	rBV2	315	291	0.04%	0.004%
57	8.635	2360	2362	2368	rVB	268	186	0.02%	0.003%
58	8.670	2368	2373	2376	rBV2	230	203	0.03%	0.003%
59	8.789	2397	2410	2435	rBV	424975	696498	86.75%	9.609%
60	8.960	2457	2463	2472	rVB2	4934	6109	0.76%	0.084%
61	9.034	2483	2486	2492	rVB2	466	387	0.05%	0.005%
62	9.082	2492	2501	2515	rBV2	4933	8551	1.07%	0.118%
63	9.169	2525	2528	2531	rBV2	214	185	0.02%	0.003%
64	9.217	2541	2543	2545	rBV2	207	118	0.01%	0.002%
65	9.246	2546	2552	2556	rVB3	291	371	0.05%	0.005%
66	9.323	2573	2576	2579	rBV2	219	141	0.02%	0.002%
67	9.487	2621	2627	2641	rVV5	3602	5857	0.73%	0.081%
68	9.551	2644	2647	2650	rBV2	231	154	0.02%	0.002%
69	9.622	2665	2669	2671	rBV	277	182	0.02%	0.003%
70	9.799	2719	2724	2726	rBV2	280	250	0.03%	0.003%
71	9.927	2761	2764	2768	rBV	185	170	0.02%	0.002%
72	9.950	2768	2771	2774	rVV2	201	146	0.02%	0.002%
73	10.159	2825	2836	2859	rBV	300366	466838	58.14%	6.441%
74	10.297	2872	2879	2883	rBV3	1336	1518	0.19%	0.021%
75	10.397	2903	2910	2924	rBV4	1991	4221	0.53%	0.058%
76	10.487	2932	2938	2949	rVB4	1363	1790	0.22%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031574.D
 Acq On : 16 Jun 2023 14:23
 Operator : SY/MD
 Sample : 03249-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	10.590	2966	2970	2973	rBV	212	186	0.02%	0.003%
78	10.680	2992	2998	3011	rBV3	3854	5959	0.74%	0.082%
79	10.860	3047	3054	3068	rVB2	8474	13203	1.64%	0.182%
80	10.966	3085	3087	3091	rBV	278	222	0.03%	0.003%
81	11.030	3102	3107	3110	rBV3	573	595	0.07%	0.008%
82	11.140	3134	3141	3146	rBV2	804	903	0.11%	0.012%
83	11.191	3146	3157	3177	rBV	455233	691145	86.08%	9.535%
84	11.358	3206	3209	3215	rBV4	302	336	0.04%	0.005%
85	11.468	3237	3243	3244	rBV4	1777	1432	0.18%	0.020%
86	11.567	3262	3274	3297	rVB	401200	627195	78.12%	8.653%
87	11.918	3380	3383	3384	rBV	328	215	0.03%	0.003%
88	12.336	3511	3513	3516	rBV	248	137	0.02%	0.002%
89	12.410	3532	3536	3546	rBV3	930	1226	0.15%	0.017%
90	12.808	3657	3660	3661	rBV3	354	171	0.02%	0.002%
91	12.824	3661	3665	3671	rVV6	1241	1350	0.17%	0.019%
92	12.924	3694	3696	3697	rBV6	341	137	0.02%	0.002%
93	13.043	3729	3733	3737	rBV	309	301	0.04%	0.004%
94	13.271	3802	3804	3807	rBV	328	163	0.02%	0.002%
95	13.358	3829	3831	3835	rVB2	338	177	0.02%	0.002%
96	13.448	3854	3859	3860	rBV2	2043	1438	0.18%	0.020%
97	13.818	3972	3974	3976	rBV2	307	181	0.02%	0.002%
98	13.882	3991	3994	3995	rBV	267	173	0.02%	0.002%
99	14.268	4110	4114	4119	rBV2	456	397	0.05%	0.005%
100	14.410	4155	4158	4160	rBV3	468	372	0.05%	0.005%

Sum of corrected areas: 7248319




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031574.D
Acq On : 16 Jun 2023 14:23
Operator : SY/MD
Sample : 03249-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

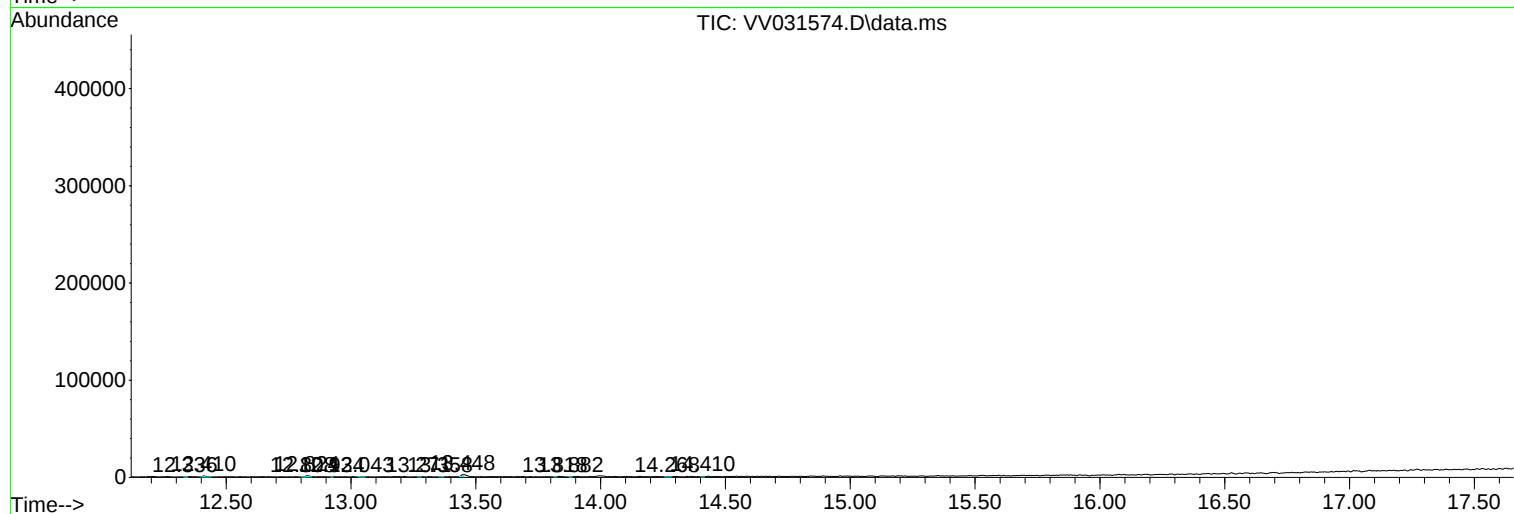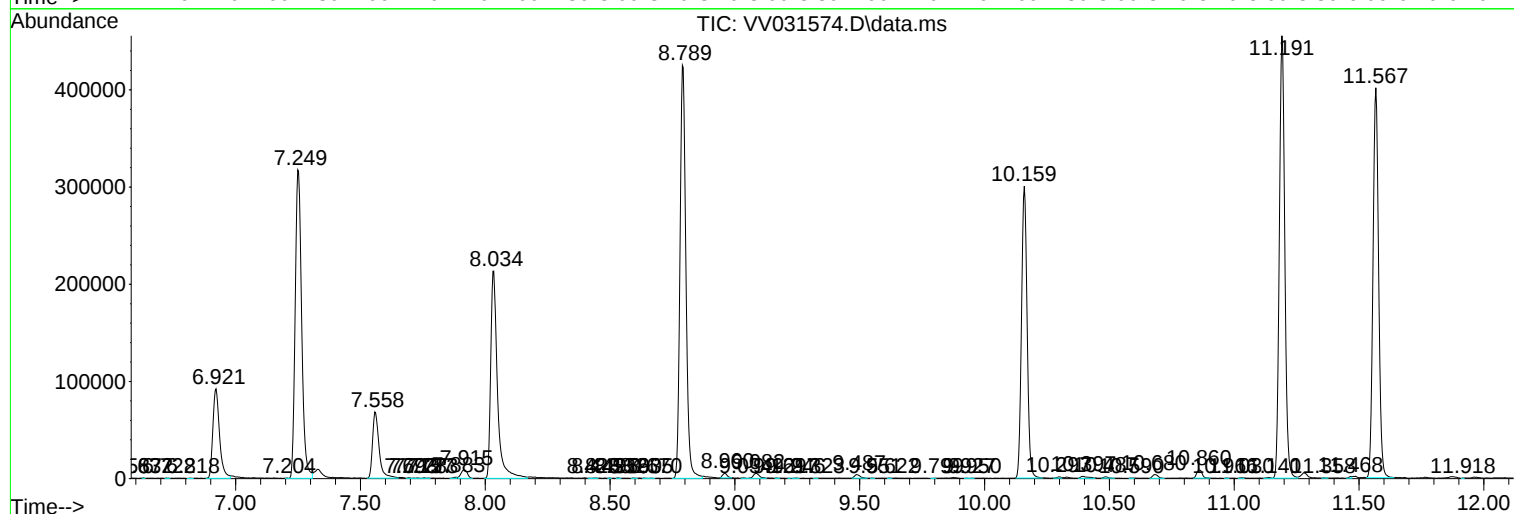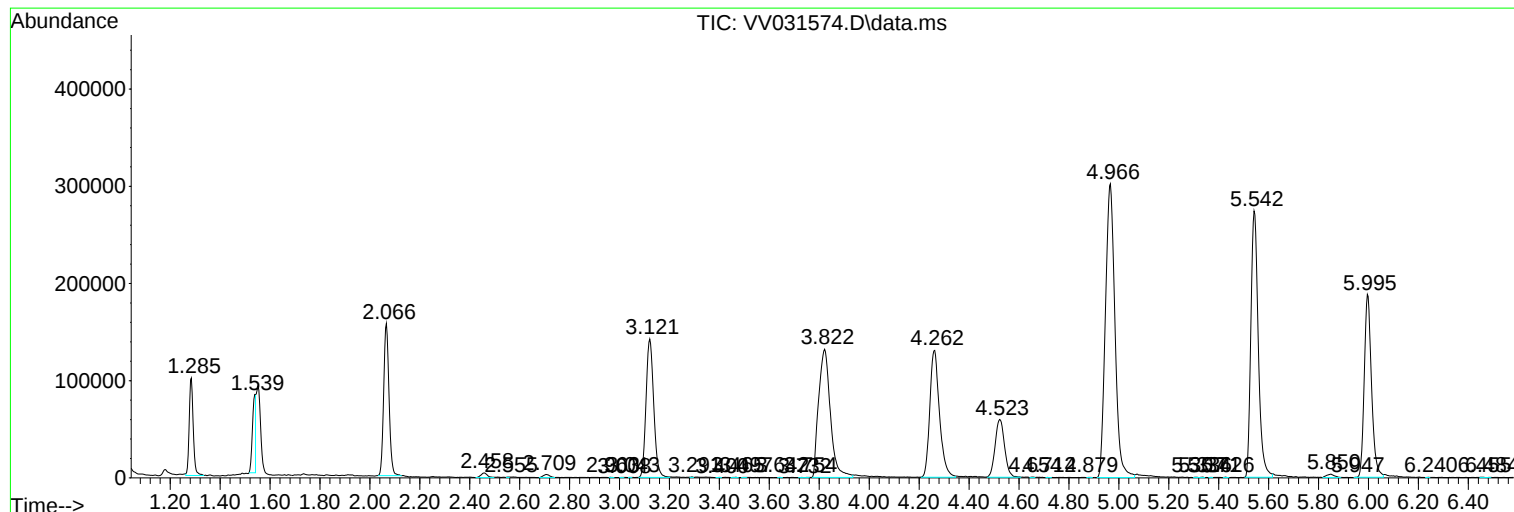

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031574.D
Acq On : 16 Jun 2023 14:23
Operator : SY/MD
Sample : 03249-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031574.D
Acq On : 16 Jun 2023 14:23
Operator : SY/MD
Sample : 03249-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------