

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031575.D
 Acq On : 16 Jun 2023 14:46
 Operator : SY/MD
 Sample : 03249-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	88	rVB2	93879	100854	12.30%	1.354%
2	1.535	148	154	168	rVB	78613	98795	12.05%	1.326%
3	2.066	310	319	334	rVB2	162353	235432	28.72%	3.161%
4	2.458	431	441	453	rBV2	6859	11656	1.42%	0.156%
5	2.548	467	469	471	rBV2	394	243	0.03%	0.003%
6	2.709	509	519	529	rVB5	2502	4400	0.54%	0.059%
7	2.867	564	568	570	rBV	222	207	0.03%	0.003%
8	3.053	625	626	630	rBV	189	105	0.01%	0.001%
9	3.121	635	647	668	rVV	88761	183707	22.41%	2.466%
10	3.365	718	723	724	rBV2	194	166	0.02%	0.002%
11	3.429	737	743	747	rBV2	235	284	0.03%	0.004%
12	3.452	747	750	751	rBV	114	48	0.01%	0.001%
13	3.465	751	754	756	rBV2	224	150	0.02%	0.002%
14	3.497	761	764	766	rBV2	80	56	0.01%	0.001%
15	3.593	792	794	796	rBV2	133	71	0.01%	0.001%
16	3.625	800	804	806	rBV2	182	145	0.02%	0.002%
17	3.641	806	809	815	rVB	195	167	0.02%	0.002%
18	3.699	824	827	829	rBV	230	126	0.02%	0.002%
19	3.719	829	833	836	rBV	282	219	0.03%	0.003%
20	3.821	847	865	901	rBV3	214448	645552	78.74%	8.667%
21	4.259	986	1001	1026	rBV	135448	358392	43.72%	4.811%
22	4.522	1068	1083	1105	rVB2	93525	235970	28.78%	3.168%
23	4.738	1148	1150	1153	rBV2	314	190	0.02%	0.003%
24	4.889	1194	1197	1201	rBV2	146	141	0.02%	0.002%
25	4.966	1203	1221	1249	rBV2	306079	819822	100.00%	11.006%
26	5.281	1316	1319	1321	rBV	320	219	0.03%	0.003%
27	5.352	1339	1341	1343	rBB2	396	95	0.01%	0.001%
28	5.542	1388	1400	1426	rBV	277760	571700	69.73%	7.675%
29	5.847	1485	1495	1506	rBV	3676	7693	0.94%	0.103%
30	5.947	1522	1526	1528	rBV2	347	239	0.03%	0.003%
31	5.995	1528	1541	1565	rBV	192251	396252	48.33%	5.320%
32	6.198	1601	1604	1607	rBV	219	163	0.02%	0.002%
33	6.220	1610	1611	1613	rBV	170	48	0.01%	0.001%
34	6.275	1626	1628	1631	rBV	196	125	0.02%	0.002%
35	6.429	1674	1676	1683	rVB2	310	222	0.03%	0.003%
36	6.882	1814	1817	1818	rBV	171	93	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031575.D
 Acq On : 16 Jun 2023 14:46
 Operator : SY/MD
 Sample : 03249-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.918	1818	1828	1854	rBV	92985	176763	21.56%	2.373%
38	7.136	1890	1896	1898	rBV4	839	782	0.10%	0.010%
39	7.165	1903	1905	1907	rBV2	321	163	0.02%	0.002%
40	7.249	1919	1931	1958	rBV	323184	576310	70.30%	7.737%
41	7.558	2015	2027	2053	rBV	69751	128369	15.66%	1.723%
42	7.780	2093	2096	2099	rBV	312	223	0.03%	0.003%
43	7.969	2151	2155	2156	rBV	289	209	0.03%	0.003%
44	8.030	2165	2174	2203	rBV	222633	401685	49.00%	5.393%
45	8.300	2256	2258	2261	rBV2	312	132	0.02%	0.002%
46	8.390	2283	2286	2292	rBV2	301	382	0.05%	0.005%
47	8.493	2316	2318	2322	rBV2	331	227	0.03%	0.003%
48	8.699	2379	2382	2385	rBV2	223	150	0.02%	0.002%
49	8.789	2398	2410	2434	rBV	423464	693107	84.54%	9.305%
50	9.323	2569	2576	2581	rBV3	370	544	0.07%	0.007%
51	9.406	2600	2602	2605	rBV2	196	129	0.02%	0.002%
52	9.426	2605	2608	2610	rVB2	259	139	0.02%	0.002%
53	9.493	2623	2629	2636	rBV3	766	1038	0.13%	0.014%
54	9.561	2645	2650	2652	rVB2	173	165	0.02%	0.002%
55	9.577	2652	2655	2657	rBV2	207	162	0.02%	0.002%
56	9.625	2667	2670	2675	rVB3	273	207	0.03%	0.003%
57	10.159	2825	2836	2856	rBV	308992	484245	59.07%	6.501%
58	10.487	2935	2938	2943	rBV3	550	466	0.06%	0.006%
59	10.513	2943	2946	2948	rBV2	315	196	0.02%	0.003%
60	10.744	3013	3018	3021	rBV	197	172	0.02%	0.002%
61	10.863	3048	3055	3057	rBV4	1223	1260	0.15%	0.017%
62	10.911	3068	3070	3071	rBV4	178	80	0.01%	0.001%
63	11.008	3097	3100	3101	rBV2	275	167	0.02%	0.002%
64	11.078	3121	3122	3123	rBV2	227	58	0.01%	0.001%
65	11.191	3145	3157	3177	rBV	433951	668247	81.51%	8.971%
66	11.461	3238	3241	3245	rBV2	230	242	0.03%	0.003%
67	11.567	3262	3274	3298	rBV	404001	635739	77.55%	8.535%
68	11.866	3364	3367	3368	rBV	504	267	0.03%	0.004%
69	12.162	3456	3459	3460	rBV	222	131	0.02%	0.002%
70	12.500	3563	3564	3565	rBV	232	76	0.01%	0.001%
71	12.815	3656	3662	3665	rBV	339	470	0.06%	0.006%
72	12.879	3679	3682	3684	rBV	205	148	0.02%	0.002%
73	13.046	3731	3734	3735	rBV	256	129	0.02%	0.002%
74	13.451	3856	3860	3870	rVB4	975	1299	0.16%	0.017%
75	13.574	3895	3898	3900	rBV2	269	148	0.02%	0.002%
76	13.744	3948	3951	3955	rVB2	442	267	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031575.D
Acq On : 16 Jun 2023 14:46
Operator : SY/MD
Sample : 03249-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis

77	14.528	4193	4195	4196	rBV2	567	223	0.03%	0.003%
----	--------	------	------	------	------	-----	-----	-------	--------




Sum of corrected areas: 7448663

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031575.D
Acq On : 16 Jun 2023 14:46
Operator : SY/MD
Sample : 03249-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

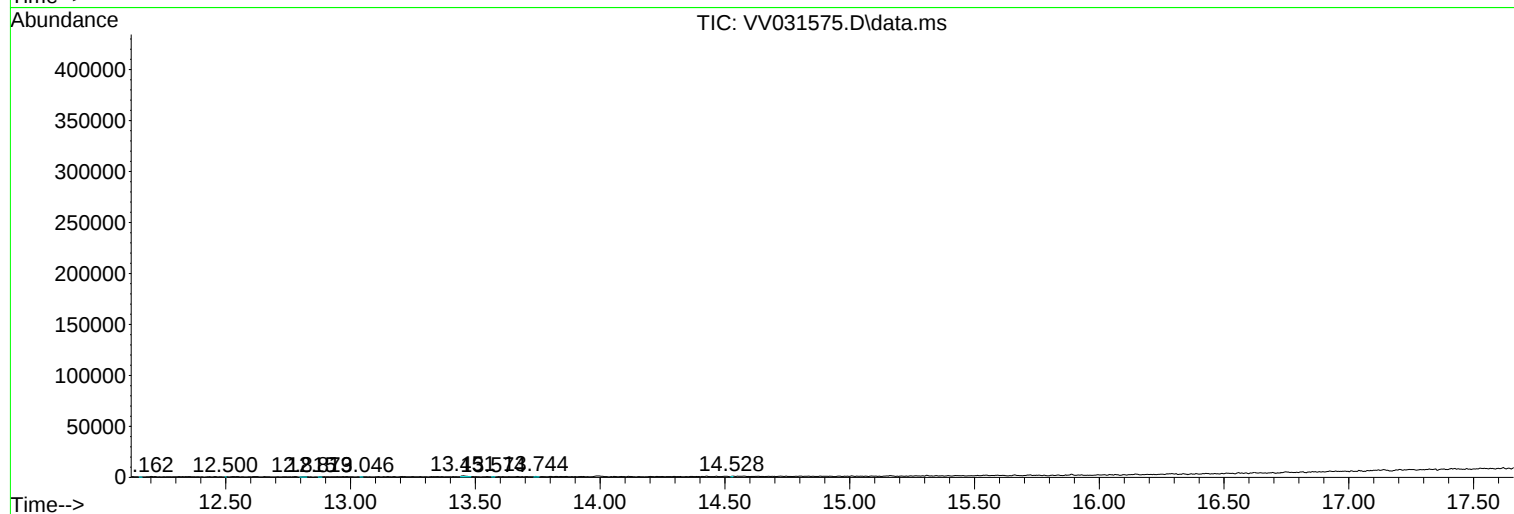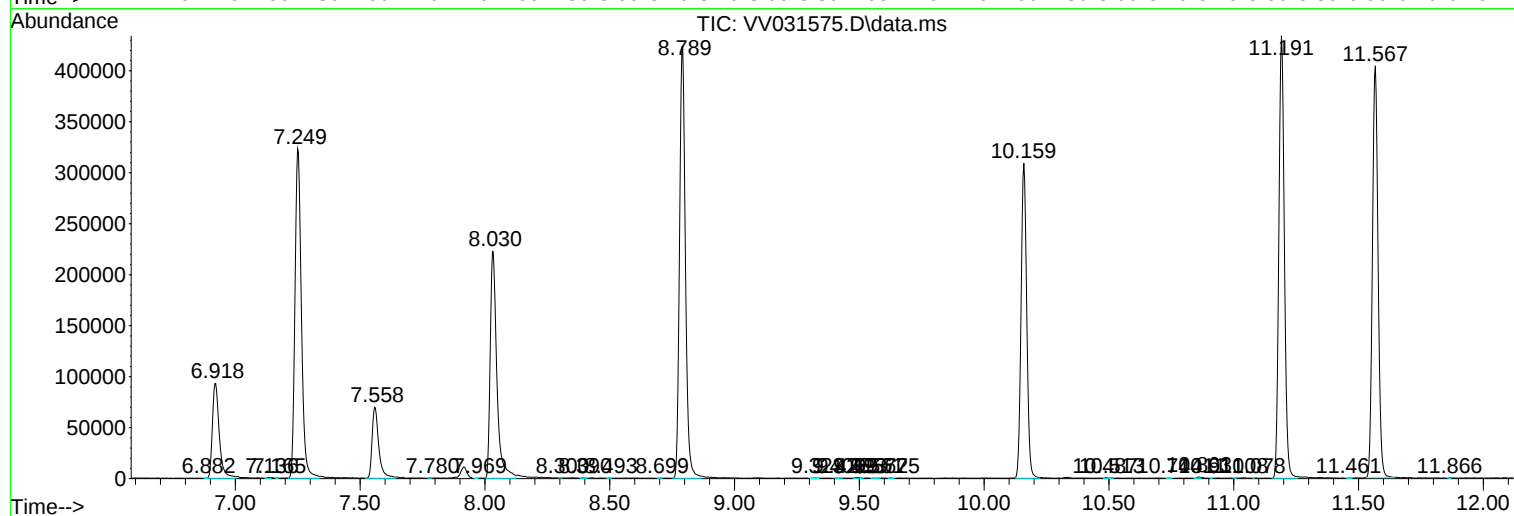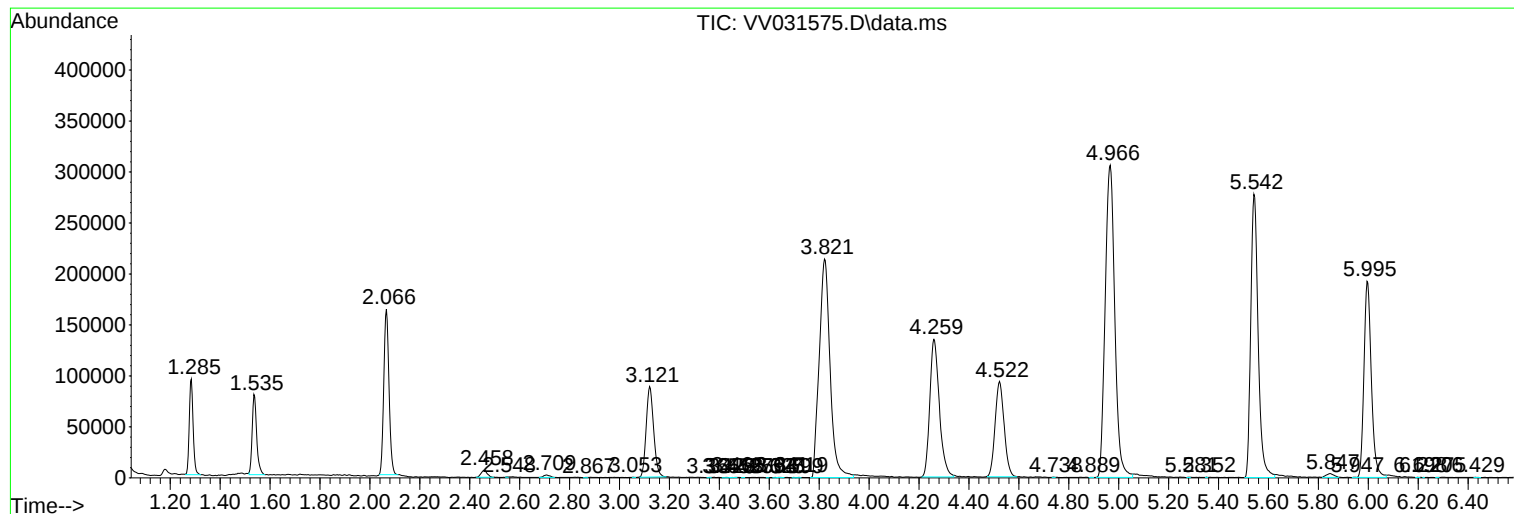

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031575.D
Acq On : 16 Jun 2023 14:46
Operator : SY/MD
Sample : 03249-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031575.D
Acq On : 16 Jun 2023 14:46
Operator : SY/MD
Sample : 03249-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------