

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031576.D
 Acq On : 16 Jun 2023 15:10
 Operator : SY/MD
 Sample : 03249-06DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	91	rVB2	84329	93529	11.66%	1.314%
2	1.535	148	154	170	rVB	77333	93371	11.64%	1.312%
3	2.066	309	319	336	rBV	156501	229959	28.68%	3.232%
4	2.455	429	440	455	rVB	9689	17276	2.15%	0.243%
5	2.561	471	473	476	rBV	459	301	0.04%	0.004%
6	2.706	510	518	524	rBV4	1495	2384	0.30%	0.034%
7	2.738	526	528	530	rBV	133	65	0.01%	0.001%
8	2.773	534	539	546	rBV3	282	445	0.06%	0.006%
9	2.825	553	555	558	rVB	231	104	0.01%	0.001%
10	2.982	601	604	607	rBV2	248	157	0.02%	0.002%
11	3.047	622	624	626	rBV2	169	86	0.01%	0.001%
12	3.121	635	647	665	rBV2	48341	99170	12.37%	1.394%
13	3.391	727	731	733	rBV2	230	197	0.02%	0.003%
14	3.474	755	757	759	rBV	236	161	0.02%	0.002%
15	3.510	765	768	770	rBV	195	152	0.02%	0.002%
16	3.597	793	795	798	rVB2	219	135	0.02%	0.002%
17	3.616	798	801	804	rBV2	230	193	0.02%	0.003%
18	3.822	848	865	898	rBV3	177704	543693	67.80%	7.641%
19	4.259	985	1001	1032	rBV	134144	354698	44.23%	4.985%
20	4.523	1069	1083	1101	rVB2	60913	151737	18.92%	2.132%
21	4.625	1113	1115	1119	rBV3	409	192	0.02%	0.003%
22	4.674	1127	1130	1132	rBV2	311	174	0.02%	0.002%
23	4.722	1143	1145	1149	rBV2	231	227	0.03%	0.003%
24	4.883	1192	1195	1199	rVB2	380	310	0.04%	0.004%
25	4.963	1199	1220	1249	rBV2	299906	801941	100.00%	11.270%
26	5.413	1358	1360	1363	rBV2	375	204	0.03%	0.003%
27	5.542	1387	1400	1427	rBV	284222	580923	72.44%	8.164%
28	5.841	1484	1493	1507	rVB6	2569	5602	0.70%	0.079%
29	5.995	1528	1541	1567	rBV	189001	390496	48.69%	5.488%
30	6.275	1626	1628	1630	rBV2	183	81	0.01%	0.001%
31	6.400	1664	1667	1671	rVB	429	237	0.03%	0.003%
32	6.426	1671	1675	1679	rBV2	228	209	0.03%	0.003%
33	6.481	1690	1692	1694	rVB	210	93	0.01%	0.001%
34	6.664	1747	1749	1755	rBV2	193	187	0.02%	0.003%
35	6.728	1764	1769	1771	rBV	168	149	0.02%	0.002%
36	6.776	1781	1784	1786	rBV	172	111	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031576.D
 Acq On : 16 Jun 2023 15:10
 Operator : SY/MD
 Sample : 03249-06DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.921	1818	1829	1863	rBV	90532	172445	21.50%	2.423%
38	7.133	1892	1895	1899	rVB2	553	416	0.05%	0.006%
39	7.153	1899	1901	1902	rBV	233	82	0.01%	0.001%
40	7.252	1920	1932	1954	rBV	316014	561793	70.05%	7.895%
41	7.493	2003	2007	2009	rBV2	264	252	0.03%	0.004%
42	7.558	2015	2027	2049	rBV	69504	124660	15.54%	1.752%
43	7.805	2101	2104	2106	rBV	486	278	0.03%	0.004%
44	7.876	2123	2126	2127	rBV2	524	331	0.04%	0.005%
45	7.915	2131	2138	2149	rVB5	6171	10245	1.28%	0.144%
46	7.969	2151	2155	2156	rBV2	291	185	0.02%	0.003%
47	8.034	2164	2175	2202	rBV	213321	388843	48.49%	5.464%
48	8.423	2292	2296	2297	rBV2	345	252	0.03%	0.004%
49	8.509	2321	2323	2327	rVB2	258	129	0.02%	0.002%
50	8.657	2366	2369	2371	rBV2	157	109	0.01%	0.002%
51	8.792	2399	2411	2433	rBV	429167	705546	87.98%	9.915%
52	8.992	2472	2473	2477	rVB	233	113	0.01%	0.002%
53	9.037	2485	2487	2489	rBV	275	108	0.01%	0.002%
54	9.091	2501	2504	2511	rVB3	612	432	0.05%	0.006%
55	9.204	2536	2539	2542	rBV2	274	190	0.02%	0.003%
56	9.435	2609	2611	2613	rBV2	164	79	0.01%	0.001%
57	9.490	2621	2628	2630	rBV4	1368	1569	0.20%	0.022%
58	9.558	2647	2649	2651	rBV	155	72	0.01%	0.001%
59	9.632	2668	2672	2677	rBV2	208	219	0.03%	0.003%
60	9.696	2690	2692	2697	rBV2	151	122	0.02%	0.002%
61	9.728	2698	2702	2706	rVB2	244	251	0.03%	0.004%
62	9.751	2706	2709	2710	rBV	192	110	0.01%	0.002%
63	9.770	2714	2715	2716	rBV	196	66	0.01%	0.001%
64	9.873	2744	2747	2748	rBV2	321	188	0.02%	0.003%
65	9.934	2763	2766	2769	rVB	374	241	0.03%	0.003%
66	9.956	2769	2773	2775	rBV	262	223	0.03%	0.003%
67	10.085	2810	2813	2815	rBV2	245	155	0.02%	0.002%
68	10.159	2825	2836	2864	rVB	302079	470923	58.72%	6.618%
69	10.275	2869	2872	2874	rBV	313	137	0.02%	0.002%
70	10.291	2874	2877	2880	rBV	428	358	0.04%	0.005%
71	10.487	2933	2938	2945	rBV2	805	923	0.12%	0.013%
72	10.628	2980	2982	2984	rBV2	125	70	0.01%	0.001%
73	10.718	3006	3010	3013	rBV2	367	288	0.04%	0.004%
74	10.831	3039	3045	3048	rBV2	308	419	0.05%	0.006%
75	10.866	3048	3056	3061	rBV5	1872	2464	0.31%	0.035%
76	11.005	3097	3099	3103	rBV	308	230	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031576.D
 Acq On : 16 Jun 2023 15:10
 Operator : SY/MD
 Sample : 03249-06DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.062	3115	3117	3118	rBV	144	60	0.01%	0.001%
78	11.107	3128	3131	3133	rBV2	206	150	0.02%	0.002%
79	11.191	3145	3157	3175	rBV	446078	680081	84.80%	9.557%
80	11.519	3257	3259	3261	rBV	364	169	0.02%	0.002%
81	11.567	3262	3274	3293	rVV	403185	617599	77.01%	8.679%
82	11.947	3390	3392	3394	rBV	170	106	0.01%	0.001%
83	12.767	3646	3647	3648	rBV	263	57	0.01%	0.001%
84	12.824	3661	3665	3668	rBV3	478	349	0.04%	0.005%
85	13.185	3774	3777	3778	rBV	296	151	0.02%	0.002%
86	13.252	3795	3798	3801	rBV	267	180	0.02%	0.003%
87	13.316	3813	3818	3822	rBV2	538	551	0.07%	0.008%
88	13.397	3840	3843	3845	rBV2	347	234	0.03%	0.003%
89	13.439	3853	3856	3858	rBV3	773	559	0.07%	0.008%
90	13.493	3870	3873	3874	rBV	327	174	0.02%	0.002%
91	14.435	4164	4166	4169	rBV	362	271	0.03%	0.004%
92	14.532	4194	4196	4198	rBV	389	180	0.02%	0.003%
93	14.680	4239	4242	4245	rBV2	628	507	0.06%	0.007%




Sum of corrected areas: 7115843

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031576.D
Acq On : 16 Jun 2023 15:10
Operator : SY/MD
Sample : 03249-06DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

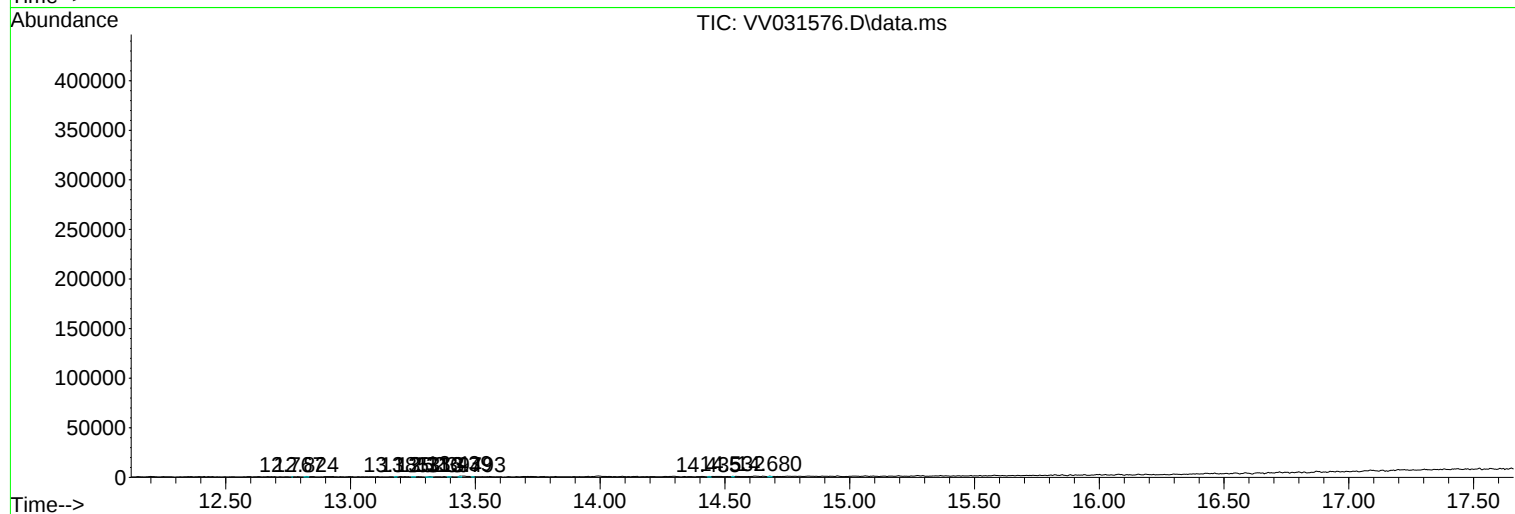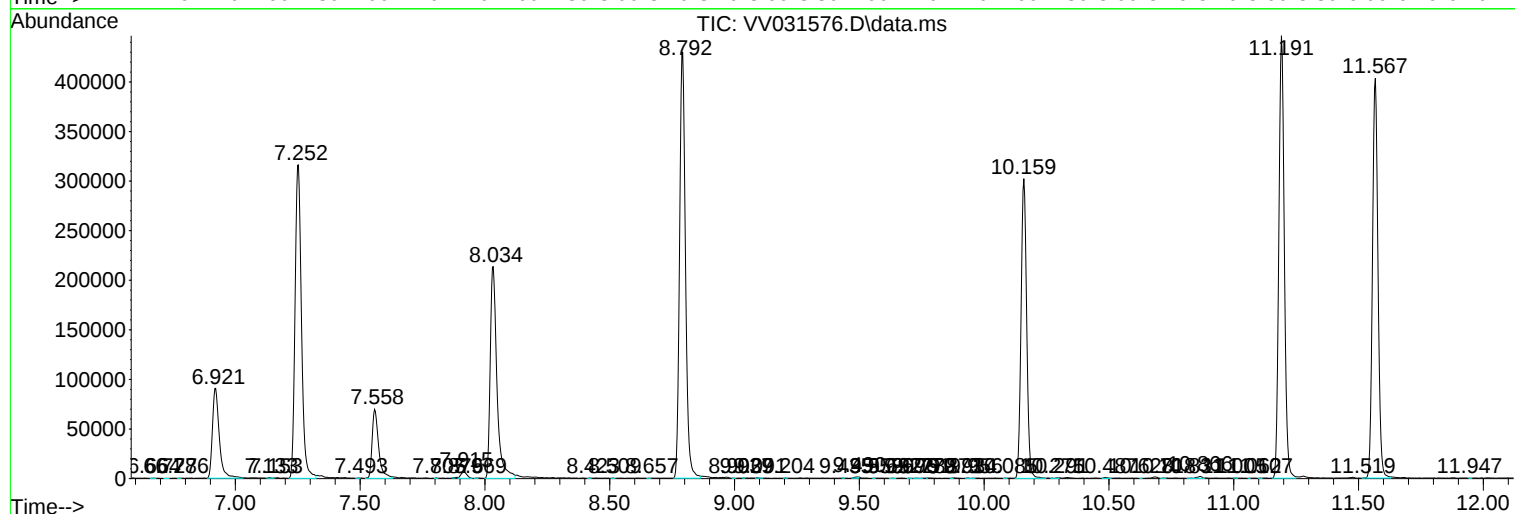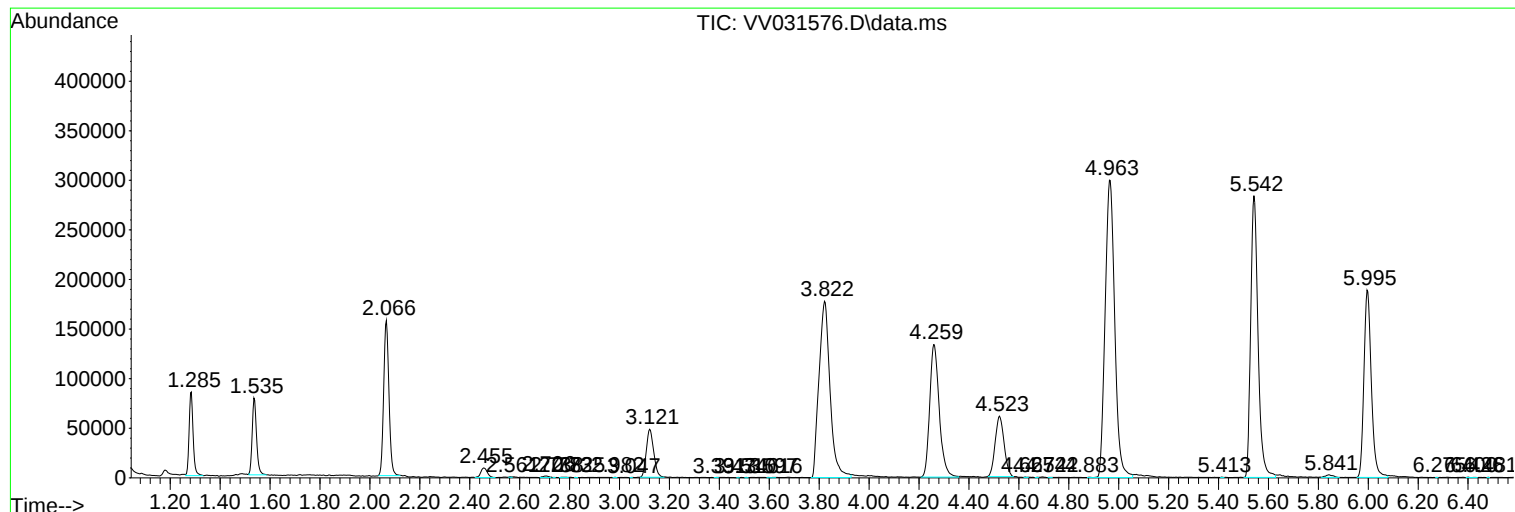

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031576.D
Acq On : 16 Jun 2023 15:10
Operator : SY/MD
Sample : 03249-06DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031576.D
Acq On : 16 Jun 2023 15:10
Operator : SY/MD
Sample : 03249-06DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------