

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031577.D
 Acq On : 16 Jun 2023 15:33
 Operator : SY/MD
 Sample : 03249-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	62331	67180	11.13%	1.273%
2	1.535	148	154	168	rVB	62460	74581	12.36%	1.413%
3	2.066	309	319	334	rBV2	129027	197361	32.71%	3.740%
4	2.516	456	459	460	rBV2	154	89	0.01%	0.002%
5	2.706	510	518	521	rBV4	1759	2131	0.35%	0.040%
6	2.828	554	556	561	rBV2	315	102	0.02%	0.002%
7	2.953	593	595	600	rBV2	266	229	0.04%	0.004%
8	3.060	625	628	631	rBV	323	190	0.03%	0.004%
9	3.121	635	647	665	rVV	21186	44074	7.30%	0.835%
10	3.230	678	681	684	rBV2	182	182	0.03%	0.003%
11	3.275	692	695	698	rBV2	215	145	0.02%	0.003%
12	3.301	698	703	706	rBV2	209	272	0.05%	0.005%
13	3.458	749	752	755	rBV2	245	157	0.03%	0.003%
14	3.474	755	757	759	rBV	160	95	0.02%	0.002%
15	3.510	764	768	771	rBV2	264	210	0.03%	0.004%
16	3.555	779	782	784	rBV	206	102	0.02%	0.002%
17	3.571	784	787	792	rBV2	189	208	0.03%	0.004%
18	3.616	797	801	803	rBV2	137	117	0.02%	0.002%
19	3.754	842	844	845	rBV	150	39	0.01%	0.001%
20	3.799	849	858	894	rBV2	59300	184400	30.56%	3.495%
21	4.262	985	1002	1029	rBV2	100208	274833	45.55%	5.208%
22	4.523	1065	1083	1104	rBV	150358	388371	64.37%	7.360%
23	4.783	1161	1164	1167	rBV2	321	196	0.03%	0.004%
24	4.966	1204	1221	1248	rBV3	226752	603371	100.00%	11.435%
25	5.275	1314	1317	1320	rVB3	507	274	0.05%	0.005%
26	5.368	1343	1346	1349	rBV2	257	168	0.03%	0.003%
27	5.545	1388	1401	1429	rBV	185513	388690	64.42%	7.366%
28	5.850	1486	1496	1514	rVB7	8128	17569	2.91%	0.333%
29	5.995	1528	1541	1567	rBV2	140993	294897	48.87%	5.589%
30	6.281	1627	1630	1631	rBV	175	79	0.01%	0.001%
31	6.439	1677	1679	1680	rBV	140	35	0.01%	0.001%
32	6.921	1819	1829	1848	rBV2	67189	124060	20.56%	2.351%
33	7.095	1880	1883	1887	rBV2	292	252	0.04%	0.005%
34	7.252	1920	1932	1961	rBV	218084	395907	65.62%	7.503%
35	7.561	2018	2028	2047	rBV	51423	90987	15.08%	1.724%
36	7.757	2086	2089	2092	rBV2	418	237	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031577.D
 Acq On : 16 Jun 2023 15:33
 Operator : SY/MD
 Sample : 03249-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.831	2110	2112	2119	rVB2	260	147	0.02%	0.003%
38	7.883	2119	2128	2129	rBV4	2359	2843	0.47%	0.054%
39	7.992	2159	2162	2165	rBV2	324	242	0.04%	0.005%
40	8.034	2165	2175	2209	rBV	193390	354469	58.75%	6.718%
41	8.551	2334	2336	2337	rBV	239	51	0.01%	0.001%
42	8.792	2399	2411	2432	rBV	294886	492327	81.60%	9.330%
43	9.001	2474	2476	2481	rVB	206	129	0.02%	0.002%
44	9.030	2482	2485	2489	rBV2	358	252	0.04%	0.005%
45	9.111	2508	2510	2515	rVB2	231	122	0.02%	0.002%
46	9.268	2556	2559	2561	rBV	274	216	0.04%	0.004%
47	9.304	2566	2570	2572	rBV	242	194	0.03%	0.004%
48	9.394	2592	2598	2600	rBV	429	512	0.08%	0.010%
49	9.609	2664	2665	2666	rBV	162	34	0.01%	0.001%
50	9.876	2746	2748	2750	rBV	310	151	0.03%	0.003%
51	10.159	2825	2836	2861	rBV	244465	385633	63.91%	7.308%
52	10.278	2870	2873	2874	rBV	273	118	0.02%	0.002%
53	10.329	2884	2889	2898	rVB4	2732	3805	0.63%	0.072%
54	10.490	2938	2939	2942	rBV2	256	141	0.02%	0.003%
55	10.635	2980	2984	2988	rBV	279	243	0.04%	0.005%
56	10.853	3048	3052	3053	rBV	370	243	0.04%	0.005%
57	11.001	3093	3098	3102	rBV3	337	354	0.06%	0.007%
58	11.098	3124	3128	3130	rBV	330	265	0.04%	0.005%
59	11.133	3136	3139	3140	rVB2	424	201	0.03%	0.004%
60	11.146	3140	3143	3146	rBV	165	115	0.02%	0.002%
61	11.191	3146	3157	3182	rVV	291163	454973	75.41%	8.622%
62	11.567	3262	3274	3296	rBV	272441	423065	70.12%	8.018%
63	11.815	3349	3351	3358	rVB2	356	231	0.04%	0.004%
64	11.879	3369	3371	3372	rBV	315	136	0.02%	0.003%
65	12.021	3410	3415	3419	rBV3	489	586	0.10%	0.011%
66	12.204	3463	3472	3481	rBV4	1181	1766	0.29%	0.033%
67	12.336	3510	3513	3514	rBV	276	175	0.03%	0.003%
68	12.750	3639	3642	3643	rBV	295	185	0.03%	0.004%
69	13.455	3856	3861	3865	rBV4	859	933	0.15%	0.018%




Sum of corrected areas: 5276647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031577.D
Acq On : 16 Jun 2023 15:33
Operator : SY/MD
Sample : 03249-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

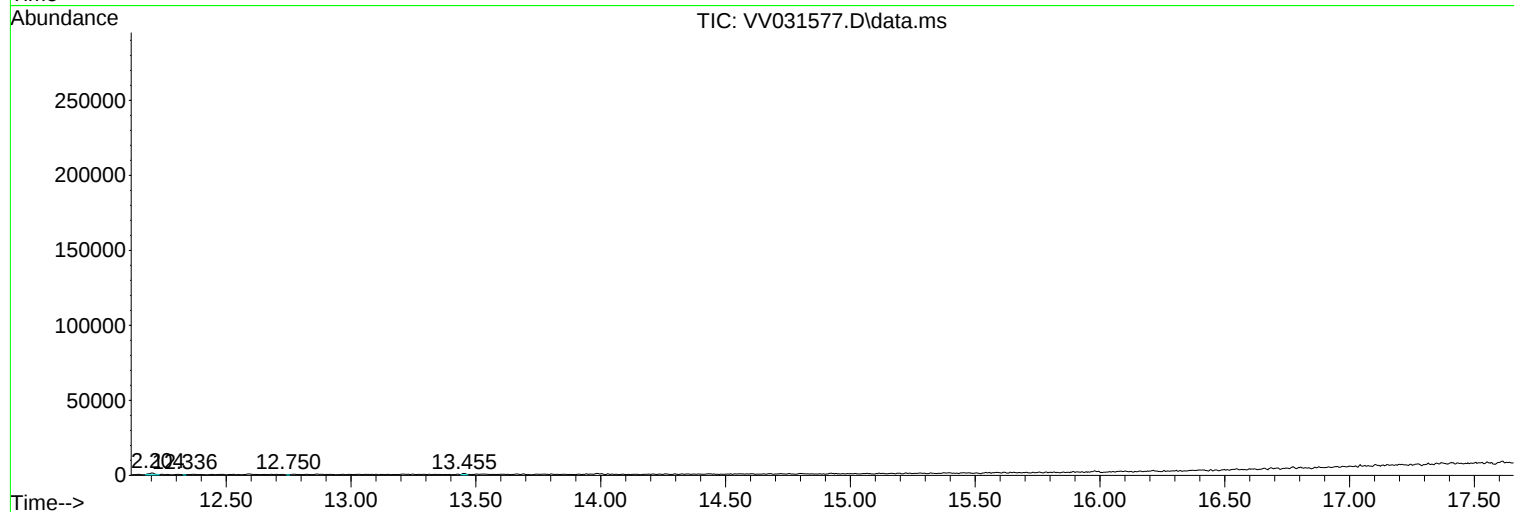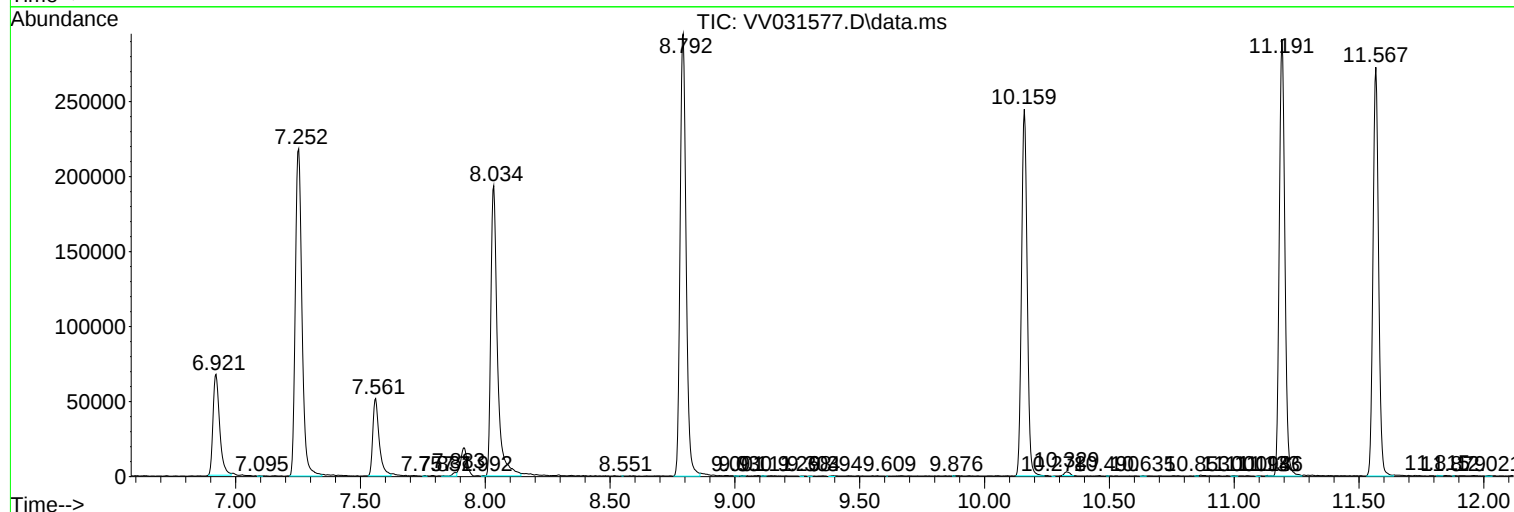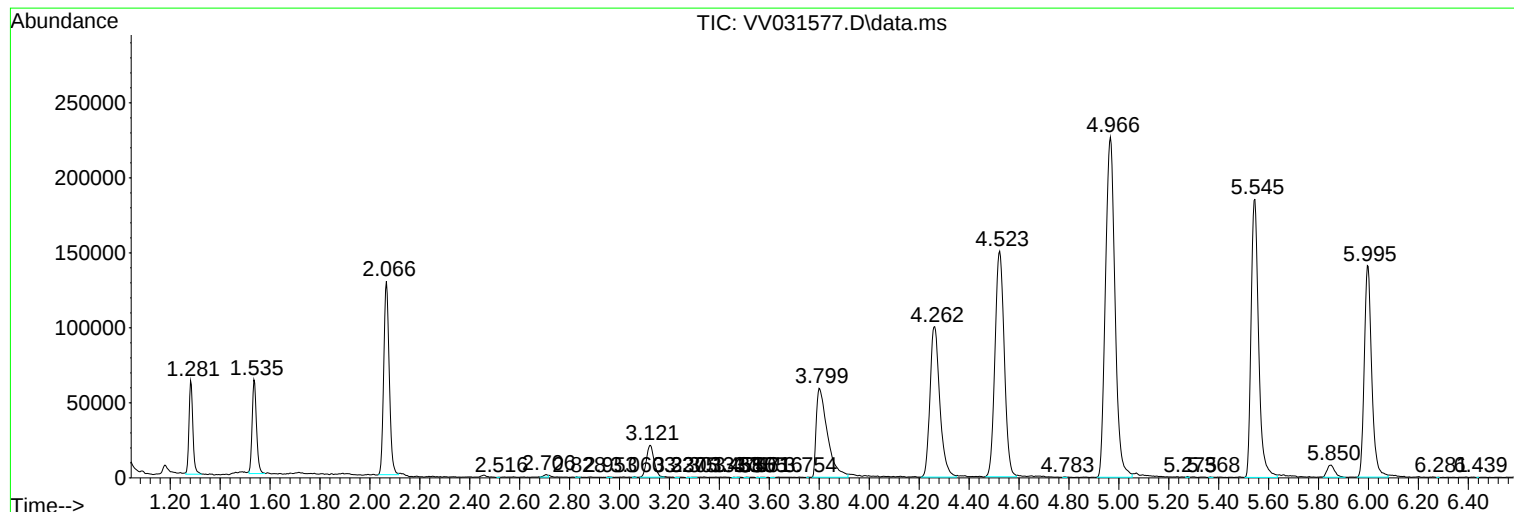

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031577.D
Acq On : 16 Jun 2023 15:33
Operator : SY/MD
Sample : 03249-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031577.D
Acq On : 16 Jun 2023 15:33
Operator : SY/MD
Sample : 03249-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc