

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031578.D
 Acq On : 16 Jun 2023 15:56
 Operator : SY/MD
 Sample : 03249-08DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	92	rVB2	121230	136691	16.33%	1.803%
2	1.536	148	154	170	rVB	86350	106574	12.73%	1.405%
3	2.066	308	319	335	rBV	184134	272718	32.58%	3.597%
4	2.333	400	402	405	rBV	263	165	0.02%	0.002%
5	2.458	432	441	452	rVB3	6958	12401	1.48%	0.164%
6	2.519	458	460	462	rBV2	199	137	0.02%	0.002%
7	2.709	511	519	528	rVB4	2190	3581	0.43%	0.047%
8	2.818	548	553	556	rBV2	224	271	0.03%	0.004%
9	2.954	592	595	598	rBV	257	198	0.02%	0.003%
10	3.040	619	622	626	rBV	177	103	0.01%	0.001%
11	3.066	628	630	633	rBV	271	166	0.02%	0.002%
12	3.121	634	647	671	rVV2	63164	134079	16.02%	1.768%
13	3.436	739	745	746	rBV2	402	391	0.05%	0.005%
14	3.484	758	760	762	rBV	112	79	0.01%	0.001%
15	3.677	817	820	822	rBV	237	170	0.02%	0.002%
16	3.822	848	865	896	rBV3	214168	629820	75.25%	8.306%
17	4.259	986	1001	1028	rBV	138799	365536	43.67%	4.821%
18	4.523	1069	1083	1100	rBV3	38487	96540	11.53%	1.273%
19	4.966	1204	1221	1245	rBV2	311705	837024	100.00%	11.039%
20	5.246	1305	1308	1311	rBV2	237	230	0.03%	0.003%
21	5.404	1354	1357	1360	rBV2	377	280	0.03%	0.004%
22	5.542	1388	1400	1432	rBV	283579	584680	69.85%	7.711%
23	5.847	1484	1495	1515	rVB7	12888	28348	3.39%	0.374%
24	5.995	1528	1541	1567	rBV	195097	405350	48.43%	5.346%
25	6.359	1648	1654	1658	rBV2	344	342	0.04%	0.005%
26	6.523	1702	1705	1707	rBV	169	121	0.01%	0.002%
27	6.812	1792	1795	1799	rVB2	331	193	0.02%	0.003%
28	6.860	1807	1810	1812	rBV	164	115	0.01%	0.002%
29	6.921	1818	1829	1853	rBV	92383	176595	21.10%	2.329%
30	7.124	1890	1892	1896	rBV3	441	312	0.04%	0.004%
31	7.166	1903	1905	1908	rVB2	266	133	0.02%	0.002%
32	7.249	1920	1931	1952	rBV	323690	572591	68.41%	7.551%
33	7.558	2018	2027	2049	rBV	71787	128202	15.32%	1.691%
34	7.773	2091	2094	2097	rVB	393	232	0.03%	0.003%
35	7.789	2097	2099	2104	rBV	245	219	0.03%	0.003%
36	7.915	2119	2138	2157	rVB3	37818	74893	8.95%	0.988%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031578.D
 Acq On : 16 Jun 2023 15:56
 Operator : SY/MD
 Sample : 03249-08DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	8.030	2165	2174	2205	rBV	214782	388898	46.46%	5.129%
38	8.220	2229	2233	2241	rBV5	1855	2603	0.31%	0.034%
39	8.455	2303	2306	2307	rBV	257	120	0.01%	0.002%
40	8.497	2314	2319	2326	rBV2	449	550	0.07%	0.007%
41	8.555	2335	2337	2342	rBV2	286	169	0.02%	0.002%
42	8.629	2355	2360	2364	rBV	397	379	0.05%	0.005%
43	8.661	2369	2370	2373	rBV	124	63	0.01%	0.001%
44	8.683	2373	2377	2380	rBV2	247	234	0.03%	0.003%
45	8.789	2399	2410	2441	rBV	435811	722098	86.27%	9.523%
46	9.030	2483	2485	2487	rBV	242	87	0.01%	0.001%
47	9.075	2495	2499	2502	rBV3	523	511	0.06%	0.007%
48	9.178	2529	2531	2534	rBV	170	73	0.01%	0.001%
49	9.230	2544	2547	2549	rBV3	392	273	0.03%	0.004%
50	9.342	2580	2582	2585	rBV2	265	151	0.02%	0.002%
51	9.487	2625	2627	2634	rVB3	711	591	0.07%	0.008%
52	9.645	2670	2676	2684	rVB5	1773	2467	0.29%	0.033%
53	9.818	2728	2730	2732	rBV	163	90	0.01%	0.001%
54	9.879	2742	2749	2759	rBV4	1009	1633	0.20%	0.022%
55	9.953	2768	2772	2774	rBV2	380	339	0.04%	0.004%
56	10.008	2784	2789	2793	rVB3	291	350	0.04%	0.005%
57	10.072	2805	2809	2816	rVB5	821	713	0.09%	0.009%
58	10.159	2825	2836	2859	rVB	303044	474333	56.67%	6.255%
59	10.301	2873	2880	2883	rBV3	2171	2736	0.33%	0.036%
60	10.487	2926	2938	2946	rBV5	4240	6915	0.83%	0.091%
61	10.612	2974	2977	2979	rBV	210	163	0.02%	0.002%
62	10.683	2990	2999	3008	rBV3	11365	16300	1.95%	0.215%
63	10.812	3037	3039	3042	rBV2	285	119	0.01%	0.002%
64	10.860	3046	3054	3066	rVB2	6463	9028	1.08%	0.119%
65	11.005	3094	3099	3102	rBV3	646	644	0.08%	0.008%
66	11.095	3125	3127	3134	rBV2	208	292	0.03%	0.004%
67	11.140	3134	3141	3146	rBV3	2027	2556	0.31%	0.034%
68	11.191	3146	3157	3177	rBV	452800	701857	83.85%	9.256%
69	11.368	3209	3212	3215	rBV2	321	207	0.02%	0.003%
70	11.477	3238	3246	3254	rBV9	3823	8164	0.98%	0.108%
71	11.567	3263	3274	3294	rVB	412977	639828	76.44%	8.438%
72	11.680	3306	3309	3310	rBV3	644	401	0.05%	0.005%
73	11.767	3327	3336	3344	rBV3	4146	5766	0.69%	0.076%
74	11.825	3351	3354	3356	rBV2	342	274	0.03%	0.004%
75	11.857	3359	3364	3365	rBV3	2589	1941	0.23%	0.026%
76	12.146	3453	3454	3456	rBV	151	61	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031578.D
 Acq On : 16 Jun 2023 15:56
 Operator : SY/MD
 Sample : 03249-08DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

77	12.201	3463	3471	3479	rBV5	2063	3345	0.40%	0.044%
78	12.323	3507	3509	3513	rBV2	288	165	0.02%	0.002%
79	12.413	3529	3537	3545	rVB3	3580	4558	0.54%	0.060%
80	12.632	3603	3605	3608	rVB2	408	171	0.02%	0.002%
81	12.828	3659	3666	3674	rVB5	4380	5688	0.68%	0.075%
82	12.988	3711	3716	3721	rBV4	1307	1336	0.16%	0.018%
83	13.217	3782	3787	3789	rBV6	794	807	0.10%	0.011%
84	13.448	3854	3859	3869	rVB5	1985	2836	0.34%	0.037%
85	14.069	4048	4052	4054	rBV	471	316	0.04%	0.004%




Sum of corrected areas: 7582679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031578.D
Acq On : 16 Jun 2023 15:56
Operator : SY/MD
Sample : 03249-08DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

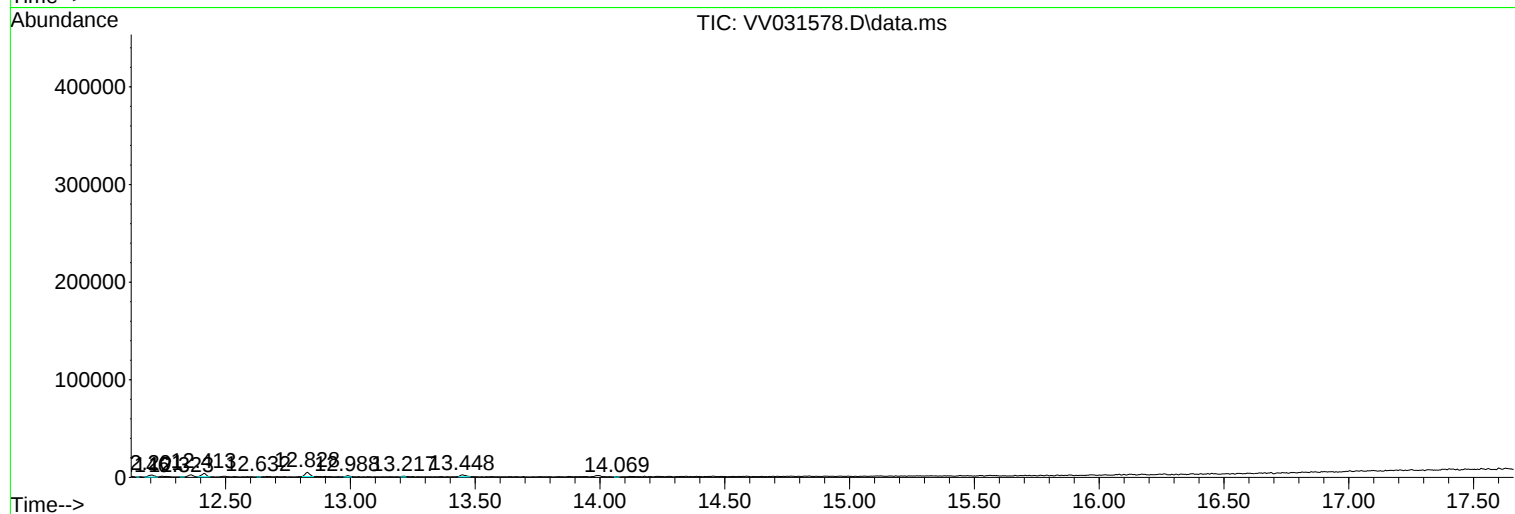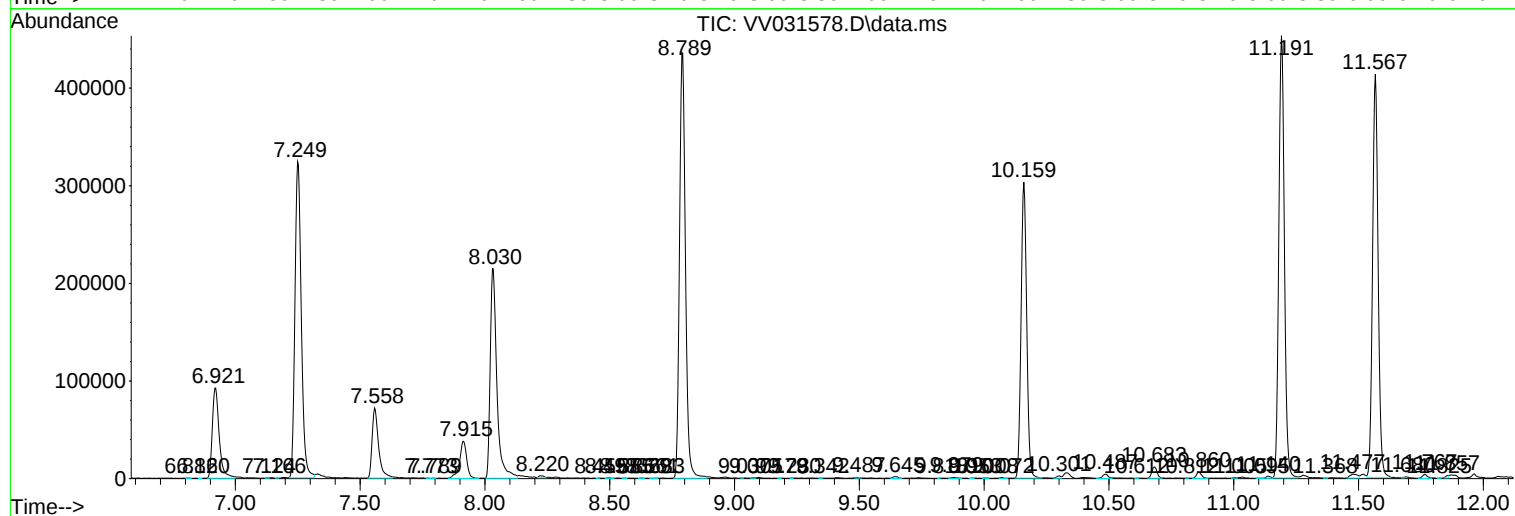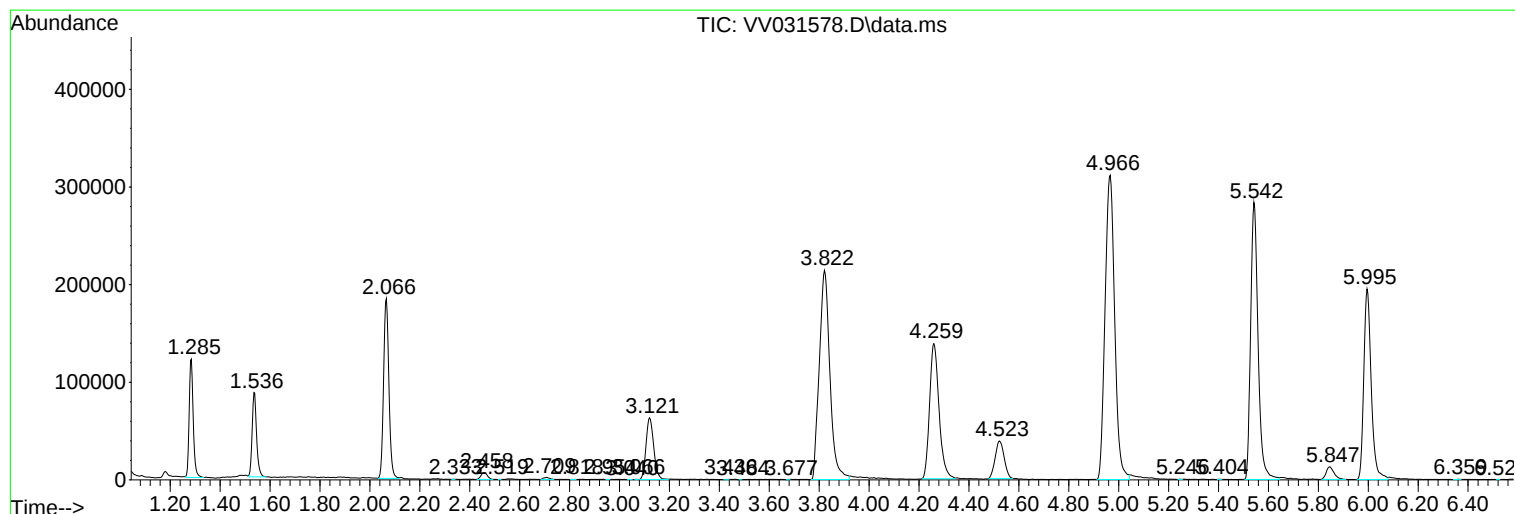

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031578.D
Acq On : 16 Jun 2023 15:56
Operator : SY/MD
Sample : 03249-08DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031578.D
Acq On : 16 Jun 2023 15:56
Operator : SY/MD
Sample : 03249-08DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------