

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031581.D
 Acq On : 16 Jun 2023 17:27
 Operator : SY/MD
 Sample : 03249-13DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rVB	82747	89652	11.12%	1.213%
2	1.535	148	154	170	rVB	78244	94406	11.71%	1.277%
3	2.066	309	319	334	rBV	167152	246418	30.58%	3.333%
4	2.458	432	441	454	rVB3	7494	12283	1.52%	0.166%
5	2.561	468	473	477	rBV3	651	753	0.09%	0.010%
6	2.677	505	509	511	rBV	251	202	0.03%	0.003%
7	2.706	511	518	531	rVB4	2176	3962	0.49%	0.054%
8	2.892	573	576	577	rBV4	237	111	0.01%	0.002%
9	3.021	614	616	618	rBV	294	201	0.02%	0.003%
10	3.121	632	647	672	rBV	110644	230961	28.66%	3.124%
11	3.301	697	703	705	rBV3	444	499	0.06%	0.007%
12	3.362	719	722	724	rBV	339	203	0.03%	0.003%
13	3.400	732	734	735	rBV	136	32	0.00%	0.000%
14	3.490	757	762	765	rBV2	291	311	0.04%	0.004%
15	3.532	771	775	776	rBV2	305	199	0.02%	0.003%
16	3.757	844	845	846	rBV2	160	51	0.01%	0.001%
17	3.822	849	865	900	rBV2	196199	590853	73.31%	7.992%
18	4.259	985	1001	1032	rBV	135904	364285	45.20%	4.927%
19	4.522	1068	1083	1103	rVB2	101208	259507	32.20%	3.510%
20	4.725	1144	1146	1150	rBV4	421	323	0.04%	0.004%
21	4.838	1178	1181	1184	rBV	174	105	0.01%	0.001%
22	4.966	1204	1221	1247	rBV2	300699	805914	100.00%	10.901%
23	5.301	1320	1325	1327	rBV2	268	263	0.03%	0.004%
24	5.429	1363	1365	1367	rBV2	134	64	0.01%	0.001%
25	5.542	1387	1400	1429	rBV2	269338	560282	69.52%	7.579%
26	5.844	1484	1494	1495	rBV5	2172	2641	0.33%	0.036%
27	5.995	1528	1541	1573	rBV	188500	396270	49.17%	5.360%
28	6.175	1595	1597	1598	rBV	339	112	0.01%	0.002%
29	6.288	1629	1632	1634	rBV2	322	188	0.02%	0.003%
30	6.519	1702	1704	1705	rBV2	153	68	0.01%	0.001%
31	6.587	1722	1725	1730	rBV4	454	507	0.06%	0.007%
32	6.651	1744	1745	1750	rVB	289	123	0.02%	0.002%
33	6.677	1750	1753	1756	rVB2	270	152	0.02%	0.002%
34	6.702	1756	1761	1764	rBV2	350	308	0.04%	0.004%
35	6.767	1779	1781	1788	rVB2	346	234	0.03%	0.003%
36	6.799	1788	1791	1795	rBV	219	246	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031581.D
 Acq On : 16 Jun 2023 17:27
 Operator : SY/MD
 Sample : 03249-13DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.918	1818	1828	1845	rBV	93359	171351	21.26%	2.318%
38	7.101	1881	1885	1890	rBV3	381	345	0.04%	0.005%
39	7.120	1890	1891	1893	rVB2	306	89	0.01%	0.001%
40	7.140	1893	1897	1899	rBV	579	338	0.04%	0.005%
41	7.252	1920	1932	1965	rBV	314759	569365	70.65%	7.701%
42	7.558	2018	2027	2055	rBV2	72439	127588	15.83%	1.726%
43	7.718	2075	2077	2080	rVB2	320	168	0.02%	0.002%
44	7.738	2080	2083	2084	rBV	259	146	0.02%	0.002%
45	8.030	2165	2174	2212	rBV	216769	395715	49.10%	5.353%
46	8.403	2288	2290	2295	rVB2	299	230	0.03%	0.003%
47	8.506	2319	2322	2324	rVB	199	90	0.01%	0.001%
48	8.526	2324	2328	2332	rBV2	509	437	0.05%	0.006%
49	8.645	2361	2365	2369	rBV2	405	424	0.05%	0.006%
50	8.792	2397	2411	2430	rBV	421190	689745	85.59%	9.330%
51	9.088	2497	2503	2505	rBV2	451	444	0.06%	0.006%
52	9.239	2548	2550	2552	rBV	169	99	0.01%	0.001%
53	9.384	2594	2595	2597	rBV	242	77	0.01%	0.001%
54	9.532	2639	2641	2646	rVB2	332	163	0.02%	0.002%
55	9.596	2659	2661	2666	rVB2	196	136	0.02%	0.002%
56	9.625	2667	2670	2672	rBV	215	126	0.02%	0.002%
57	9.683	2685	2688	2690	rBV2	315	216	0.03%	0.003%
58	9.767	2711	2714	2717	rBV	318	203	0.03%	0.003%
59	9.902	2755	2756	2757	rBV	203	47	0.01%	0.001%
60	9.998	2781	2786	2789	rBV2	327	329	0.04%	0.004%
61	10.159	2824	2836	2857	rBV	303150	477051	59.19%	6.453%
62	10.429	2915	2920	2925	rVB3	303	332	0.04%	0.004%
63	10.448	2925	2926	2927	rBV3	126	31	0.00%	0.000%
64	10.580	2964	2967	2971	rBV2	204	176	0.02%	0.002%
65	10.635	2980	2984	2987	rBV2	311	233	0.03%	0.003%
66	10.805	3035	3037	3038	rBV2	200	93	0.01%	0.001%
67	10.860	3050	3054	3055	rBV3	678	541	0.07%	0.007%
68	11.107	3129	3131	3134	rBV2	212	108	0.01%	0.001%
69	11.191	3145	3157	3179	rBV	434062	660661	81.98%	8.936%
70	11.349	3204	3206	3210	rBV	398	277	0.03%	0.004%
71	11.567	3262	3274	3295	rBV	392724	617703	76.65%	8.355%
72	11.995	3404	3407	3412	rBV2	399	437	0.05%	0.006%
73	12.050	3417	3424	3432	rVB3	445	825	0.10%	0.011%
74	12.082	3432	3434	3436	rBV	246	152	0.02%	0.002%
75	12.095	3436	3438	3439	rBV	194	60	0.01%	0.001%
76	12.130	3446	3449	3450	rBV	212	127	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031581.D
 Acq On : 16 Jun 2023 17:27
 Operator : SY/MD
 Sample : 03249-13DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.156	3454	3457	3462	rBV	283	267	0.03%	0.004%
78	12.583	3587	3590	3591	rBV	474	274	0.03%	0.004%
79	12.760	3642	3645	3649	rBV	227	186	0.02%	0.003%
80	13.207	3779	3784	3793	rBV5	1586	2286	0.28%	0.031%
81	13.255	3796	3799	3801	rBV	396	217	0.03%	0.003%
82	13.451	3853	3860	3871	rVB3	3889	5975	0.74%	0.081%
83	13.586	3898	3902	3903	rBV2	395	277	0.03%	0.004%
84	13.689	3927	3934	3943	rBV5	2313	3621	0.45%	0.049%
85	13.789	3962	3965	3967	rBV5	304	184	0.02%	0.002%
86	13.892	3994	3997	3999	rBV3	452	327	0.04%	0.004%




Sum of corrected areas: 7392981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031581.D
Acq On : 16 Jun 2023 17:27
Operator : SY/MD
Sample : 03249-13DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

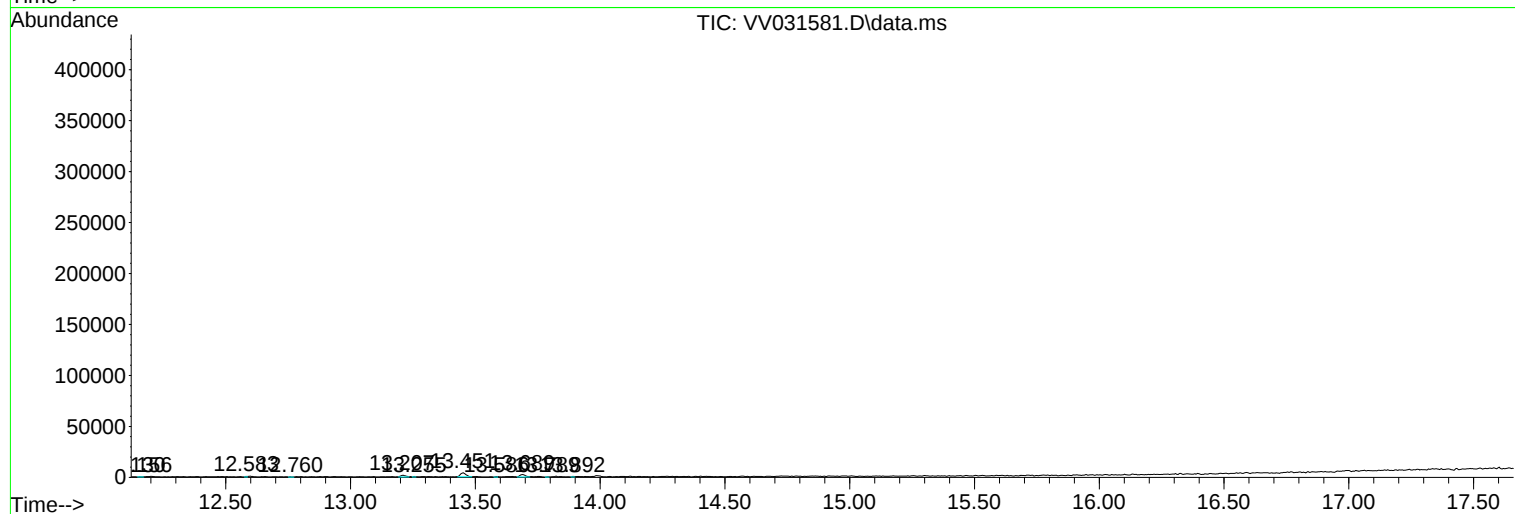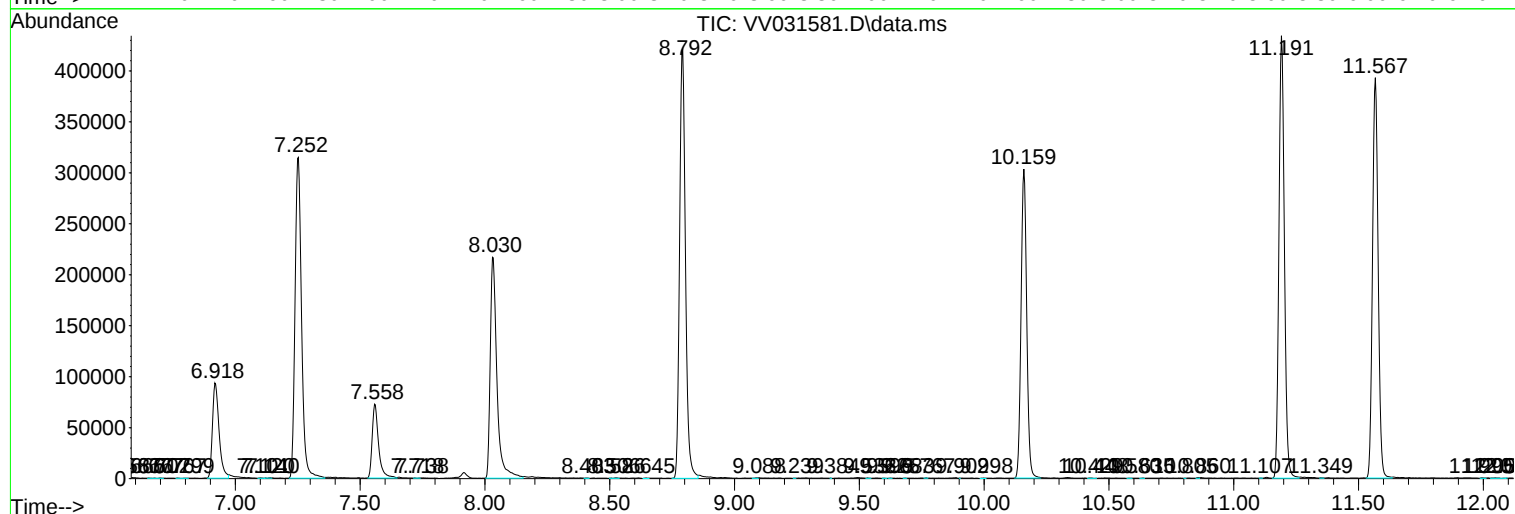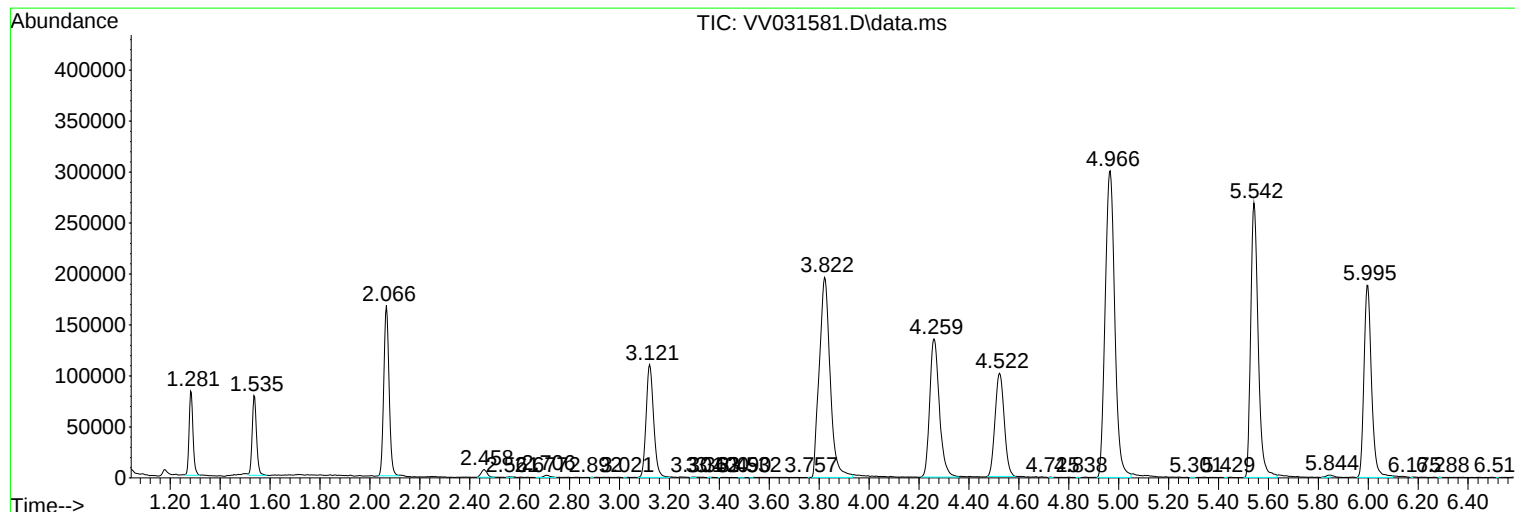

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031581.D
Acq On : 16 Jun 2023 17:27
Operator : SY/MD
Sample : 03249-13DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031581.D
Acq On : 16 Jun 2023 17:27
Operator : SY/MD
Sample : 03249-13DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------