

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031582.D
 Acq On : 16 Jun 2023 17:50
 Operator : SY/MD
 Sample : 03249-16DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	94	rVB	76343	83508	10.42%	1.146%
2	1.536	147	154	166	rBV	74416	89766	11.20%	1.232%
3	2.066	309	319	333	rBV2	164078	245742	30.66%	3.372%
4	2.458	432	441	451	rBV2	8507	13973	1.74%	0.192%
5	2.648	496	500	504	rBV2	320	350	0.04%	0.005%
6	2.796	542	546	547	rBV	387	262	0.03%	0.004%
7	2.815	550	552	554	rVB	118	42	0.01%	0.001%
8	2.921	583	585	588	rBV	256	123	0.02%	0.002%
9	2.960	594	597	599	rBV	309	192	0.02%	0.003%
10	3.018	612	615	619	rBV2	224	198	0.02%	0.003%
11	3.121	636	647	666	rVB2	9561	19331	2.41%	0.265%
12	3.275	692	695	696	rBV	201	117	0.01%	0.002%
13	3.288	696	699	701	rVB	193	120	0.01%	0.002%
14	3.420	737	740	744	rVB2	334	254	0.03%	0.003%
15	3.445	744	748	750	rBV	184	137	0.02%	0.002%
16	3.503	763	766	769	rBV	235	195	0.02%	0.003%
17	3.622	800	803	805	rBV	143	121	0.02%	0.002%
18	3.667	814	817	819	rBV3	385	277	0.03%	0.004%
19	3.738	838	839	842	rBV3	211	109	0.01%	0.001%
20	3.802	848	859	900	rBV	62709	195451	24.39%	2.682%
21	4.262	987	1002	1028	rBV2	134800	354553	44.24%	4.865%
22	4.523	1065	1083	1105	rBV	211561	542783	67.72%	7.448%
23	4.847	1177	1184	1186	rBV2	210	259	0.03%	0.004%
24	4.963	1203	1220	1250	rBV2	299349	801491	100.00%	10.998%
25	5.542	1388	1400	1426	rBV	274192	563913	70.36%	7.738%
26	5.847	1483	1495	1513	rBV4	28750	60849	7.59%	0.835%
27	5.995	1528	1541	1566	rBV	188144	391721	48.87%	5.375%
28	6.256	1621	1622	1625	rBV	154	49	0.01%	0.001%
29	6.420	1671	1673	1676	rVB2	162	69	0.01%	0.001%
30	6.439	1676	1679	1680	rBV	258	158	0.02%	0.002%
31	6.526	1705	1706	1709	rBV	150	65	0.01%	0.001%
32	6.638	1739	1741	1743	rBV	206	97	0.01%	0.001%
33	6.921	1818	1829	1851	rBV	90211	167470	20.89%	2.298%
34	7.124	1888	1892	1895	rBV2	441	387	0.05%	0.005%
35	7.249	1919	1931	1955	rBV	316946	560046	69.88%	7.685%
36	7.558	2017	2027	2055	rBV	69587	127552	15.91%	1.750%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031582.D
 Acq On : 16 Jun 2023 17:50
 Operator : SY/MD
 Sample : 03249-16DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.722	2076	2078	2083	rVB2	296	208	0.03%	0.003%
38	7.776	2092	2095	2096	rBV	322	159	0.02%	0.002%
39	7.911	2127	2137	2160	rVB2	132706	230430	28.75%	3.162%
40	8.030	2165	2174	2203	rBV	213375	383911	47.90%	5.268%
41	8.448	2301	2304	2307	rVB2	296	165	0.02%	0.002%
42	8.468	2307	2310	2311	rBV	167	91	0.01%	0.001%
43	8.645	2361	2365	2366	rBV	181	118	0.01%	0.002%
44	8.792	2399	2411	2433	rBV	428102	695218	86.74%	9.540%
45	9.317	2572	2574	2576	rBV	222	134	0.02%	0.002%
46	9.481	2622	2625	2628	rBV	271	250	0.03%	0.003%
47	9.590	2657	2659	2660	rBV	156	61	0.01%	0.001%
48	9.706	2691	2695	2698	rVB3	443	416	0.05%	0.006%
49	9.741	2698	2706	2709	rBV3	425	575	0.07%	0.008%
50	9.789	2719	2721	2722	rBV	170	94	0.01%	0.001%
51	9.899	2754	2755	2756	rVB	219	42	0.01%	0.001%
52	10.159	2824	2836	2858	rBV	301662	469542	58.58%	6.443%
53	10.333	2884	2890	2897	rVB6	2460	3114	0.39%	0.043%
54	10.480	2932	2936	2939	rBV3	610	485	0.06%	0.007%
55	10.593	2968	2971	2974	rBV3	227	142	0.02%	0.002%
56	11.072	3118	3120	3121	rBV3	210	75	0.01%	0.001%
57	11.191	3146	3157	3181	rBV	427302	664368	82.89%	9.117%
58	11.567	3261	3274	3294	rBV	396765	612783	76.46%	8.409%
59	11.725	3320	3323	3332	rBV3	409	480	0.06%	0.007%
60	12.210	3465	3474	3478	rVB3	962	1432	0.18%	0.020%
61	12.287	3495	3498	3504	rVB2	401	352	0.04%	0.005%
62	13.522	3879	3882	3885	rBV3	335	197	0.02%	0.003%
63	13.545	3887	3889	3892	rVV2	378	160	0.02%	0.002%
64	14.377	4146	4148	4150	rBV2	432	266	0.03%	0.004%
65	14.480	4179	4180	4181	rBV2	235	84	0.01%	0.001%
66	14.644	4228	4231	4234	rVB2	478	283	0.04%	0.004%




Sum of corrected areas: 7287365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031582.D
Acq On : 16 Jun 2023 17:50
Operator : SY/MD
Sample : 03249-16DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

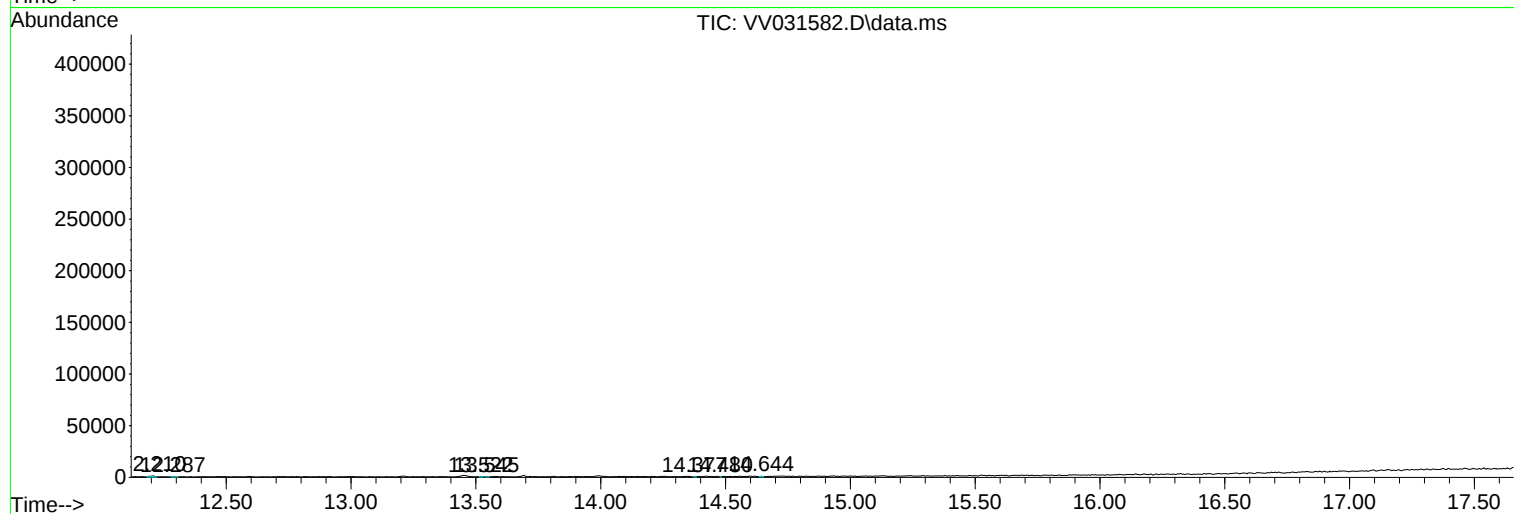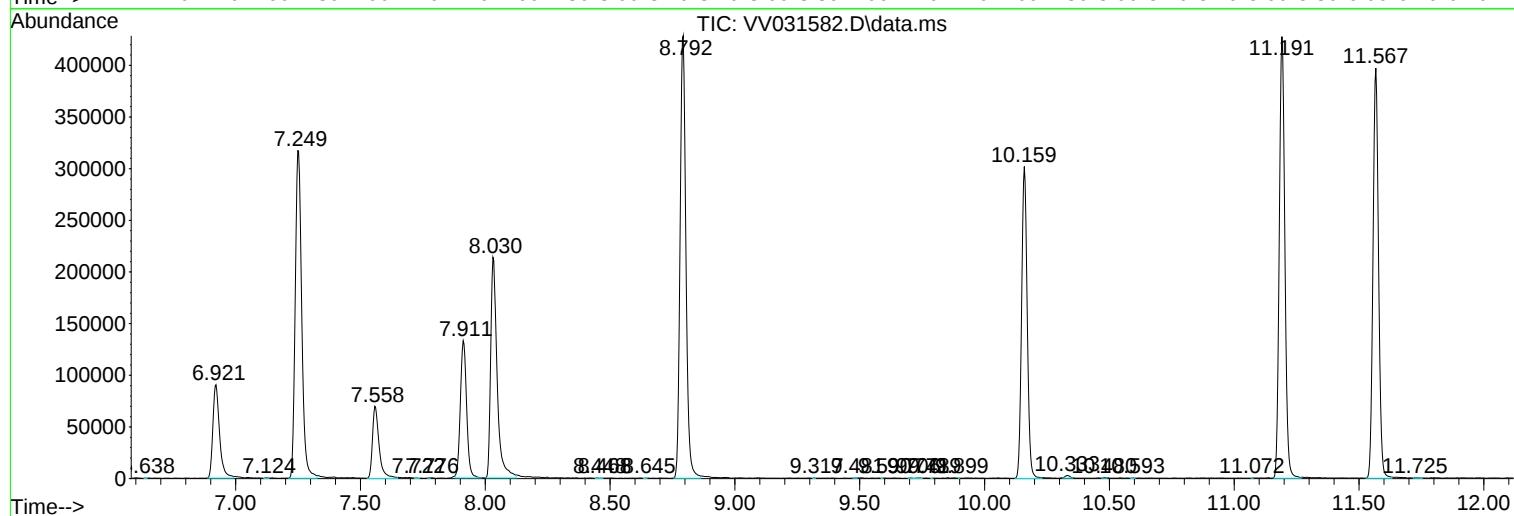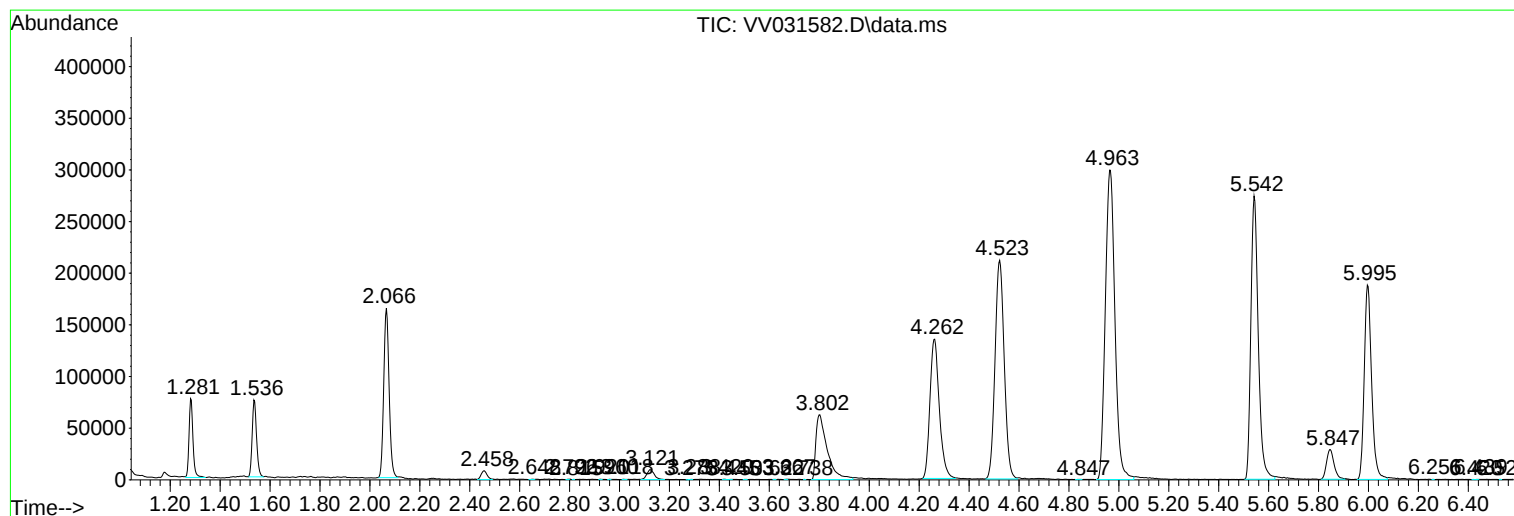

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031582.D
Acq On : 16 Jun 2023 17:50
Operator : SY/MD
Sample : 03249-16DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031582.D
Acq On : 16 Jun 2023 17:50
Operator : SY/MD
Sample : 03249-16DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc