

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031583.D
 Acq On : 16 Jun 2023 18:13
 Operator : SY/MD
 Sample : 03249-17DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	86	rVB2	100073	106463	13.50%	1.510%
2	1.539	148	155	156	rBV	81066	71619	9.08%	1.016%
3	2.066	310	319	334	rVB	154513	224041	28.40%	3.177%
4	2.455	432	440	453	rVB3	9031	14694	1.86%	0.208%
5	2.568	471	475	478	rVB	457	358	0.05%	0.005%
6	2.587	478	481	483	rBV2	255	154	0.02%	0.002%
7	2.703	511	517	529	rBV2	2699	5234	0.66%	0.074%
8	2.770	533	538	543	rVB3	331	379	0.05%	0.005%
9	2.854	559	564	569	rBV3	209	276	0.03%	0.004%
10	3.121	633	647	669	rBV	148528	310299	39.33%	4.400%
11	3.246	682	686	687	rBV	241	161	0.02%	0.002%
12	3.432	741	744	745	rBV2	178	102	0.01%	0.001%
13	3.516	767	770	772	rBV2	207	147	0.02%	0.002%
14	3.532	772	775	777	rVV	123	97	0.01%	0.001%
15	3.619	797	802	804	rBV2	445	357	0.05%	0.005%
16	3.683	820	822	827	rVB2	178	131	0.02%	0.002%
17	3.712	827	831	833	rBV	151	104	0.01%	0.001%
18	3.731	833	837	840	rBV2	234	219	0.03%	0.003%
19	3.760	844	846	849	rBV2	215	176	0.02%	0.002%
20	3.822	849	865	891	rBV2	131509	416549	52.80%	5.907%
21	4.259	985	1001	1032	rBV2	131031	349656	44.32%	4.958%
22	4.522	1068	1083	1112	rVB	63652	163517	20.73%	2.319%
23	4.680	1130	1132	1135	rVB2	395	217	0.03%	0.003%
24	4.696	1135	1137	1140	rVB2	258	94	0.01%	0.001%
25	4.815	1172	1174	1179	rVB	176	84	0.01%	0.001%
26	4.838	1179	1181	1183	rBV	254	126	0.02%	0.002%
27	4.966	1204	1221	1254	rBV2	295773	788897	100.00%	11.187%
28	5.378	1346	1349	1352	rBV2	172	131	0.02%	0.002%
29	5.493	1383	1385	1387	rBV2	222	104	0.01%	0.001%
30	5.542	1388	1400	1425	rBV	270330	552084	69.98%	7.829%
31	5.931	1517	1521	1522	rBV	215	163	0.02%	0.002%
32	5.995	1527	1541	1563	rBV	183926	383492	48.61%	5.438%
33	6.172	1592	1596	1597	rBV3	390	245	0.03%	0.003%
34	6.223	1609	1612	1622	rBV3	438	555	0.07%	0.008%
35	6.513	1699	1702	1703	rBV3	222	118	0.01%	0.002%
36	6.558	1713	1716	1721	rBV2	196	192	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031583.D
 Acq On : 16 Jun 2023 18:13
 Operator : SY/MD
 Sample : 03249-17DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.612	1732	1733	1737	rVB	354	176	0.02%	0.002%
38	6.632	1737	1739	1743	rVB2	290	202	0.03%	0.003%
39	6.651	1743	1745	1746	rBV	304	157	0.02%	0.002%
40	6.866	1805	1812	1815	rBV2	315	396	0.05%	0.006%
41	6.921	1817	1829	1850	rBV	91415	169104	21.44%	2.398%
42	7.252	1920	1932	1949	rBV	309182	542910	68.82%	7.699%
43	7.558	2018	2027	2042	rBV	67284	119176	15.11%	1.690%
44	7.825	2107	2110	2113	rBV2	292	148	0.02%	0.002%
45	7.882	2118	2128	2130	rBV4	1829	2311	0.29%	0.033%
46	7.972	2152	2156	2160	rBV3	255	246	0.03%	0.003%
47	8.034	2165	2175	2211	rBV	203491	375973	47.66%	5.331%
48	8.246	2239	2241	2246	rBV4	533	488	0.06%	0.007%
49	8.435	2296	2300	2302	rBV	352	325	0.04%	0.005%
50	8.484	2314	2315	2316	rBV	208	48	0.01%	0.001%
51	8.545	2332	2334	2337	rBV	286	142	0.02%	0.002%
52	8.564	2337	2340	2342	rBV	270	170	0.02%	0.002%
53	8.587	2345	2347	2348	rBV	315	131	0.02%	0.002%
54	8.667	2371	2372	2376	rBV2	229	134	0.02%	0.002%
55	8.712	2384	2386	2388	rBV2	199	103	0.01%	0.001%
56	8.792	2399	2411	2436	rBV	411958	682612	86.53%	9.680%
57	8.956	2455	2462	2477	rVB2	4167	7077	0.90%	0.100%
58	9.014	2477	2480	2483	rBV2	464	219	0.03%	0.003%
59	9.046	2485	2490	2493	rBV3	537	391	0.05%	0.006%
60	9.091	2495	2504	2512	rVB4	3518	5697	0.72%	0.081%
61	9.387	2593	2596	2598	rBV	356	187	0.02%	0.003%
62	9.487	2619	2627	2637	rBV4	3604	5700	0.72%	0.081%
63	9.545	2642	2645	2646	rBV4	187	123	0.02%	0.002%
64	9.751	2707	2709	2711	rBV2	121	73	0.01%	0.001%
65	9.870	2744	2746	2756	rVB2	818	964	0.12%	0.014%
66	9.963	2772	2775	2777	rBV	241	151	0.02%	0.002%
67	9.992	2780	2784	2791	rVB4	304	367	0.05%	0.005%
68	10.021	2791	2793	2794	rBV4	192	82	0.01%	0.001%
69	10.159	2824	2836	2853	rBV	296956	465227	58.97%	6.597%
70	10.255	2864	2866	2870	rVB2	383	222	0.03%	0.003%
71	10.304	2872	2881	2883	rBV4	1204	1505	0.19%	0.021%
72	10.368	2898	2901	2903	rBV2	255	182	0.02%	0.003%
73	10.394	2903	2909	2910	rBV2	1103	1126	0.14%	0.016%
74	10.763	3021	3024	3028	rBV	236	170	0.02%	0.002%
75	10.808	3035	3038	3042	rVB2	366	254	0.03%	0.004%
76	10.863	3046	3055	3065	rVB2	6794	10147	1.29%	0.144%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031583.D
 Acq On : 16 Jun 2023 18:13
 Operator : SY/MD
 Sample : 03249-17DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	10.911	3065	3070	3072	rBV2	327	276	0.03%	0.004%
78	10.969	3085	3088	3090	rBV2	310	197	0.02%	0.003%
79	11.059	3113	3116	3119	rVB2	332	187	0.02%	0.003%
80	11.088	3120	3125	3128	rBV2	248	211	0.03%	0.003%
81	11.191	3146	3157	3177	rBV	426095	651032	82.52%	9.232%
82	11.567	3263	3274	3293	rBV	390002	608970	77.19%	8.635%
83	12.516	3566	3569	3572	rBV	416	285	0.04%	0.004%
84	12.628	3602	3604	3605	rBV	299	112	0.01%	0.002%
85	12.831	3661	3667	3671	rBV4	1006	1113	0.14%	0.016%
86	13.075	3738	3743	3746	rBV2	410	403	0.05%	0.006%
87	13.210	3780	3785	3790	rBV4	880	876	0.11%	0.012%
88	13.458	3854	3862	3866	rBV3	1456	1850	0.23%	0.026%
89	13.676	3929	3930	3932	rBV	357	175	0.02%	0.002%
90	14.387	4148	4151	4155	rVB3	510	369	0.05%	0.005%




Sum of corrected areas: 7052107

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031583.D
Acq On : 16 Jun 2023 18:13
Operator : SY/MD
Sample : 03249-17DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

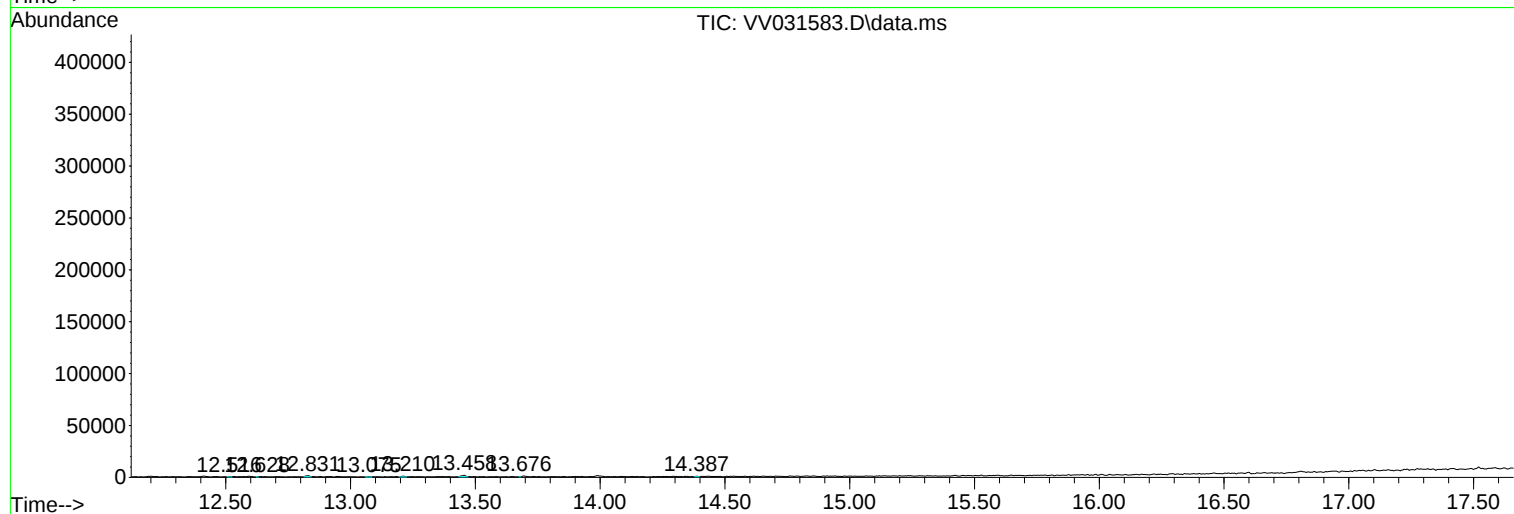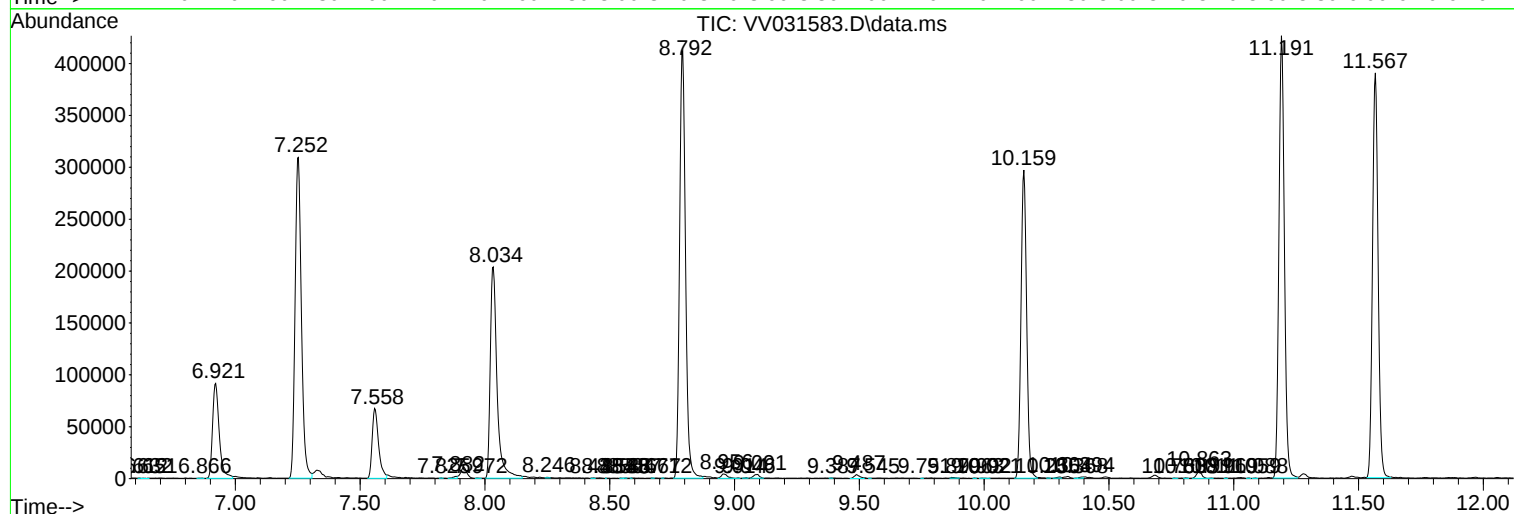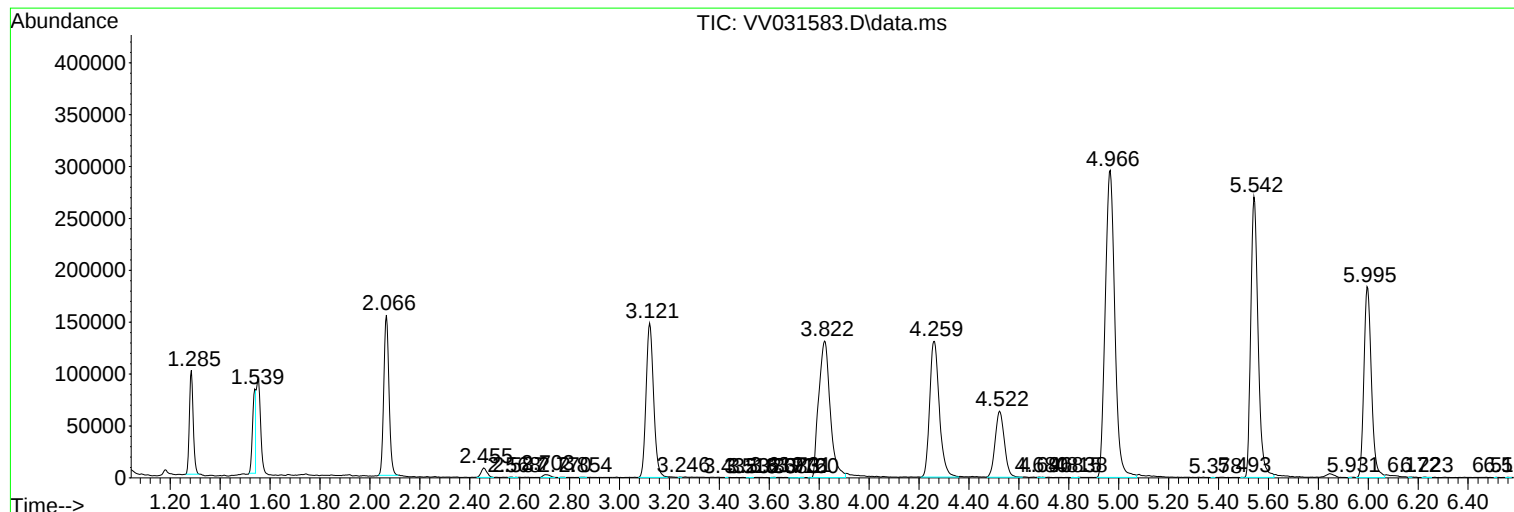

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031583.D
Acq On : 16 Jun 2023 18:13
Operator : SY/MD
Sample : 03249-17DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031583.D
Acq On : 16 Jun 2023 18:13
Operator : SY/MD
Sample : 03249-17DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------