

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031586.D
 Acq On : 16 Jun 2023 19:23
 Operator : SY/MD
 Sample : 03249-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	70834	75761	9.55%	1.031%
2	1.539	148	155	170	rVB	71516	85975	10.84%	1.169%
3	2.066	309	319	333	rBV	153530	226052	28.50%	3.075%
4	2.455	431	440	457	rVB	12223	21199	2.67%	0.288%
5	2.523	457	461	464	rBV2	162	149	0.02%	0.002%
6	2.545	464	468	469	rBV	215	130	0.02%	0.002%
7	2.590	479	482	486	rBV2	226	211	0.03%	0.003%
8	2.709	512	519	526	rBV5	1161	1613	0.20%	0.022%
9	2.806	541	549	551	rBV3	389	488	0.06%	0.007%
10	2.905	575	580	583	rVB	247	250	0.03%	0.003%
11	2.934	583	589	591	rBV2	281	347	0.04%	0.005%
12	3.053	622	626	627	rBV	171	147	0.02%	0.002%
13	3.124	635	648	663	rBV2	15020	30587	3.86%	0.416%
14	3.326	707	711	712	rBV	223	131	0.02%	0.002%
15	3.474	753	757	761	rBV	282	293	0.04%	0.004%
16	3.494	761	763	767	rBV2	248	167	0.02%	0.002%
17	3.603	795	797	802	rVB	354	256	0.03%	0.003%
18	3.683	819	822	827	rBV2	271	250	0.03%	0.003%
19	3.822	848	865	889	rBV3	194536	564036	71.12%	7.672%
20	4.259	984	1001	1028	rBV	130492	353227	44.54%	4.805%
21	4.522	1065	1083	1111	rBV	175948	452468	57.05%	6.155%
22	4.751	1152	1154	1159	rBV2	210	176	0.02%	0.002%
23	4.863	1186	1189	1193	rBV	258	245	0.03%	0.003%
24	4.966	1203	1221	1252	rBV2	294264	793078	100.00%	10.788%
25	5.336	1333	1336	1339	rBV4	291	225	0.03%	0.003%
26	5.387	1351	1352	1356	rBV2	174	131	0.02%	0.002%
27	5.542	1387	1400	1423	rBV	279516	573254	72.28%	7.798%
28	5.738	1459	1461	1464	rBV2	462	235	0.03%	0.003%
29	5.892	1506	1509	1511	rBV	211	117	0.01%	0.002%
30	5.995	1528	1541	1565	rBV	186652	385667	48.63%	5.246%
31	6.278	1625	1629	1634	rBV2	437	433	0.05%	0.006%
32	6.313	1637	1640	1642	rVV	332	163	0.02%	0.002%
33	6.416	1666	1672	1673	rBV3	239	232	0.03%	0.003%
34	6.503	1696	1699	1701	rBV	204	159	0.02%	0.002%
35	6.609	1730	1732	1735	rVB2	262	124	0.02%	0.002%
36	6.699	1757	1760	1763	rVV2	408	292	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061623\
 Data File : VW031586.D
 Acq On : 16 Jun 2023 19:23
 Operator : SY/MD
 Sample : 03249-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.731	1767	1770	1773	rBV	290	283	0.04%	0.004%
38	6.918	1818	1828	1850	rBV	86877	163579	20.63%	2.225%
39	7.249	1920	1931	1949	rBV	312000	545977	68.84%	7.427%
40	7.558	2014	2027	2046	rBV	66312	121426	15.31%	1.652%
41	7.796	2099	2101	2106	rBV2	276	246	0.03%	0.003%
42	7.847	2115	2117	2118	rBV	361	128	0.02%	0.002%
43	7.876	2122	2126	2128	rBV3	1725	1336	0.17%	0.018%
44	7.947	2146	2148	2150	rBV	223	138	0.02%	0.002%
45	7.995	2161	2163	2165	rBV	222	124	0.02%	0.002%
46	8.030	2165	2174	2206	rBV	201625	371534	46.85%	5.054%
47	8.371	2271	2280	2289	rBV4	2396	3738	0.47%	0.051%
48	8.484	2312	2315	2316	rBV	314	131	0.02%	0.002%
49	8.506	2318	2322	2325	rVV3	418	258	0.03%	0.004%
50	8.538	2330	2332	2336	rVB2	348	224	0.03%	0.003%
51	8.558	2336	2338	2341	rBV2	335	179	0.02%	0.002%
52	8.599	2348	2351	2356	rVB2	513	359	0.05%	0.005%
53	8.628	2357	2360	2363	rBV	234	159	0.02%	0.002%
54	8.722	2387	2389	2394	rVB2	253	180	0.02%	0.002%
55	8.792	2398	2411	2437	rBV	433719	713082	89.91%	9.700%
56	9.082	2492	2501	2517	rVV2	10284	16669	2.10%	0.227%
57	9.165	2524	2527	2529	rBV	193	122	0.02%	0.002%
58	9.278	2559	2562	2564	rBV2	199	122	0.02%	0.002%
59	9.487	2621	2627	2635	rBV4	4013	5793	0.73%	0.079%
60	9.609	2661	2665	2668	rBV2	219	164	0.02%	0.002%
61	9.651	2676	2678	2681	rBV2	377	232	0.03%	0.003%
62	9.754	2707	2710	2712	rBV	223	143	0.02%	0.002%
63	9.767	2712	2714	2719	rVB3	338	200	0.03%	0.003%
64	9.831	2731	2734	2737	rBV	177	131	0.02%	0.002%
65	9.882	2740	2750	2760	rVV4	571	1090	0.14%	0.015%
66	10.043	2798	2800	2803	rBV	214	157	0.02%	0.002%
67	10.159	2824	2836	2854	rBV	299772	467693	58.97%	6.362%
68	10.252	2863	2865	2869	rVB	465	210	0.03%	0.003%
69	10.397	2900	2910	2929	rVB2	5696	11312	1.43%	0.154%
70	10.484	2930	2937	2945	rVB2	2951	4140	0.52%	0.056%
71	10.532	2950	2952	2955	rVB2	208	113	0.01%	0.002%
72	10.609	2973	2976	2977	rBV2	262	173	0.02%	0.002%
73	10.683	2995	2999	3008	rVB3	2451	3078	0.39%	0.042%
74	10.812	3034	3039	3042	rBV2	341	404	0.05%	0.005%
75	10.860	3046	3054	3070	rVB2	14100	20335	2.56%	0.277%
76	10.918	3070	3072	3077	rBV	257	274	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
 Data File : VV031586.D
 Acq On : 16 Jun 2023 19:23
 Operator : SY/MD
 Sample : 03249-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.046	3110	3112	3114	rBV	348	189	0.02%	0.003%
78	11.104	3127	3130	3135	rBV2	296	295	0.04%	0.004%
79	11.191	3145	3157	3178	rBV	450887	692871	87.36%	9.425%
80	11.365	3208	3211	3212	rBV	267	153	0.02%	0.002%
81	11.416	3225	3227	3229	rBV	255	179	0.02%	0.002%
82	11.448	3234	3237	3238	rVV	293	147	0.02%	0.002%
83	11.474	3238	3245	3251	rVB5	1149	1787	0.23%	0.024%
84	11.567	3262	3274	3290	rBV	403321	626501	79.00%	8.522%
85	11.969	3394	3399	3403	rVV3	482	530	0.07%	0.007%
86	11.988	3403	3405	3408	rVB2	442	168	0.02%	0.002%
87	12.159	3456	3458	3460	rBV2	313	139	0.02%	0.002%
88	12.644	3606	3609	3611	rBV	261	161	0.02%	0.002%
89	12.683	3617	3621	3627	rBV3	383	366	0.05%	0.005%
90	12.902	3686	3689	3692	rVB2	419	252	0.03%	0.003%
91	12.921	3692	3695	3697	rBV	216	162	0.02%	0.002%
92	13.030	3727	3729	3732	rBV	284	154	0.02%	0.002%
93	13.152	3764	3767	3768	rBV2	251	161	0.02%	0.002%
94	13.255	3796	3799	3802	rBV	383	294	0.04%	0.004%
95	13.644	3917	3920	3926	rVB3	436	336	0.04%	0.005%
96	13.676	3927	3930	3934	rBV2	453	375	0.05%	0.005%
97	13.699	3934	3937	3939	rVB	616	336	0.04%	0.005%
98	13.988	4020	4027	4031	rBV2	1230	1616	0.20%	0.022%
99	14.056	4046	4048	4050	rBV	399	174	0.02%	0.002%
100	14.123	4067	4069	4071	rBV2	421	226	0.03%	0.003%




Sum of corrected areas: 7351476

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031586.D
Acq On : 16 Jun 2023 19:23
Operator : SY/MD
Sample : 03249-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

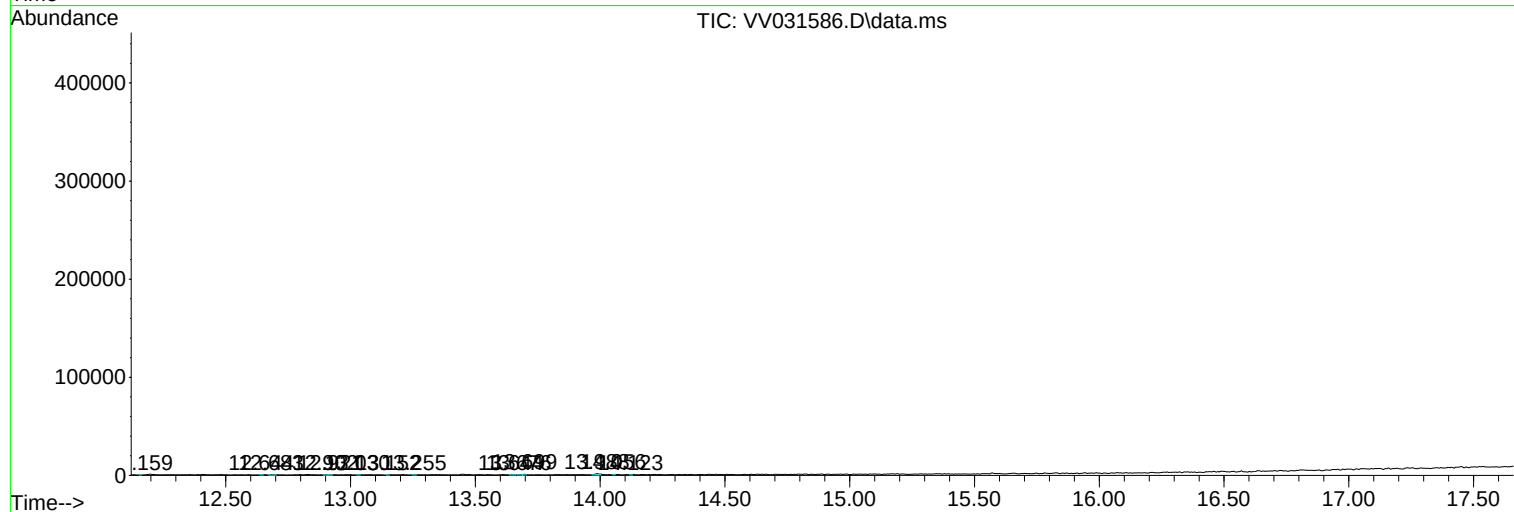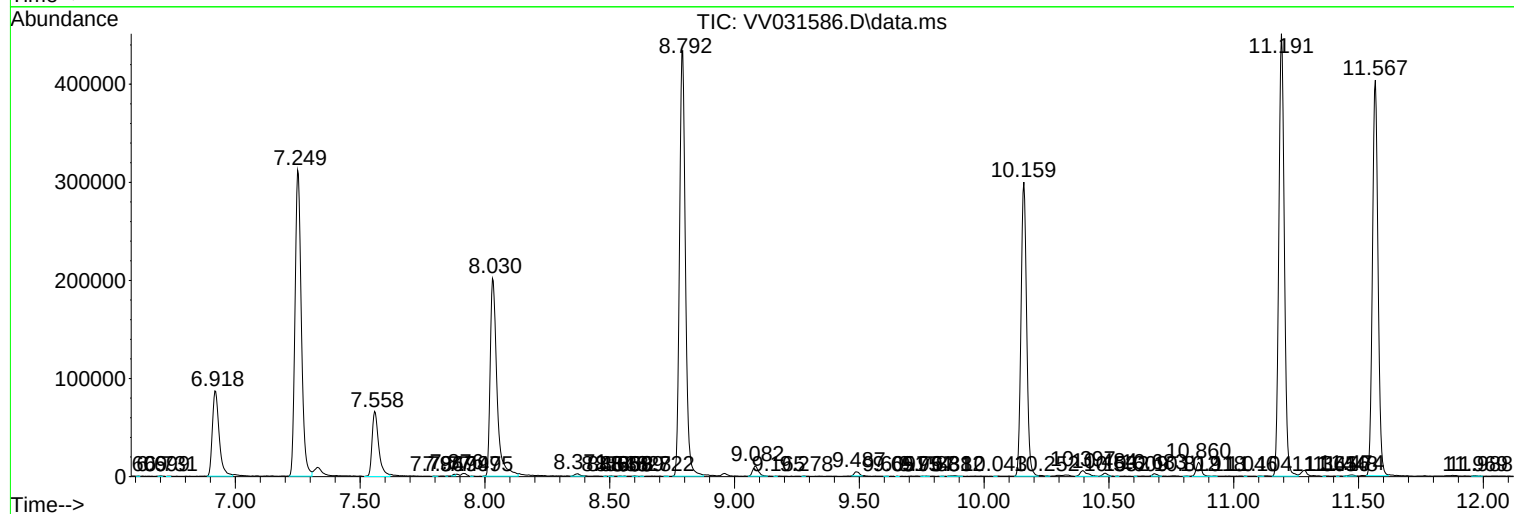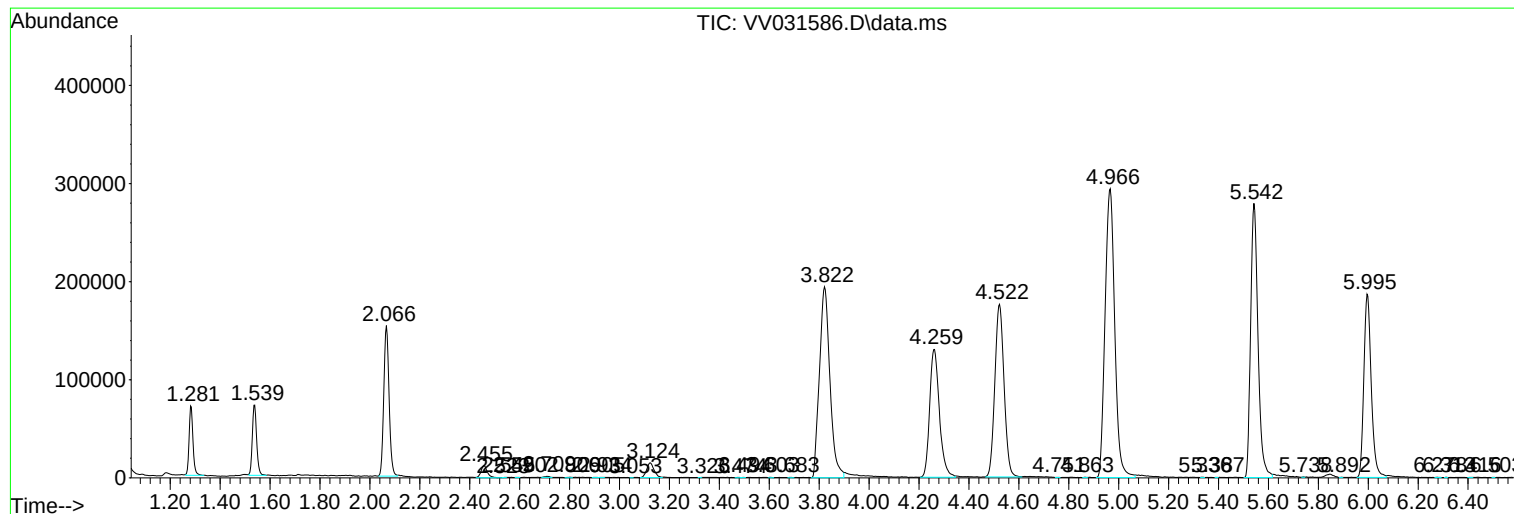

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031586.D
Acq On : 16 Jun 2023 19:23
Operator : SY/MD
Sample : 03249-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031586.D
Acq On : 16 Jun 2023 19:23
Operator : SY/MD
Sample : 03249-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------