


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061623\
Data File : VV031562.D
Acq On : 16 Jun 2023 09:12
Operator : SY/MD
Sample : BFB389
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB389

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Thu Jun 22 02:14:12 2023

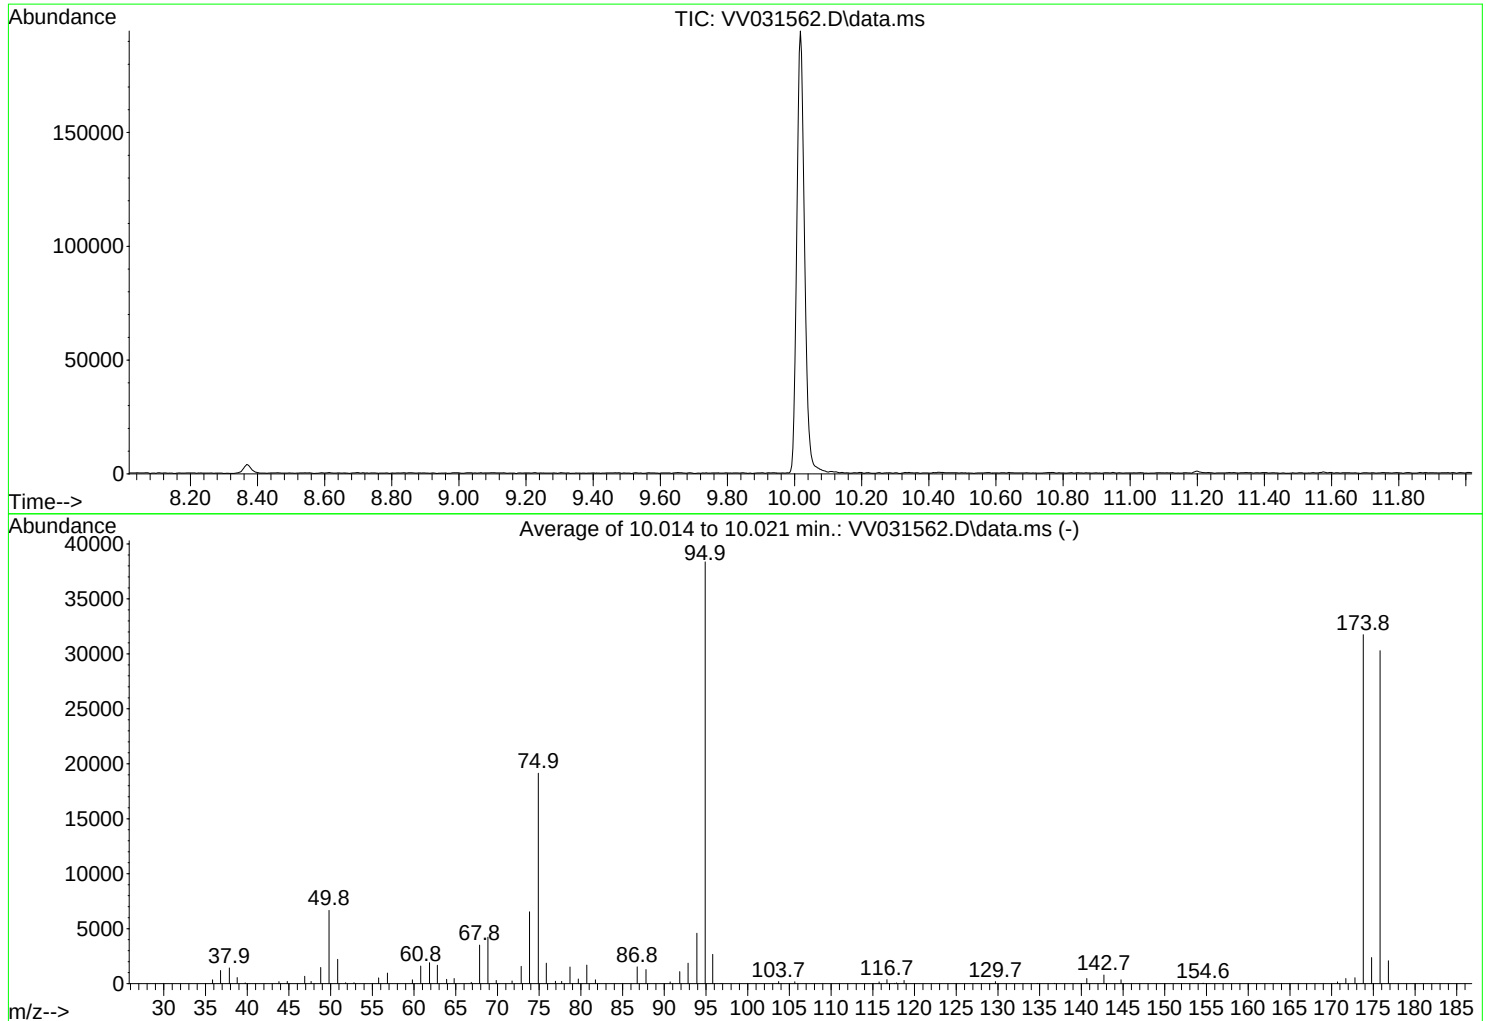

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6674	PASS
75	95	30	80	49.9	19144	PASS
95	95	100	100	100.0	38371	PASS
96	95	5	9	7.0	2668	PASS
173	174	0.00	2	1.7	536	PASS
174	95	50	120	82.7	31749	PASS
175	174	5	9	7.5	2366	PASS
176	174	95	105	95.4	30291	PASS
177	176	5	10	6.9	2083	PASS

m/z	Abundance
39.70	150.0
43.80	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389

m/z	Abundance
35.80	309.0
36.80	1190.0
37.80	1416.0
38.80	584.0
39.80	206.0
43.80	486.0
44.80	194.0
46.90	681.0
47.70	231.0
48.80	1514.0
49.80	6616.0
50.80	2064.0
51.80	158.0
55.70	529.0
56.80	993.0
59.80	310.0
60.80	1629.0
61.80	1909.0
62.80	1702.0
63.90	383.0
64.80	448.0
66.90	108.0
67.80	3367.0
68.90	4339.0
69.80	295.0
71.80	276.0
72.90	1523.0
73.90	6447.0
74.90	19104.0
75.90	2017.0
77.00	230.0
77.70	230.0
78.70	1477.0
79.70	479.0
80.70	1770.0
81.80	362.0
86.70	1619.0
87.80	1212.0
90.70	114.0
91.80	1064.0
92.90	1657.0
93.90	4682.0
94.90	37792.0
95.80	2682.0
96.80	107.0
103.70	196.0
105.60	166.0
115.70	157.0
116.70	361.0
118.70	275.0
129.70	172.0
140.60	460.0
142.70	782.0
144.70	341.0
170.70	137.0
171.70	333.0
172.80	523.0
173.80	30912.0
174.80	2446.0
175.80	29272.0
176.80	2059.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389

m/z	Abundance
35.90	342.0
36.80	1237.0
37.90	1510.0
38.80	561.0
39.80	253.0
43.80	524.0
44.80	196.0
46.90	737.0
47.70	211.0
48.80	1511.0
49.80	6929.0
50.90	2271.0
51.80	105.0
52.80	106.0
55.70	556.0
56.80	1008.0
59.80	379.0
60.80	1648.0
61.90	1941.0
62.80	1721.0
63.90	409.0
64.80	483.0
66.90	136.0
67.80	3606.0
68.90	4389.0
69.90	304.0
71.80	260.0
72.80	1617.0
73.80	6707.0
74.90	19808.0
75.90	1921.0
76.90	231.0
77.70	224.0
78.70	1553.0
79.70	442.0
80.70	1777.0
81.70	374.0
86.80	1534.0
87.80	1344.0
90.70	173.0
91.80	1117.0
92.80	1919.0
93.90	4679.0
94.90	39696.0
95.80	2796.0
103.70	195.0
105.70	187.0
115.80	159.0
116.70	371.0
117.60	105.0
117.80	105.0
118.80	288.0
129.70	194.0
134.70	111.0
136.80	107.0
140.60	479.0
142.70	815.0
144.70	374.0
170.70	172.0
171.70	464.0
172.80	548.0
173.80	32800.0
174.80	2419.0
175.80	31304.0
176.80	2145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389

m/z	Abundance
35.90	382.0
36.80	1144.0
37.90	1354.0
38.80	538.0
39.80	226.0
43.80	521.0
44.80	206.0
46.90	607.0
47.60	177.0
48.80	1392.0
49.80	6477.0
50.90	2286.0
52.80	177.0
55.80	474.0
56.80	873.0
59.80	353.0
60.80	1525.0
61.80	1876.0
62.80	1610.0
63.90	379.0
64.80	478.0
66.80	121.0
67.90	3564.0
68.80	3957.0
69.90	294.0
71.70	195.0
72.80	1594.0
73.80	6447.0
74.90	18520.0
75.80	1643.0
76.90	215.0
77.70	159.0
78.70	1497.0
79.70	361.0
80.70	1532.0
81.70	336.0
86.80	1456.0
87.80	1302.0
90.70	212.0
91.90	1098.0
92.80	2001.0
93.90	4393.0
94.90	37624.0
95.80	2525.0
103.70	182.0
105.70	180.0
115.80	174.0
116.70	371.0
117.90	103.0
118.80	325.0
129.70	193.0
140.70	458.0
142.70	771.0
144.80	338.0
154.60	115.0
170.70	168.0
171.70	590.0
172.80	536.0
173.80	31536.0
174.80	2234.0
175.80	30296.0
176.80	2044.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389