




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026385.D
 Acq On : 17 Jun 2022 16:36
 Operator : SY/MD
 Sample : N3318-08 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ62

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 18 00:05:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 00:00:00 2022
 Response via : Initial Calibration

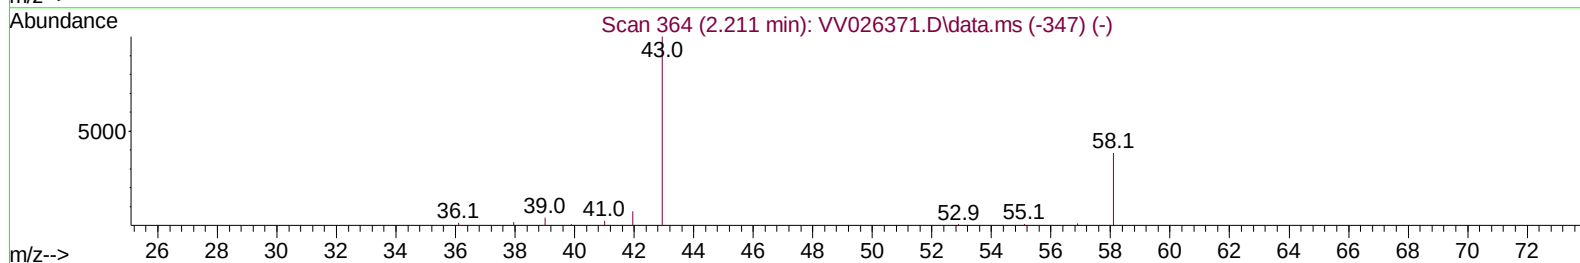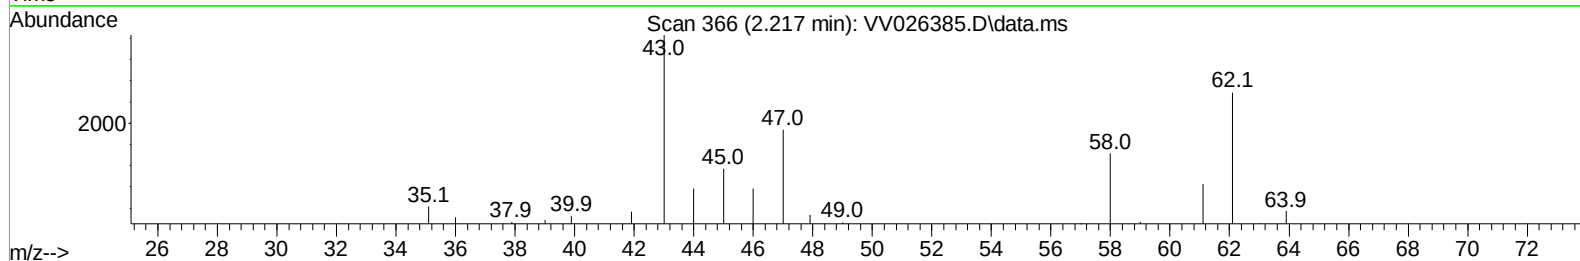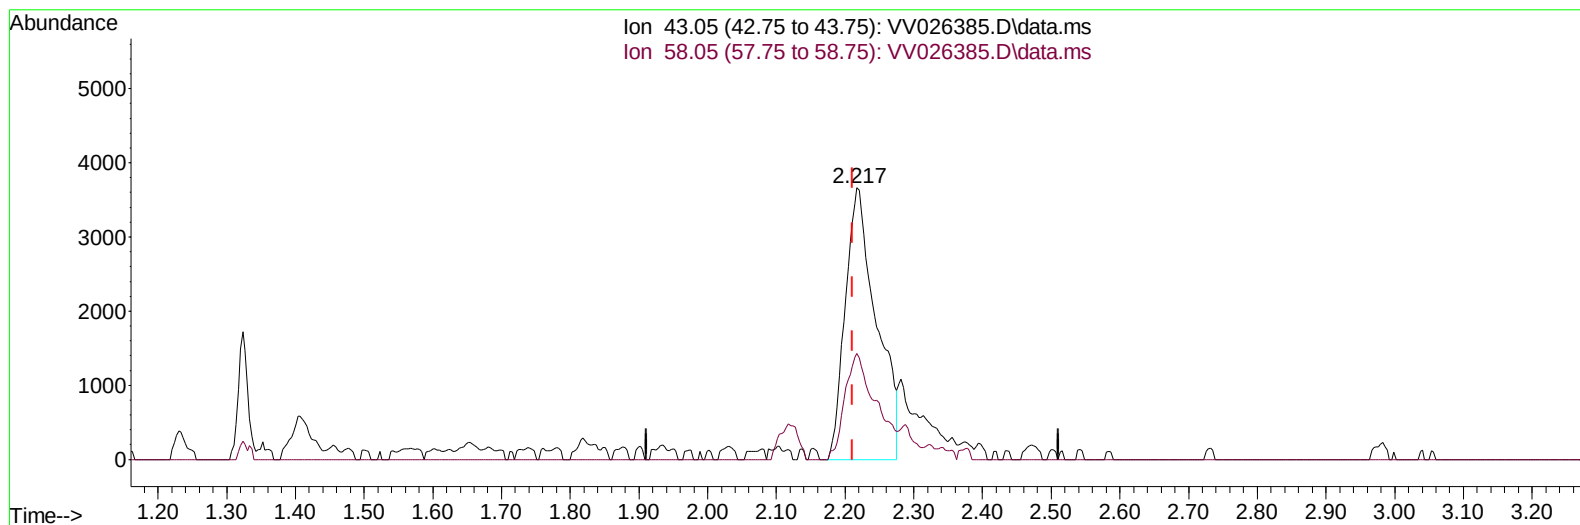

TIC: VV026385.D\data.ms

(13) Acetone (T)

2.217min (+ 0.007) 10.09 ug/L

response 11533

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	39.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026385.D
 Acq On : 17 Jun 2022 16:36
 Operator : SY/MD
 Sample : N3318-08 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ62

Manual IntegrationsAPPROVED

Quant Time: Jun 18 00:05:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 00:00:00 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

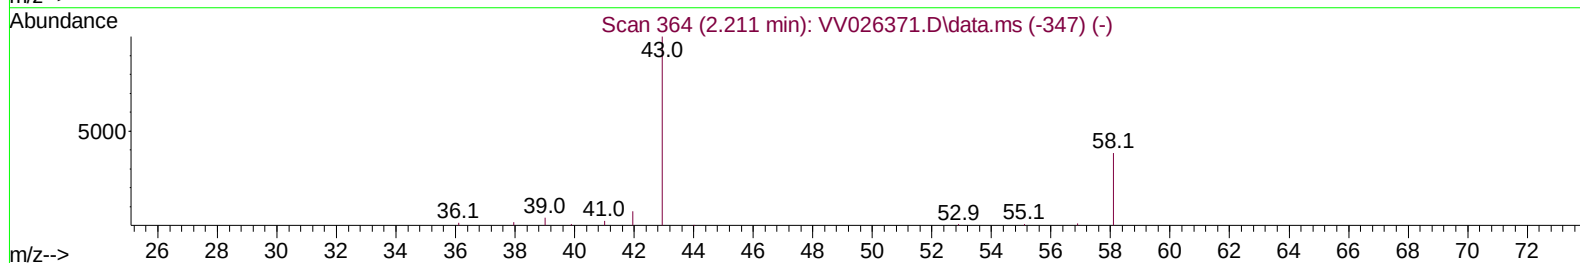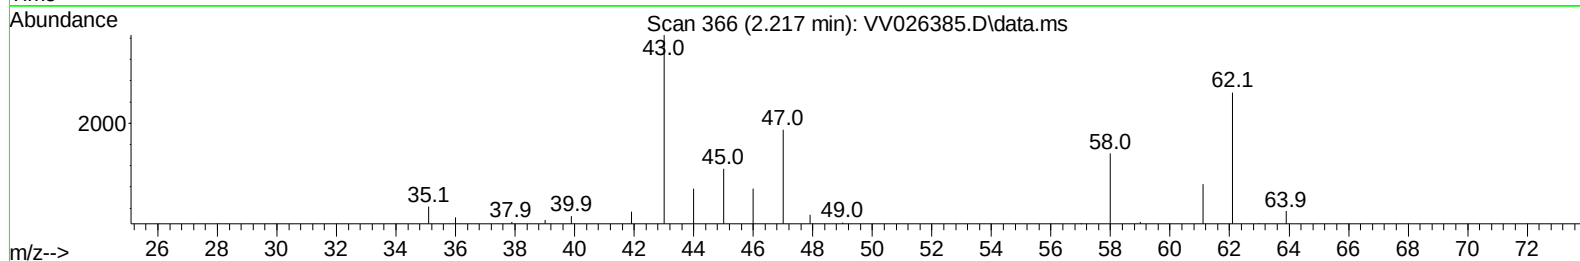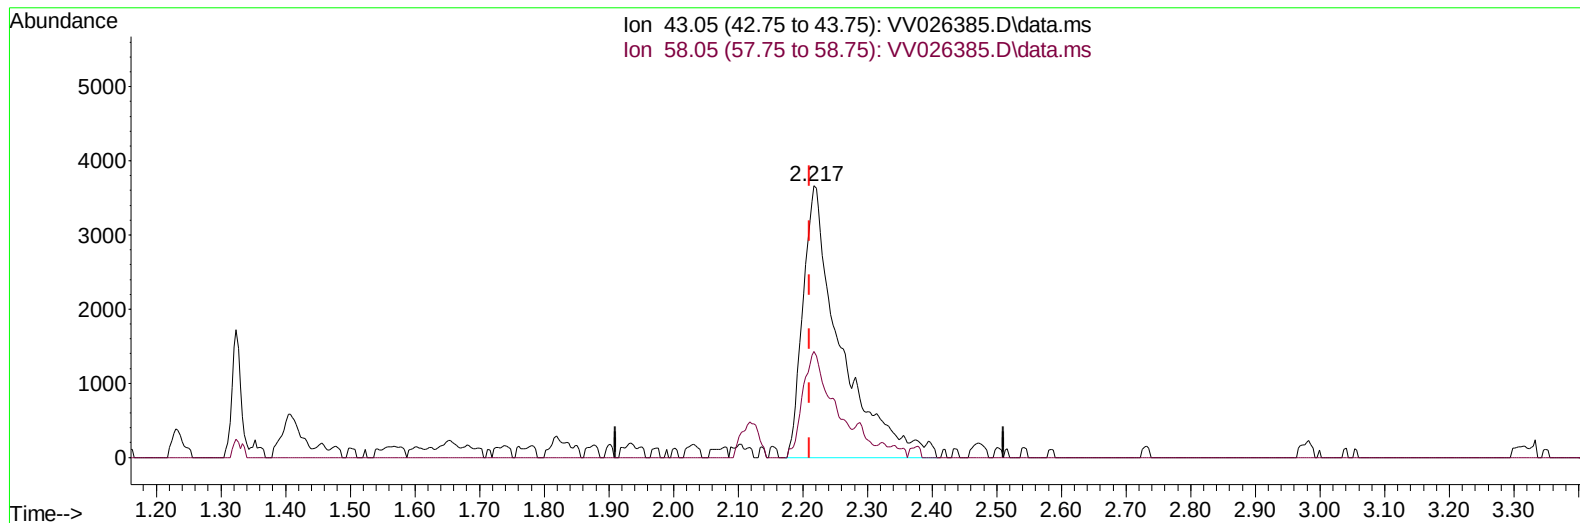

TIC: VV026385.D\data.ms

(13) Acetone (T)

2.217min (+ 0.007) 12.91 ug/L m

response 14745

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	30.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026385.D
 Acq On : 17 Jun 2022 16:36
 Operator : SY/MD
 Sample : N3318-08 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ62

Manual IntegrationsAPPROVED

Quant Time: Jun 18 00:05:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 00:00:00 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.629	114	173942	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	165662	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69240	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	55515	3.675	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	73.400%	
7) Chloroethane-d5	1.584	69	50140	4.221	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	84.400%	
11) 1,1-Dichloroethene-d2	2.124	63	81889	3.156	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.934	46	76310	51.764	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	103.520%	
24) Chloroform-d	4.368	84	107019	4.833	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.600%	
26) 1,2-Dichloroethane-d4	5.050	65	44283	4.727	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	94.600%	
32) Benzene-d6	5.063	84	193437	4.368	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	87.400%	
36) 1,2-Dichloropropane-d6	6.082	67	62136	4.807	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	96.200%	
41) Toluene-d8	7.323	98	153452	3.800	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	7.632	79	11732	2.799	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	56.000%	
46) 2-Hexanone-d5	8.095	63	54635	43.150	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	86.300%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39864	5.006	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	51559	4.834	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	96.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.217	43	14745m	12.906	ug/L	
14) Carbon disulfide	2.311	76	11807	0.436	ug/L #	92
16) Methylene chloride	2.529	84	4832	0.345	ug/L	96
18) trans-1,2-Dichloroethene	2.780	96	2681	0.252	ug/L	97
19) 1,1-Dichloroethane	3.211	63	92554	4.554	ug/L	98
22) cis-1,2-Dichloroethene	3.934	96	1154	0.107	ug/L	88
33) Benzene	5.114	78	2337	0.055	ug/L	100
47) Tetrachloroethene	7.989	164	549	0.064	ug/L	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026385.D
 Acq On : 17 Jun 2022 16:36
 Operator : SY/MD
 Sample : N3318-08 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ62

Manual IntegrationsAPPROVED

Quant Time: Jun 18 00:05:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 00:00:00 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

